



Title: Leo FCC Labelling
Project/Product Leo




1. Purpose

This document captures the FCC mandated ID, labels, warnings and notices for Leo device.


2. FCC ID

Laser etched physical label with FCC ID is to be put on each Leo device, see Fig 1.


FORMAT:

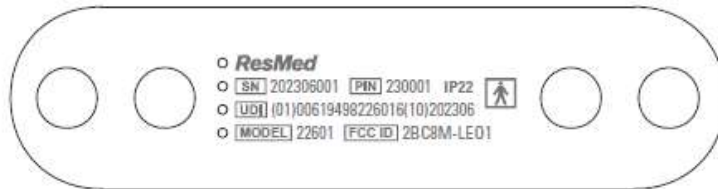

UNIVERS LT STD 57 CONDENSED FONT: 2.3MM OR 6.5PT

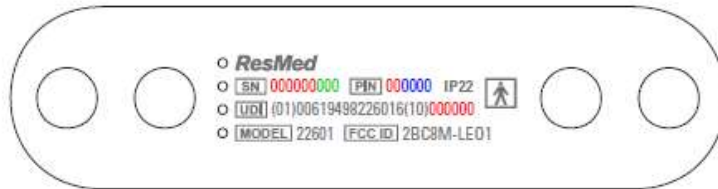

METHOD:

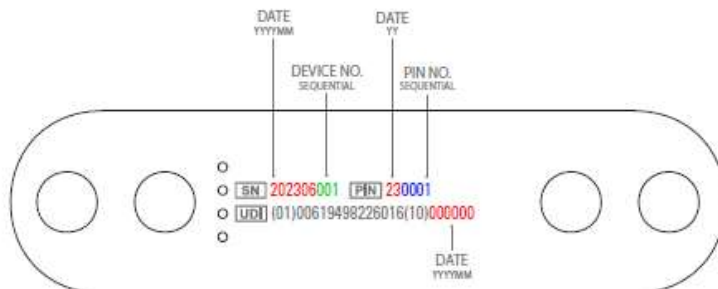

DATE IS UPDATED ONCE EVERY BATCH
 DEVICE NO. RESETS TO 001 EVERY BATCH, THEN SEQUENTIAL
 PIN NO. IS ANY 4-DIGITS, THEN SEQUENTIAL
 UDI, MODEL AND FCC ID REMAINS THE SAME AT ALL TIMES

COMPLETED
 EXAMPLE:



Figure 1. Physical FCC ID laser etched on each device

Physical printed label with FCC ID to be put on each individual Leo sensor kit's package

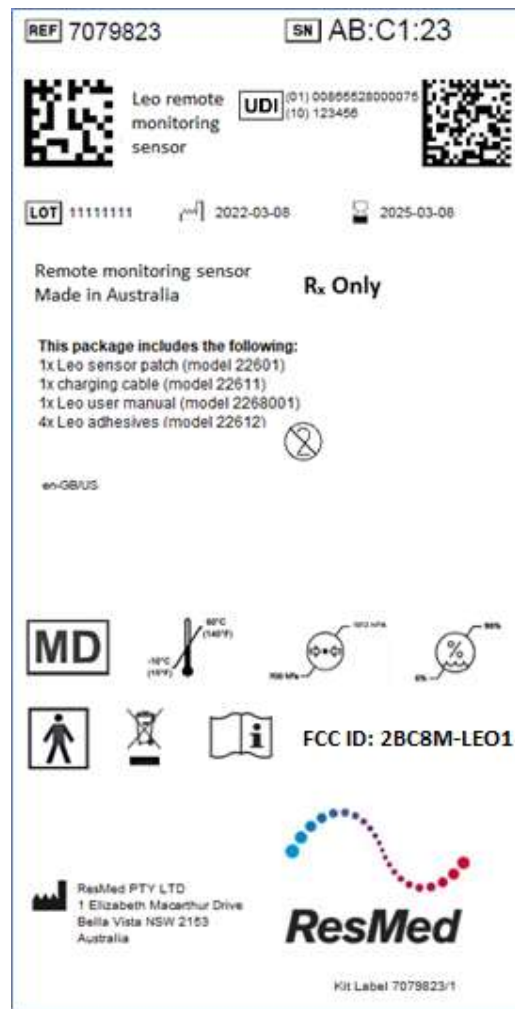


Figure 2 Printed physical package label with FCC ID

3. Labels, Warnings, Notices

FCC ID is placed on the Device as per the updated device label (Figure 1) and we also have the FCC Statement in the User Guide. The user guide will be provided in the device packaging.

47 CFR 15.105(b) requirements

Leo sensor patch is a specialized medical digital prescription-only device and therefore per 47 CFR 15.105(c) and per 47 CFR 15.103(e) provisions of 47 CFR 15.105(b) do not apply.