

## APPENDIX B: SYSTEM VERIFICATION

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 750 MHz; Type: D750V3; Serial: 1046**

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Head Medium parameters used (interpolated):

$f = 750 \text{ MHz}$ ;  $\sigma = 0.933 \text{ S/m}$ ;  $\epsilon_r = 41.499$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.5 cm

Test Date: 02-07-2014; Ambient Temp: 24.5°C; Tissue Temp: 23.8°C

Probe: ES3DV3 - SN3319; ConvF(6.49, 6.49, 6.49); Calibrated: 4/29/2013;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1368; Calibrated: 4/22/2013

Phantom: SAM front; Type: QD000P40CD; Serial: TP:1759

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 750 MHz System Verification

**Area Scan (7x15x1):** Measurement grid:  $dx=15\text{mm}$ ,  $dy=15\text{mm}$


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=8\text{mm}$ ,  $dy=8\text{mm}$ ,  $dz=5\text{mm}$

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 1.19 W/kg

**SAR(1 g) = 0.813 W/kg**

Deviation = -4.35%

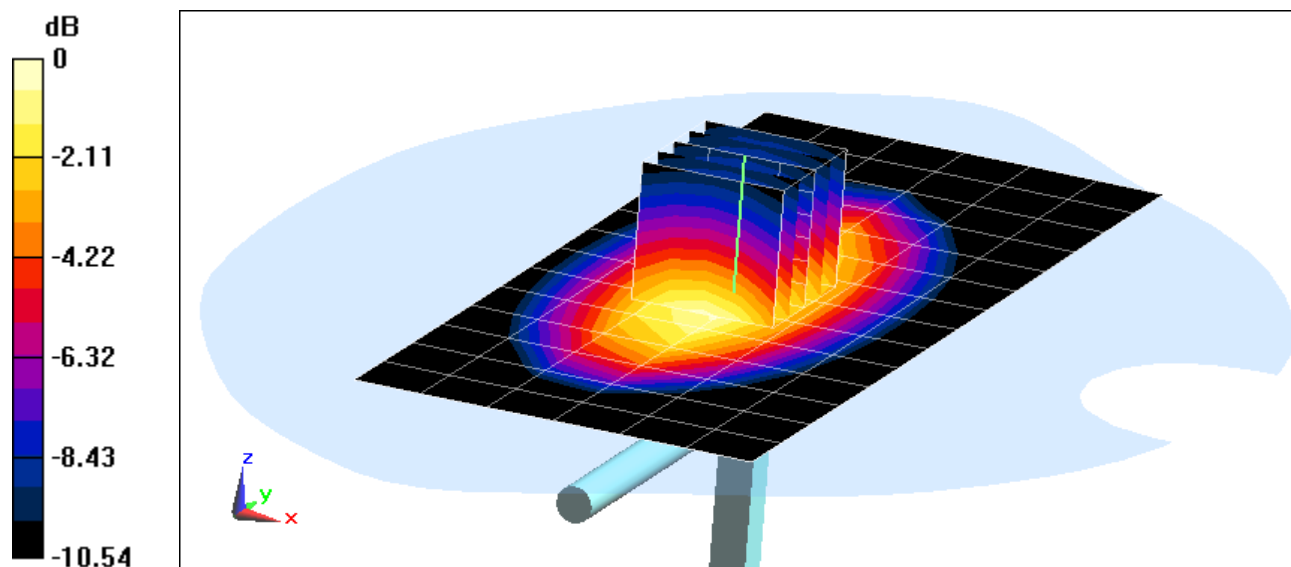

0 dB = 0.882 W/kg = -0.55 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d119**

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 835 \text{ MHz}$ ;  $\sigma = 0.892 \text{ S/m}$ ;  $\epsilon_r = 40.4$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.5 cm

Test Date: 02-07-2014; Ambient Temp: 24.6°C; Tissue Temp: 24.1°C

Probe: EX3DV4 - SN3589; ConvF(8.49, 8.49, 8.49); Calibrated: 1/29/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1272; Calibrated: 1/22/2014

Phantom: SAM; Type: QD000P40CD; Serial: TP:1758

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 835 MHz System Verification

**Area Scan (7x14x1):** Measurement grid:  $dx=15\text{mm}$ ,  $dy=15\text{mm}$


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=8\text{mm}$ ,  $dy=8\text{mm}$ ,  $dz=5\text{mm}$

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 1.41 W/kg

**SAR(1 g) = 0.941 W/kg**

Deviation = -2.79%

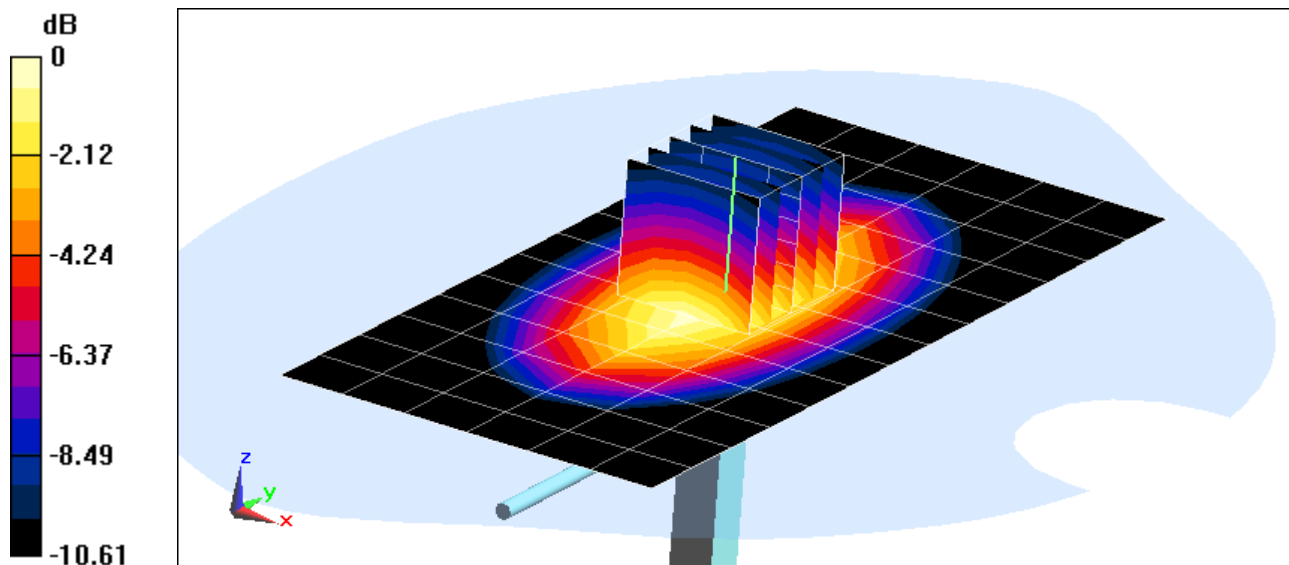

0 dB = 1.02 W/kg = 0.09 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 1765 MHz; Type: D1765V2; Serial: 1008**

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Head Medium parameters used:

$f = 1750 \text{ MHz}$ ;  $\sigma = 1.42 \text{ S/m}$ ;  $\epsilon_r = 38.996$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-10-2014; Ambient Temp: 23.6°C; Tissue Temp: 23.0°C

Probe: ES3DV3 - SN3288; ConvF(5.67, 5.67, 5.67); Calibrated: 9/23/2013;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 9/17/2013

Phantom: SAM Sub Dasy B; Type: SAM 5.0; Serial: TP-1626

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.10 (7164)

## 1750 MHz System Verification

**Area Scan (6x8x1):** Measurement grid: dx=15mm, dy=15mm


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 6.45 W/kg

**SAR(1 g) = 3.48 W/kg**

Deviation = -5.43%

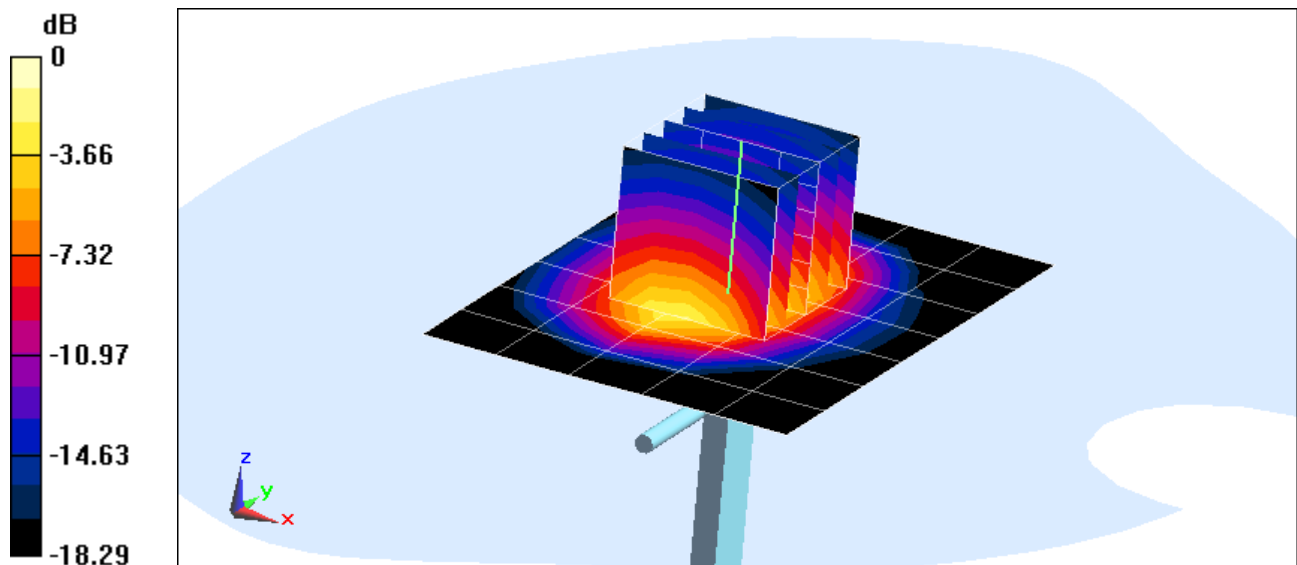

0 dB = 3.82 W/kg = 5.82 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 1900 MHz; Type: D1900V2; Serial: 5d141**

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Head Medium parameters used (interpolated):

$f = 1900 \text{ MHz}$ ;  $\sigma = 1.405 \text{ S/m}$ ;  $\epsilon_r = 38.228$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-10-2014; Ambient Temp: 23.5°C; Tissue Temp: 22.8°C

Probe: ES3DV3 - SN3288; ConvF(5.47, 5.47, 5.47); Calibrated: 9/23/2013;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 9/17/2013

Phantom: SAM with CRP; Type: SAM; Serial: TP1375

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.10 (7164)

## 1900MHz System Verification

**Area Scan (5x7x1):** Measurement grid: dx=15mm, dy=15mm


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 7.65 W/kg

**SAR(1 g) = 4.07 W/kg**

Deviation = -0.25%

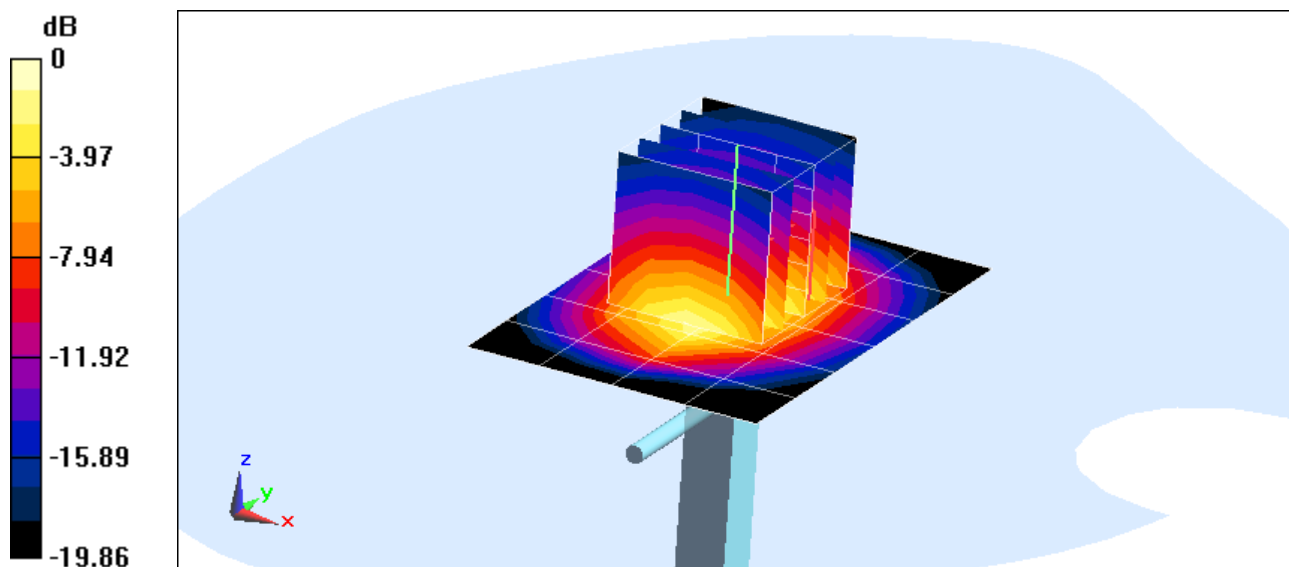

0 dB = 4.49 W/kg = 6.52 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 719**

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: 2450 Head Medium parameters used:

$f = 2450 \text{ MHz}$ ;  $\sigma = 1.84 \text{ S/m}$ ;  $\epsilon_r = 40.077$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-14-2014; Ambient Temp: 23.9°C; Tissue Temp: 23.2°C

Probe: ES3DV3 - SN3287; ConvF(4.43, 4.43, 4.43); Calibrated: 11/20/2013;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1408; Calibrated: 11/19/2013

Phantom: SAM with CRP v4.0; Type: QD000P40CD; Serial: TP:1797

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 2450 MHz System Verification

**Area Scan (8x9x1):** Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 11.1 W/kg

**SAR(1 g) = 5.42 W/kg**

Deviation = 1.88%

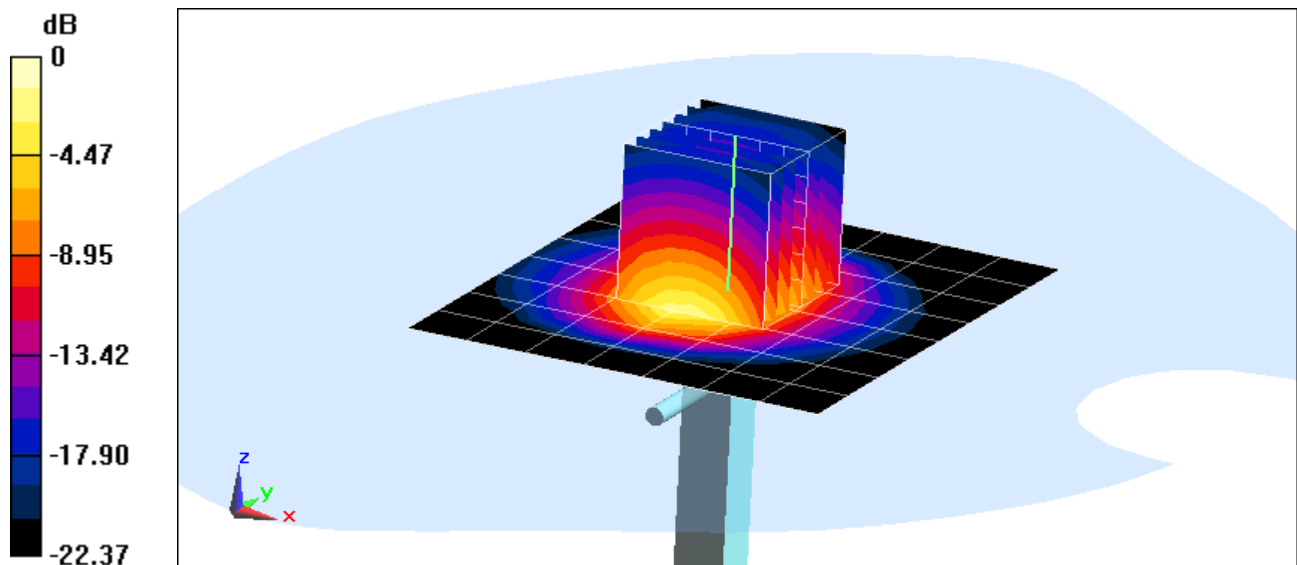

0 dB = 7.04 W/kg = 8.48 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 5200 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: 5 GHz Head; Medium parameters used:

$f = 5200 \text{ MHz}$ ;  $\sigma = 4.566 \text{ S/m}$ ;  $\epsilon_r = 37.509$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-06-2014; Ambient Temp: 24.5°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN3914; ConvF(4.99, 4.99, 4.99); Calibrated: 10/23/2013;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM V5.0 Right; Type: QD000P40CD; Serial: 1647

Measurement SW: DASY52, Version 52.8 (7);SEMCAD X Version 14.6.10 (7164)

## 5200 MHz System Verification

**Area Scan (7x8x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=4\text{mm}$ ,  $dy=4\text{mm}$ ,  $dz=1.4\text{mm}$ ; Graded Ratio: 1.4

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 32.8 W/kg

**SAR(1 g) = 7.84 W/kg**

Deviation = 3.16%

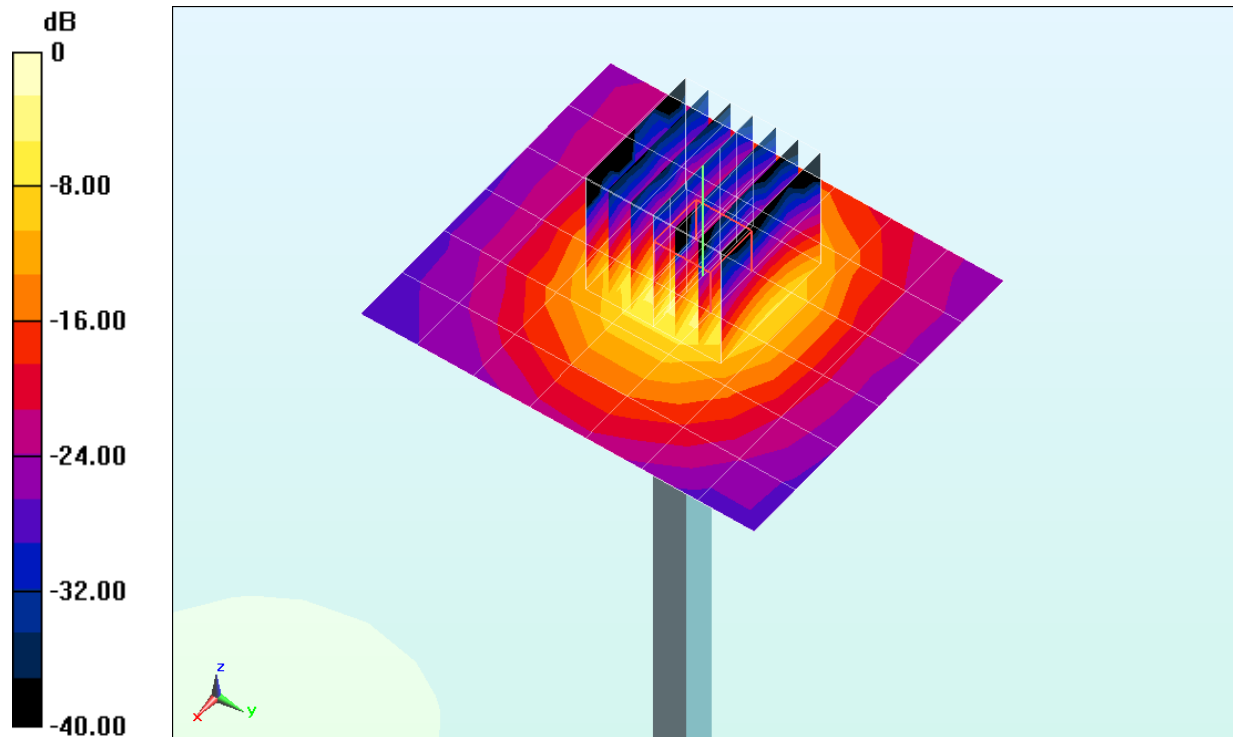

0 dB = 19.8 W/kg = 12.97 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 5300 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5300 MHz; Duty Cycle: 1:1

Medium: 5 GHz Head; Medium parameters used:

$f = 5300 \text{ MHz}$ ;  $\sigma = 4.651 \text{ S/m}$ ;  $\epsilon_r = 37.509$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-06-2014; Ambient Temp: 24.1°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN3914; ConvF(4.82, 4.82, 4.82); Calibrated: 10/23/2013;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM V5.0 Right; Type: QD000P40CD; Serial: 1647

Measurement SW: DASY52, Version 52.8 (7);SEMCAD X Version 14.6.10 (7164)

## 5300 MHz System Verification

**Area Scan (7x8x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=4\text{mm}$ ,  $dy=4\text{mm}$ ,  $dz=1.4\text{mm}$ ; Graded Ratio: 1.4

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 34.5 W/kg

**SAR(1 g) = 7.96 W/kg**

Deviation = 1.14%

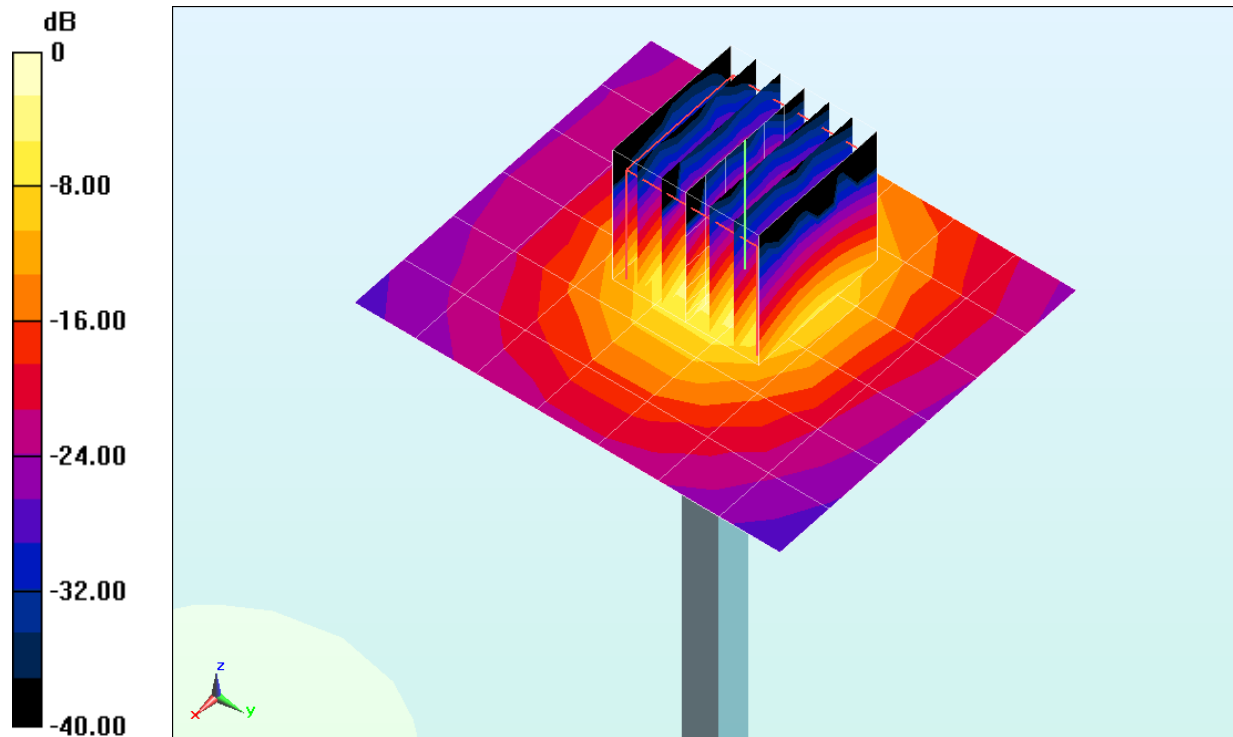



# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 5500 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5500 MHz; Duty Cycle: 1:1

Medium: 5 GHz Head; Medium parameters used:

$f = 5500 \text{ MHz}$ ;  $\sigma = 4.925 \text{ S/m}$ ;  $\epsilon_r = 37.305$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-06-2014; Ambient Temp: 23.9°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN3914; ConvF(4.55, 4.55, 4.55); Calibrated: 10/23/2013;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM V5.0 Right; Type: QD000P40CD; Serial: 1647

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 5500 MHz System Verification

**Area Scan (7x8x1):** Measurement grid: dx=10mm, dy=10mm


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 34.0 W/kg

**SAR(1 g) = 7.91 W/kg**

Deviation = -1.25%

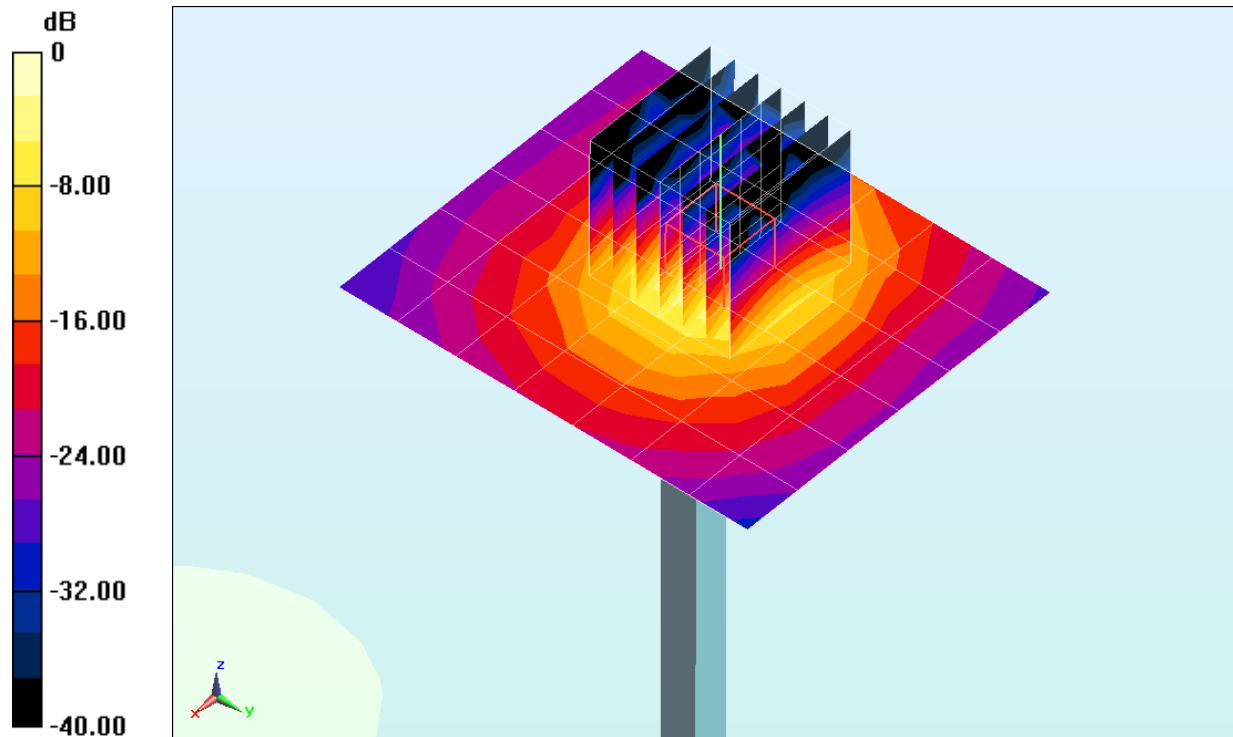

0 dB = 20.3 W/kg = 13.07 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 5500 MHz; Type: D5GHzV2; Serial: 1057**

Communication System: UID 0, CW; Frequency: 5500 MHz; Duty Cycle: 1:1

Medium: 5 GHz Head Medium parameters used:

$f = 5500 \text{ MHz}$ ;  $\sigma = 4.912 \text{ S/m}$ ;  $\epsilon_r = 36.692$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-17-2014; Ambient Temp: 24.3°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN3914; ConvF(4.55, 4.55, 4.55); Calibrated: 10/23/2013;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM V5.0 Right; Type: QD000P40CD; Serial: 1647

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 5500 MHz System Verification

**Area Scan (7x8x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=4\text{mm}$ ,  $dy=4\text{mm}$ ,  $dz=1.4\text{mm}$ ; Graded Ratio: 1.4

Input Power = 16.0 dBm (40 mW)

Peak SAR (extrapolated) = 14.1 W/kg

**SAR(1 g) = 3.16 W/kg**

Deviation = -6.29%

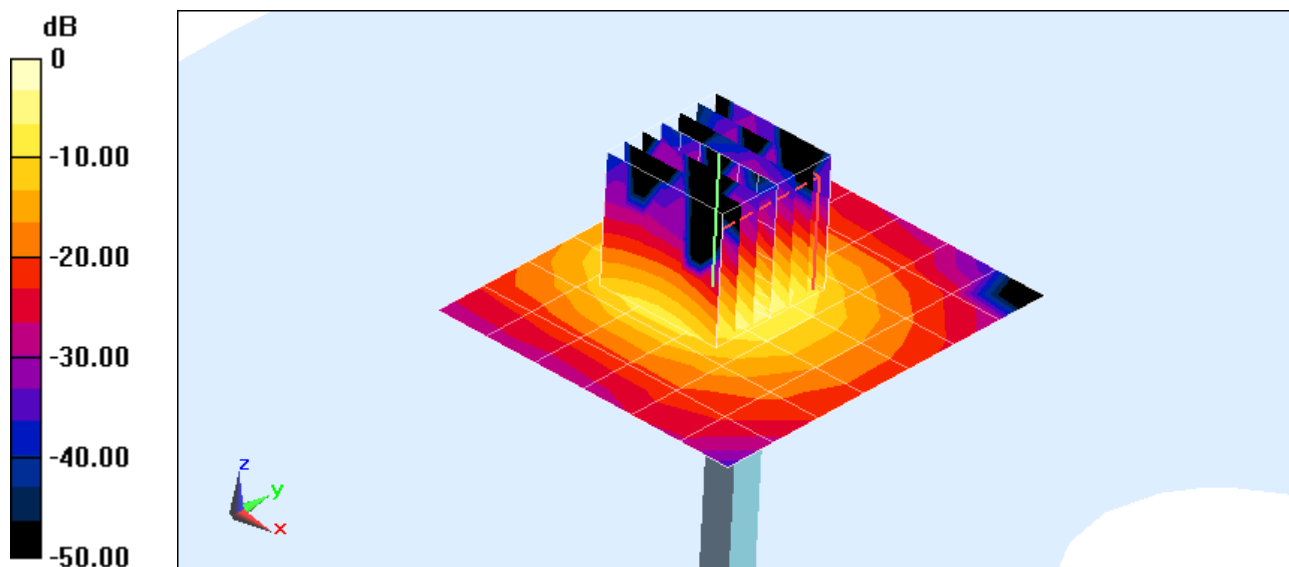

0 dB = 8.16 W/kg = 9.12 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 5600 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5600 MHz; Duty Cycle: 1:1

Medium: 5 GHz Head; Medium parameters used:

$f = 5600 \text{ MHz}$ ;  $\sigma = 5.017 \text{ S/m}$ ;  $\epsilon_r = 37.024$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-06-2014; Ambient Temp: 24.0°C; Tissue Temp: 23.4°C

Probe: EX3DV4 - SN3914; ConvF(4.37, 4.37, 4.37); Calibrated: 10/23/2013;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM V5.0 Right; Type: QD000P40CD; Serial: 1647

Measurement SW: DASY52, Version 52.8 (7);SEMCAD X Version 14.6.10 (7164)

## 5600 MHz System Verification

**Area Scan (7x8x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=4\text{mm}$ ,  $dy=4\text{mm}$ ,  $dz=1.4\text{mm}$ ; Graded Ratio: 1.4

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 36.1 W/kg

**SAR(1 g) = 7.97 W/kg**

Deviation = -0.25%

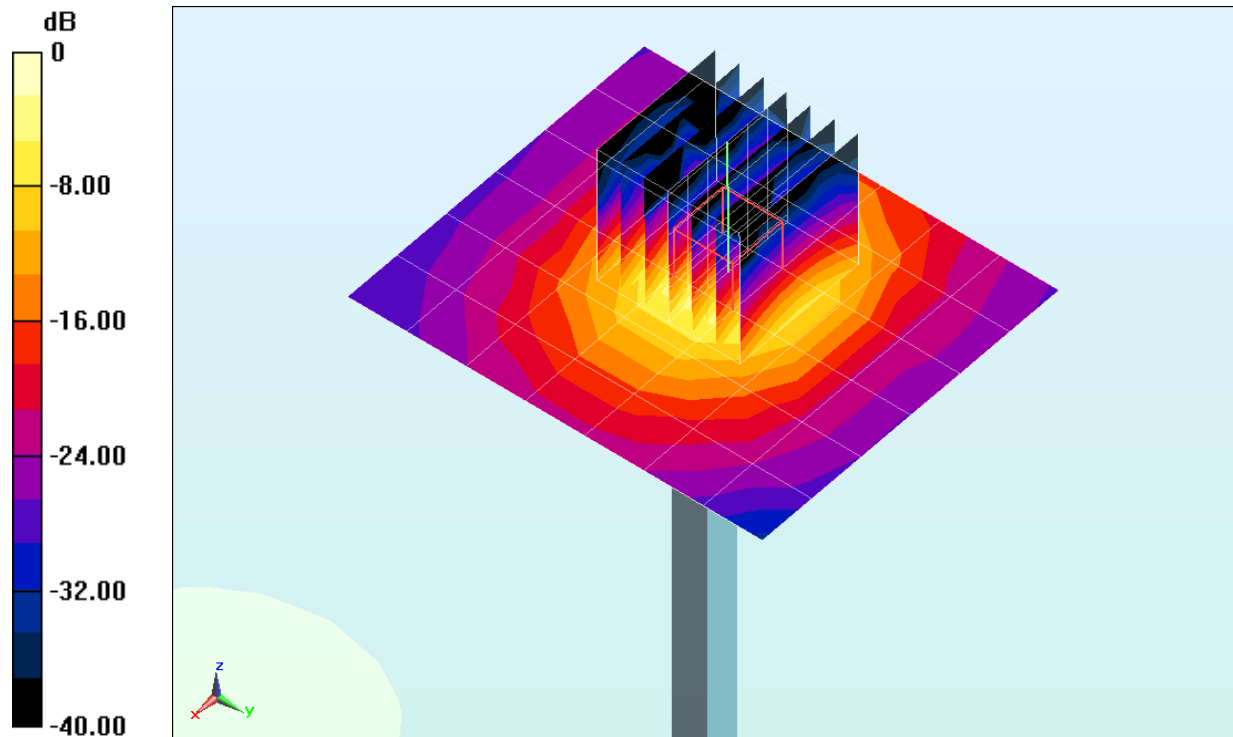

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 5800 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: 5 GHz Head; Medium parameters used:

$f = 5800 \text{ MHz}$ ;  $\sigma = 5.176 \text{ S/m}$ ;  $\epsilon_r = 36.885$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-06-2014; Ambient Temp: 24.1°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN3914; ConvF(4.52, 4.52, 4.52); Calibrated: 10/23/2013;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM V5.0 Right; Type: QD000P40CD; Serial: 1647

Measurement SW: DASY52, Version 52.8 (7);SEMCAD X Version 14.6.10 (7164)

## 5800 MHz System Verification

**Area Scan (7x8x1):** Measurement grid: dx=10mm, dy=10mm


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 34.8 W/kg

**SAR(1 g) = 7.4 W/kg**

Deviation = -1.20%

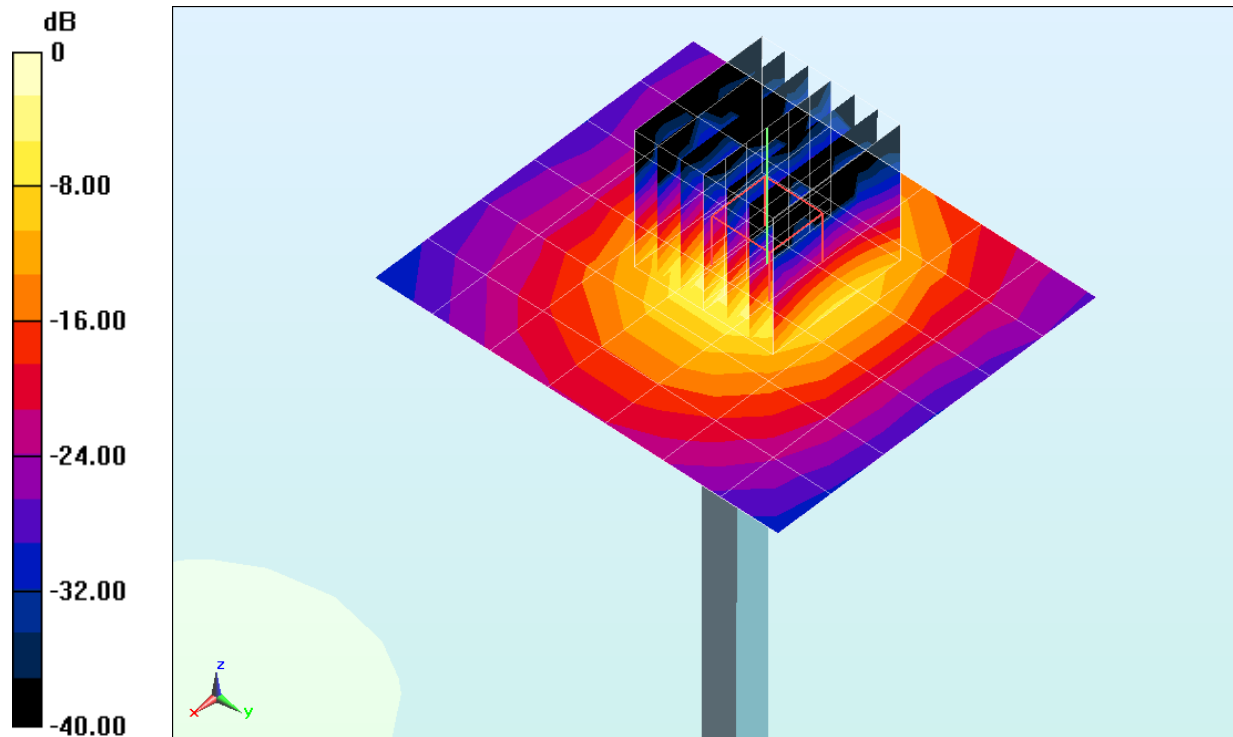

0 dB = 19.5 W/kg = 12.90 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 750 MHz; Type: D750V3; Serial: 1054**

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used (interpolated):

$f = 750 \text{ MHz}$ ;  $\sigma = 0.98 \text{ S/m}$ ;  $\epsilon_r = 55.68$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.5 cm

Test Date: 02-11-2014; Ambient Temp: 22.3°C; Tissue Temp: 21.1°C

Probe: ES3DV3 - SN3263; ConvF(6.37, 6.37, 6.37); Calibrated: 5/16/2013;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn859; Calibrated: 5/13/2013

Phantom: SAM Main; Type: SAM 4.0; Serial: TP-1114

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.10 (7164)

## 750MHz System Verification

**Area Scan (7x13x1):** Measurement grid:  $dx=15\text{mm}$ ,  $dy=15\text{mm}$


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=8\text{mm}$ ,  $dy=8\text{mm}$ ,  $dz=5\text{mm}$

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 1.26 W/kg

**SAR(1 g) = 0.880 W/kg**

Deviation = 0.92%

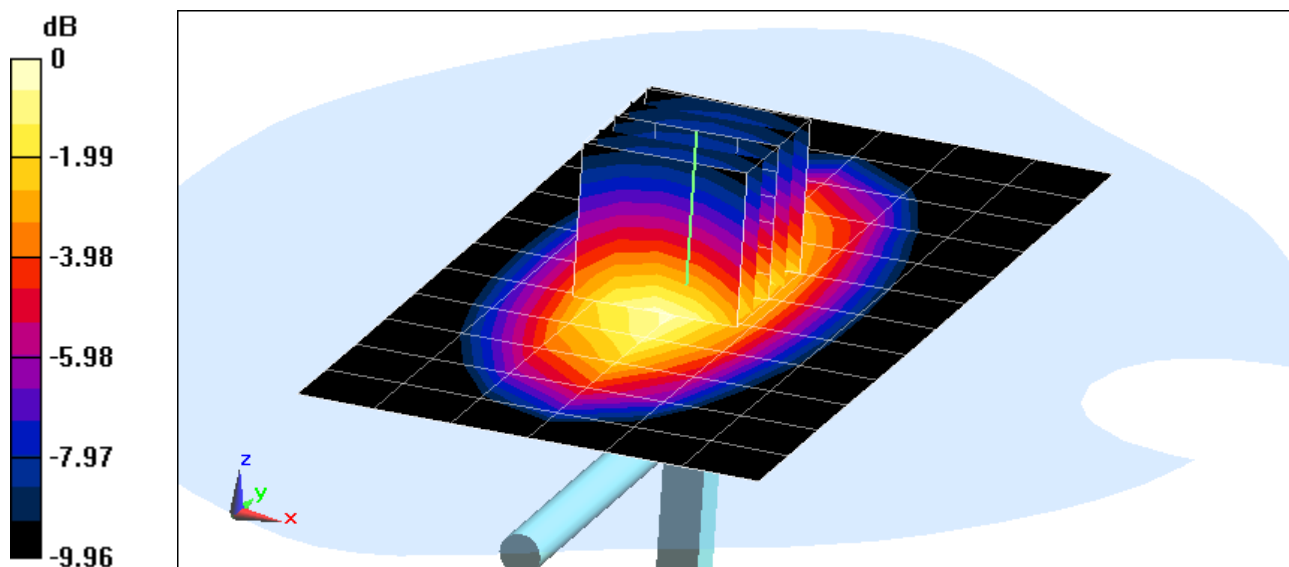

0 dB = 0.956 W/kg = -0.20 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d133**

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$ ;  $\sigma = 0.954 \text{ S/m}$ ;  $\epsilon_r = 54.628$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.5 cm

Test Date: 02-10-2014; Ambient Temp: 23.4°C; Tissue Temp: 20.1°C

Probe: ES3DV3 - SN3263; ConvF(6.29, 6.29, 6.29); Calibrated: 5/16/2013;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn859; Calibrated: 5/13/2013

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.10 (7164)

## 835MHz System Verification

**Area Scan (7x13x1):** Measurement grid:  $dx=15\text{mm}$ ,  $dy=15\text{mm}$


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=8\text{mm}$ ,  $dy=8\text{mm}$ ,  $dz=5\text{mm}$

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 1.39 W/kg

**SAR(1 g) = 0.956 W/kg**

Deviation = -0.52%

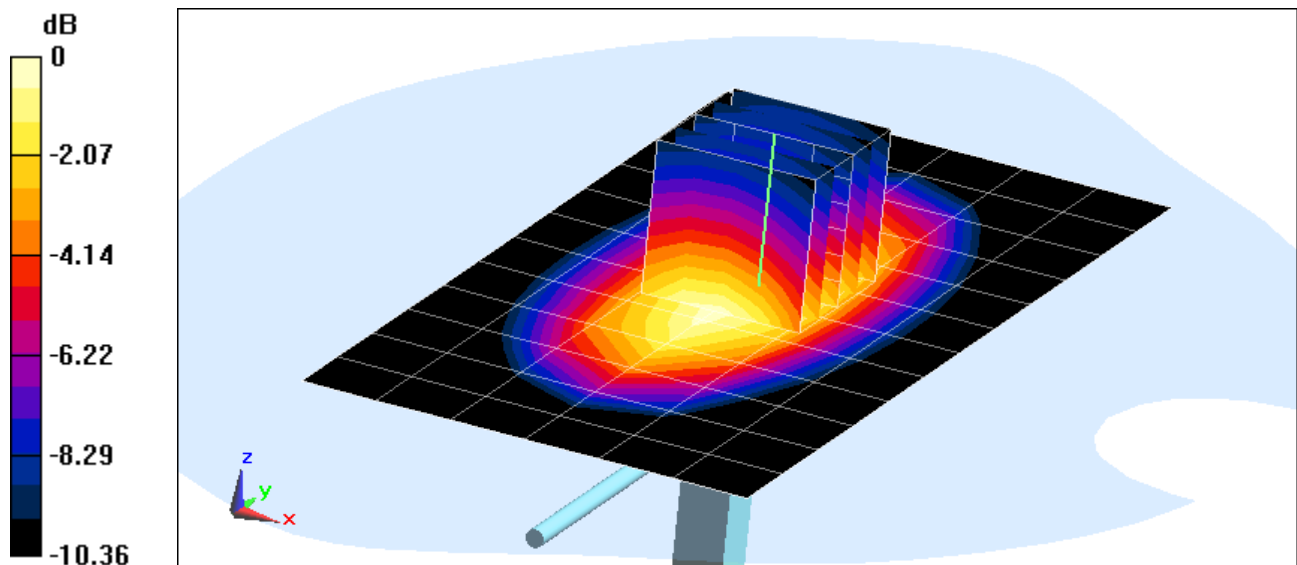

0 dB = 1.02 W/kg = 0.09 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 1765 MHz; Type: D1765V2; Serial: 1008**

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$ ;  $\sigma = 1.476 \text{ S/m}$ ;  $\epsilon_r = 51.932$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-10-2014; Ambient Temp: 23.6°C; Tissue Temp: 22.9°C

Probe: ES3DV3 - SN3288; ConvF(5.1, 5.1, 5.1); Calibrated: 9/23/2013;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 9/17/2013

Phantom: SAM with CRP; Type: SAM; Serial: TP1375

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.10 (7164)

## 1750 MHz System Verification

**Area Scan (6x8x1):** Measurement grid: dx=15mm, dy=15mm


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 6.73 W/kg

**SAR(1 g) = 3.69 W/kg**

Deviation = -3.40%

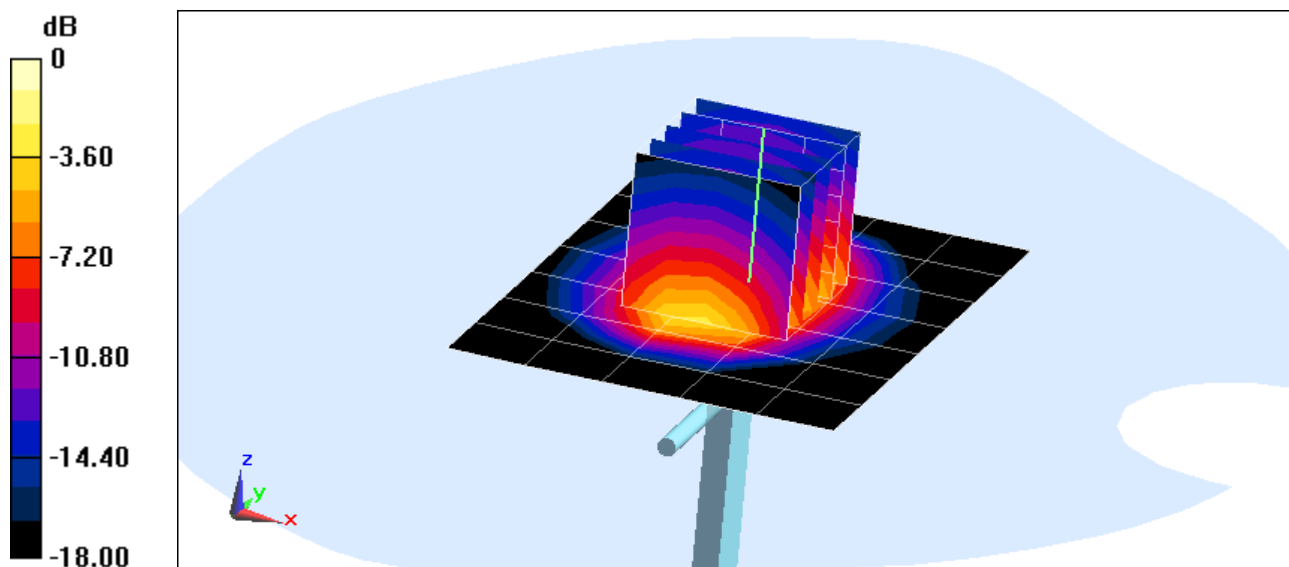

0 dB = 4.01 W/kg = 6.03 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: SAR Dipole 1900 MHz; Type: D1900V2; Serial: 5d149**

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900 \text{ MHz}$ ;  $\sigma = 1.546 \text{ S/m}$ ;  $\epsilon_r = 52.267$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-10-2014; Ambient Temp: 24.4°C; Tissue Temp: 23.6°C

Probe: ES3DV3 - SN3319; ConvF(4.85, 4.85, 4.85); Calibrated: 4/29/2013;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1368; Calibrated: 4/22/2013

Phantom: SAM front; Type: QD000P40CD; Serial: TP:1759

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 1900 MHz System Verification

**Area Scan (7x10x1):** Measurement grid:  $dx=15\text{mm}$ ,  $dy=15\text{mm}$


**Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=8\text{mm}$ ,  $dy=8\text{mm}$ ,  $dz=5\text{mm}$

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 6.81 W/kg

**SAR(1 g) = 3.82 W/kg**

Deviation = -5.68%

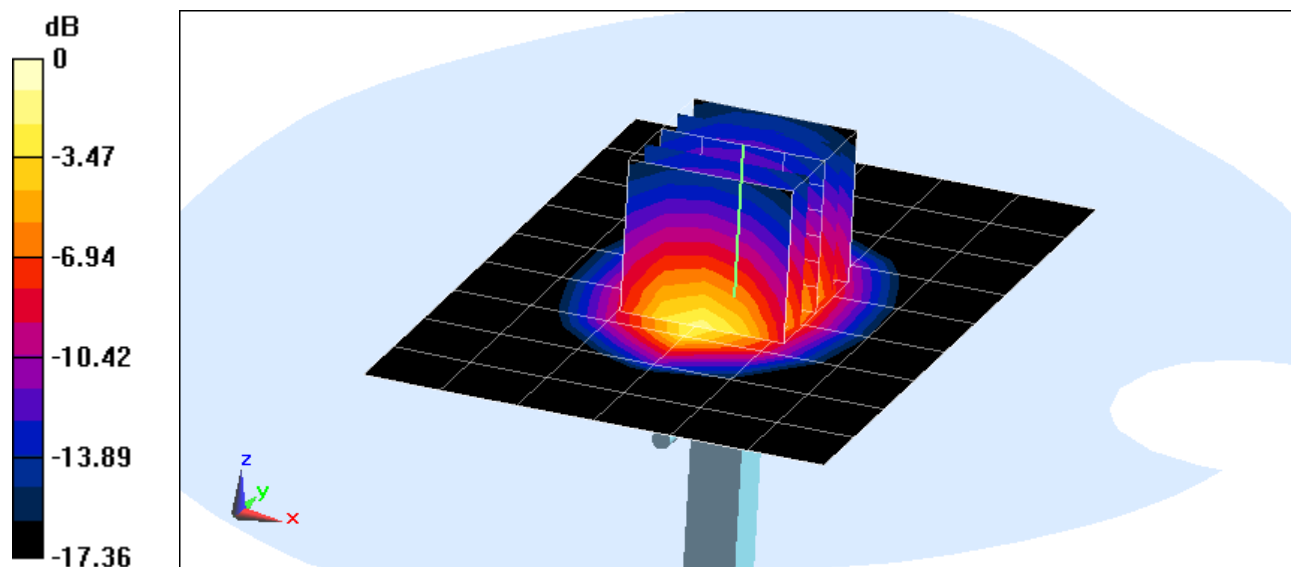

0 dB = 4.31 W/kg = 6.34 dBW/kg



# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 719**

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: 2450 Body Medium parameters used:

$f = 2450 \text{ MHz}$ ;  $\sigma = 1.937 \text{ S/m}$ ;  $\epsilon_r = 51.331$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section, Space = 1.0 cm

Test Date: 02-12-2014; Ambient Temp: 24.6°C; Tissue Temp: 24.0°C

Probe: ES3DV3 - SN3318; ConvF(4.31, 4.31, 4.31); Calibrated: 4/29/2013;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1364; Calibrated: 4/22/2013

Phantom: ELI left; Type: QDOVA002AA; Serial: TP:1202

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 2450 MHz System Verification

**Area Scan (8x9x1):** Measurement grid:  $dx=12\text{mm}$ ,  $dy=12\text{mm}$


**Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 11.1 W/kg

**SAR(1 g) = 5.41 W/kg**

Deviation = 4.64%

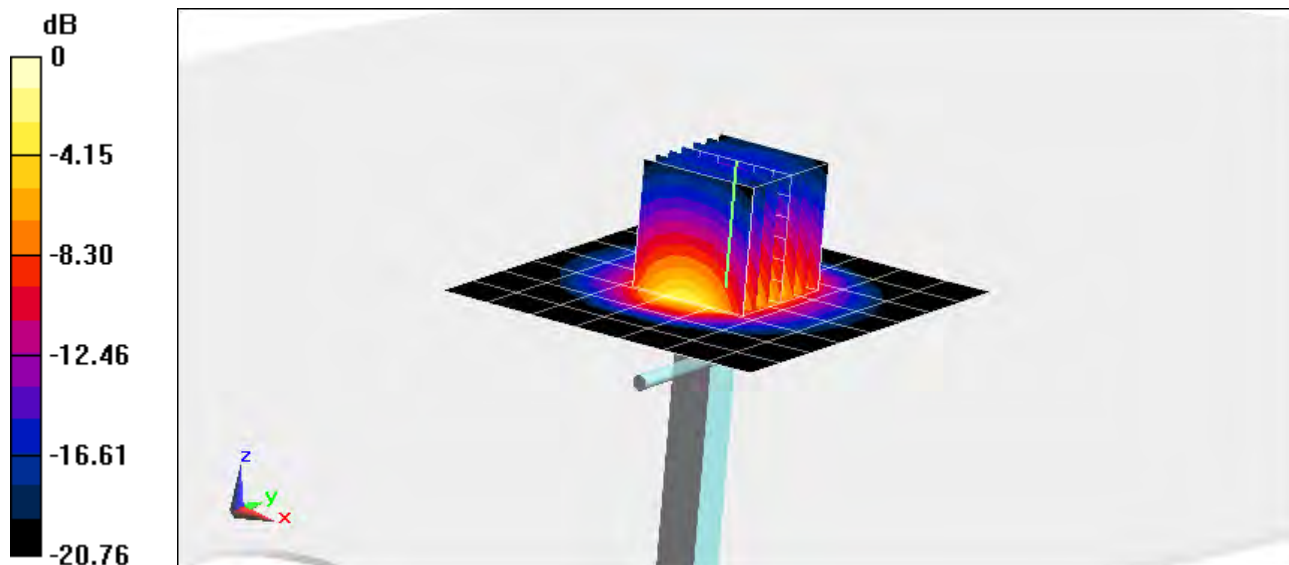

0 dB = 7.09 W/kg = 8.51 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 5200 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5200 MHz; Duty Cycle: 1:1  
Medium: 5 GHz Body, Medium parameters used:

$f = 5200 \text{ MHz}$ ;  $\sigma = 5.168 \text{ S/m}$ ;  $\epsilon_r = 47.598$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-03-2014; Ambient Temp: 24.5°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN3914; ConvF(4.52, 4.52, 4.52); Calibrated: 10/23/2013;  
Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 5200 MHz System Verification


**Area Scan (7x8x1):** Measurement grid: dx=10mm, dy=10mm

**Zoom Scan (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4  
Input Power = 16.0 dBm (40 mW)

Peak SAR (extrapolated) = 13.2 W/kg

**SAR(1 g) = 3.11 W/kg**

Deviation = 1.50%

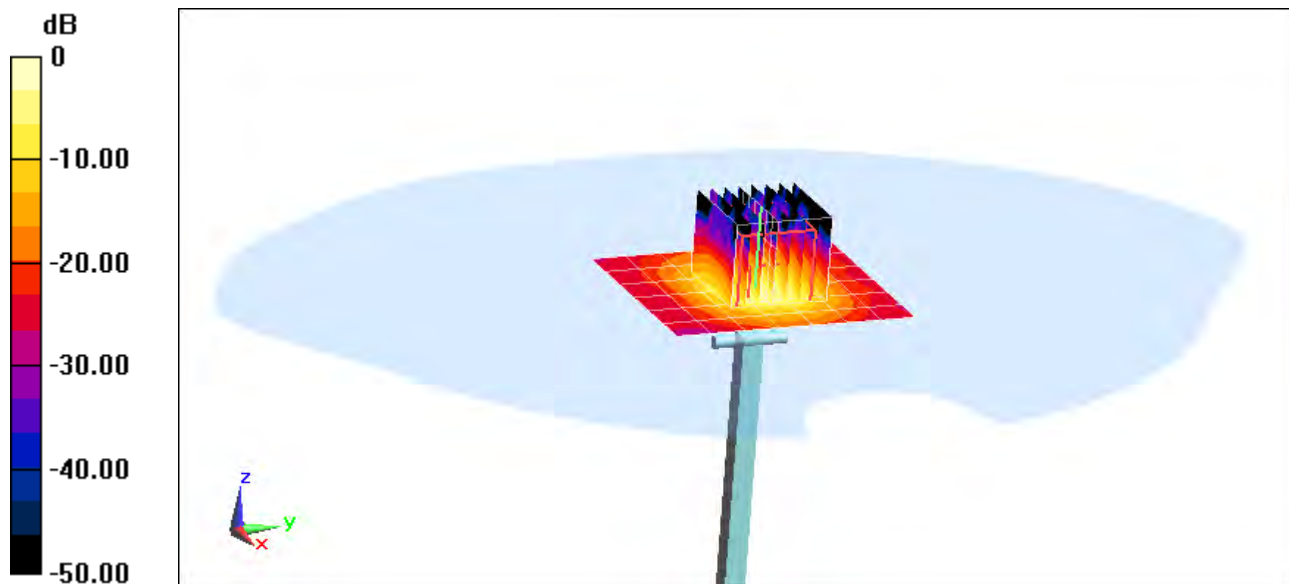

0 dB = 7.88 W/kg = 8.97 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 5300 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5300 MHz; Duty Cycle: 1:1  
Medium: 5 GHz Body, Medium parameters used:

$f = 5300 \text{ MHz}$ ;  $\sigma = 5.352 \text{ S/m}$ ;  $\epsilon_r = 47.314$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-03-2014; Ambient Temp: 24.4°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN3914; ConvF(4.32, 4.32, 4.32); Calibrated: 10/23/2013;  
Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 5300 MHz System Verification


**Area Scan (7x8x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

**Zoom Scan (9x9x7)/Cube 0:** Measurement grid:  $dx=4\text{mm}$ ,  $dy=4\text{mm}$ ,  $dz=1.4\text{mm}$ ; Graded Ratio: 1.4  
Input Power = 16.0 dBm (40 mW)

Peak SAR (extrapolated) = 14.4 W/kg

**SAR(1 g) = 3.26 W/kg**

Deviation = 6.12%

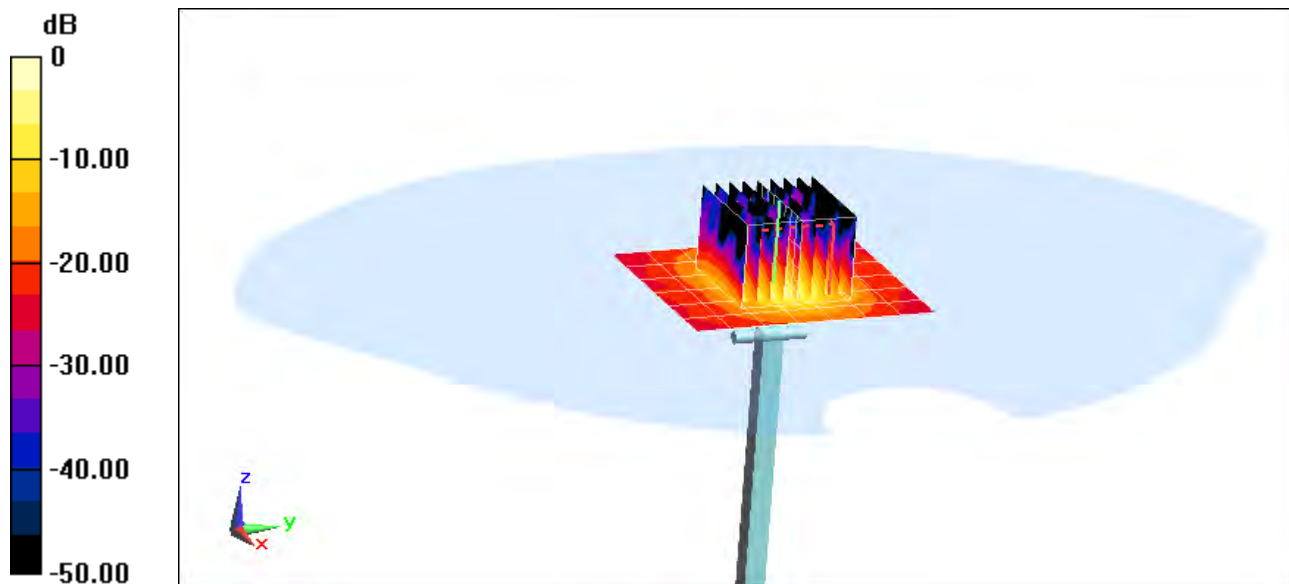

0 dB = 8.34 W/kg = 9.21 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 5500 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5500 MHz; Duty Cycle: 1:1  
Medium: 5 GHz Body, Medium parameters used:

$f = 5500 \text{ MHz}$ ;  $\sigma = 5.579 \text{ S/m}$ ;  $\epsilon_r = 46.639$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-03-2014; Ambient Temp: 24.3°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN3914; ConvF(4.07, 4.07, 4.07); Calibrated: 10/23/2013;  
Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 5500 MHz System Verification


**Area Scan (7x8x1):** Measurement grid: dx=10mm, dy=10mm

**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4  
Input Power = 16.0 dBm (40 mW)

Peak SAR (extrapolated) = 15.3 W/kg

**SAR(1 g) = 3.27 W/kg**

Deviation = 2.44%

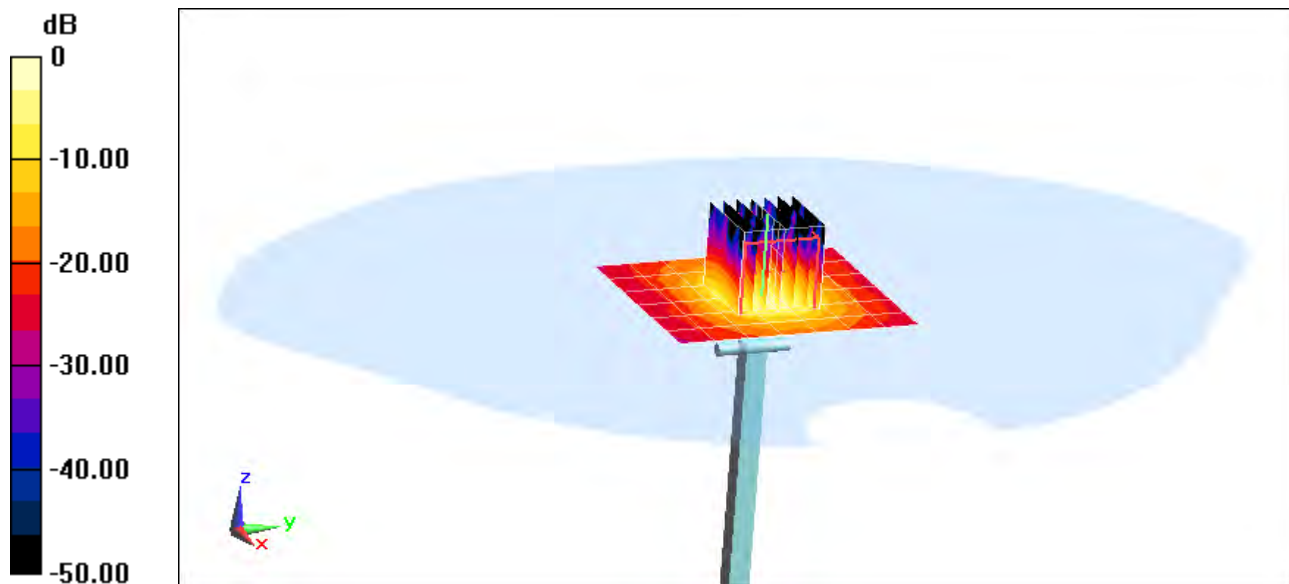

0 dB = 8.61 W/kg = 9.35 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 5600 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5600 MHz; Duty Cycle: 1:1  
Medium: 5 GHz Body, Medium parameters used:

$f = 5600 \text{ MHz}$ ;  $\sigma = 5.749 \text{ S/m}$ ;  $\epsilon_r = 46.646$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-03-2014; Ambient Temp: 24.5°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN3914; ConvF(3.97, 3.97, 3.97); Calibrated: 10/23/2013;  
Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 5600 MHz System Verification


**Area Scan (7x8x1):** Measurement grid: dx=10mm, dy=10mm

**Zoom Scan (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4  
Input Power = 16.0 dBm (40 mW)

Peak SAR (extrapolated) = 16.2 W/kg

**SAR(1 g) = 3.38 W/kg**

Deviation = 4.71%

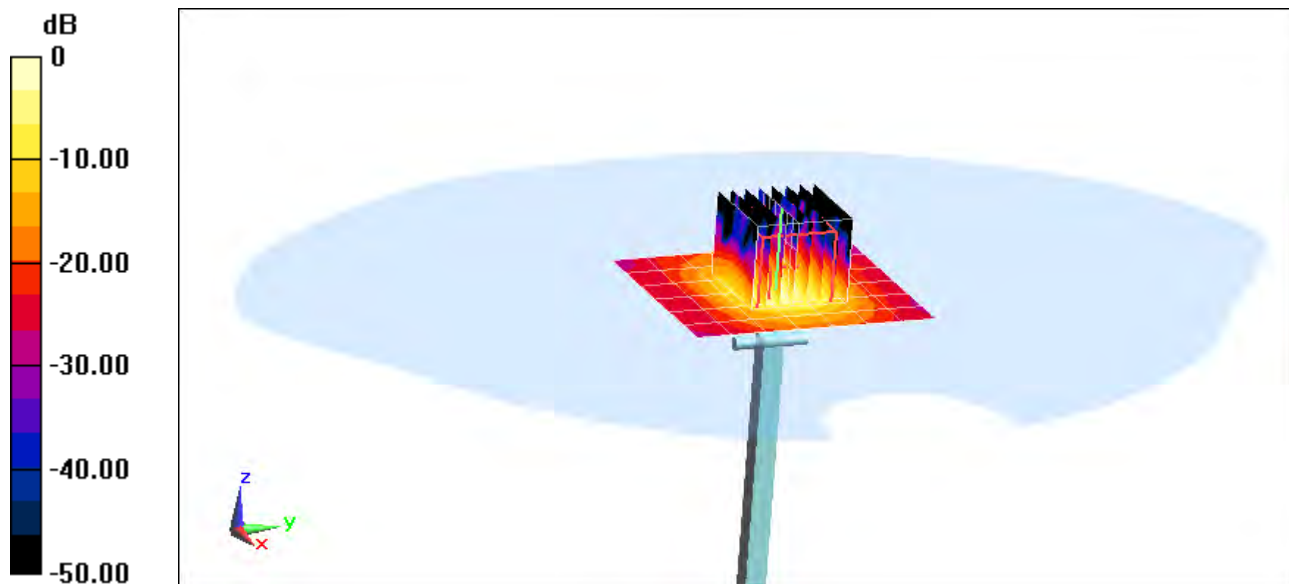

0 dB = 8.93 W/kg = 9.51 dBW/kg

# PCTEST ENGINEERING LABORATORY, INC.

**DUT: Dipole 5800 MHz; Type: D5GHzV2; Serial: 1120**

Communication System: UID 0, CW; Frequency: 5800 MHz; Duty Cycle: 1:1  
Medium: 5 GHz Body, Medium parameters used:

$f = 5800 \text{ MHz}$ ;  $\sigma = 6.172 \text{ S/m}$ ;  $\epsilon_r = 46.231$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space = 1.0 cm

Test Date: 02-09-2014; Ambient Temp: 24.5°C; Tissue Temp: 23.3°C

Probe: EX3DV4 - SN3914; ConvF(4.14, 4.14, 4.14); Calibrated: 10/23/2013;  
Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 11/19/2013

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

## 5800 MHz System Verification


**Area Scan (7x8x1):** Measurement grid: dx=10mm, dy=10mm

**Zoom Scan (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4  
Input Power = 20.0 dBm (100 mW)

Peak SAR (extrapolated) = 34.4 W/kg

**SAR(1 g) = 6.94 W/kg**

Deviation = -8.08%

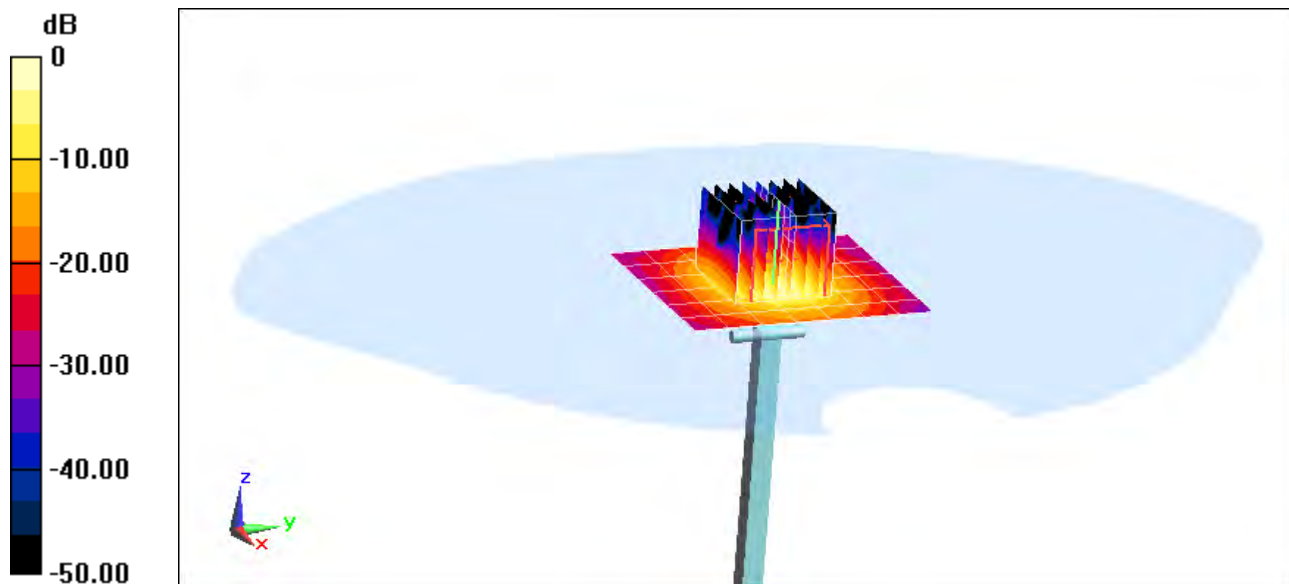

0 dB = 18.7 W/kg = 12.72 dBW/kg

## APPENDIX C: PROBE CALIBRATION



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D1765V2-1008\_May13**

## CALIBRATION CERTIFICATE

Object **D1765V2 - SN: 1008**

Calibration procedure(s) **QA CAL-05.v9**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **May 14, 2013**

*✓ 100K  
5/23/13*

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 04-Apr-13 (No. 217-01736)         | Apr-14                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 04-Apr-13 (No. 217-01739)         | Apr-14                 |
| Reference Probe ES3DV3      | SN: 3205           | 28-Dec-12 (No. ES3-3205_Dec12)    | Dec-13                 |
| DAE4                        | SN: 601            | 25-Apr-13 (No. DAE4-601_Apr13)    | Apr-14                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                |               |                       |                  |
|----------------|---------------|-----------------------|------------------|
|                | <b>Name</b>   | <b>Function</b>       | <b>Signature</b> |
| Calibrated by: | Jeton Kastrat | Laboratory Technician |                  |
| Approved by:   | Katja Pokovic | Technical Manager     |                  |

Issued: May 15, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:* SAR measured at the stated antenna input power.
- SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                        |             |
|-------------------------------------|------------------------|-------------|
| <b>DASY Version</b>                 | DASY5                  | V52.8.6     |
| <b>Extrapolation</b>                | Advanced Extrapolation |             |
| <b>Phantom</b>                      | Modular Flat Phantom   |             |
| <b>Distance Dipole Center - TSL</b> | 10 mm                  | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm      |             |
| <b>Frequency</b>                    | 1750 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 40.1           | 1.37 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 39.1 $\pm$ 6 % | 1.33 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 9.09 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>36.8 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 4.85 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>19.6 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Body TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Body TSL parameters</b>             | 22.0 °C             | 53.4           | 1.49 mho/m           |
| <b>Measured Body TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 51.7 $\pm$ 6 % | 1.47 mho/m $\pm$ 6 % |
| <b>Body TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 9.53 W/kg                                      |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>38.2 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 5.10 W/kg                                      |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>20.4 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.3 $\Omega$ - 6.4 j $\Omega$ |
| Return Loss                          | - 23.5 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 43.8 $\Omega$ - 6.1 j $\Omega$ |
| Return Loss                          | - 20.6 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.211 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                  |
|-----------------|------------------|
| Manufactured by | SPEAG            |
| Manufactured on | October 06, 2005 |

## DASY5 Validation Report for Head TSL

Date: 14.05.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1765 MHz; Type: D1765V2; Serial: D1765V2 - SN: 1008**

Communication System: UID 0 - CW ; Frequency: 1750 MHz

Medium parameters used:  $f = 1750$  MHz;  $\sigma = 1.33$  S/m;  $\epsilon_r = 39.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.18, 5.18, 5.18); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

### **Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.430 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 16.3 W/kg

**SAR(1 g) = 9.09 W/kg; SAR(10 g) = 4.85 W/kg**

Maximum value of SAR (measured) = 11.3 W/kg

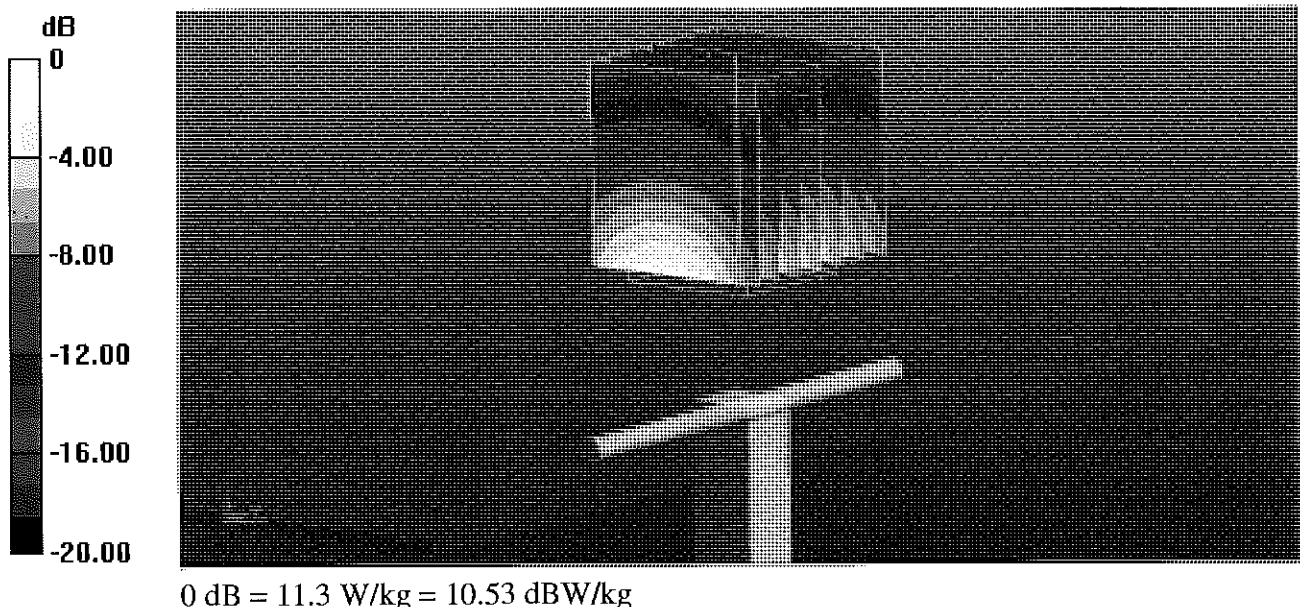

Impedance Measurement Plot for Head TSL

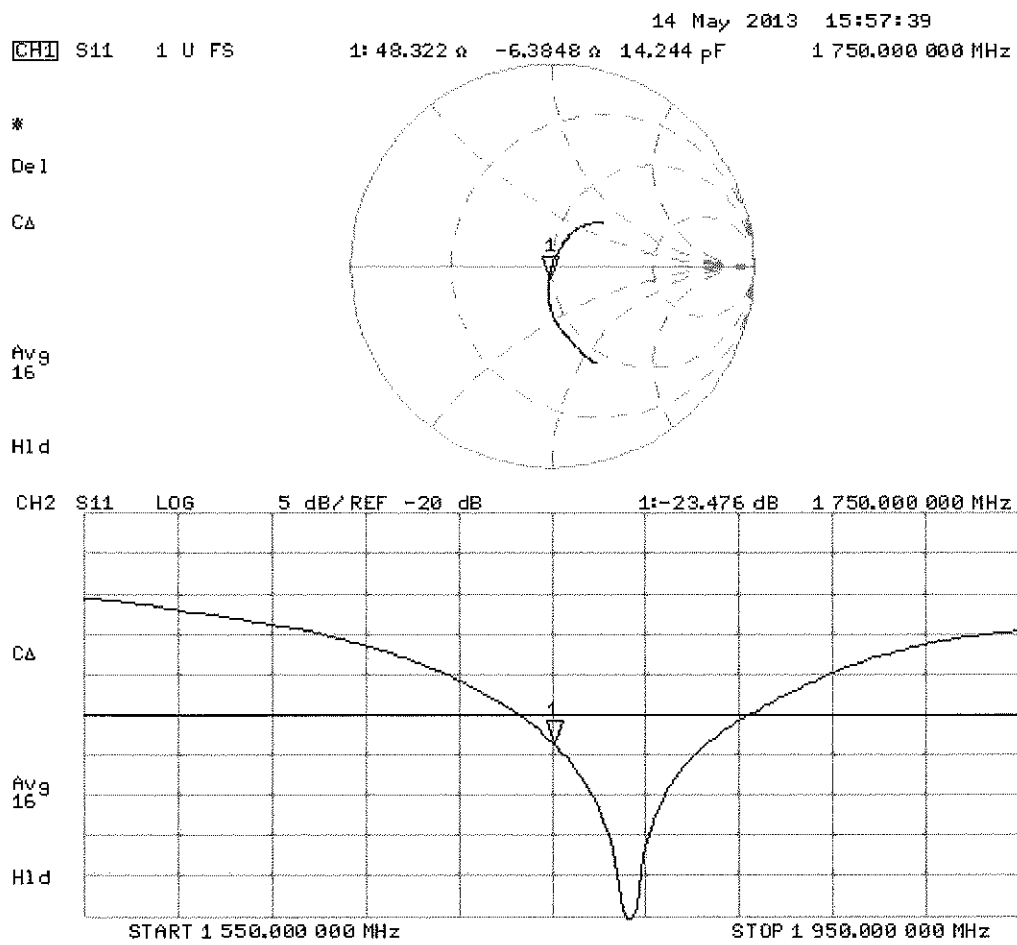

## DASY5 Validation Report for Body TSL

Date: 13.05.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1765 MHz; Type: D1765V2; Serial: D1765V2 - SN: 1008**

Communication System: UID 0 - CW ; Frequency: 1750 MHz

Medium parameters used:  $f = 1750$  MHz;  $\sigma = 1.47$  S/m;  $\epsilon_r = 51.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.83, 4.83, 4.83); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

### **Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.430 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 16.4 W/kg

**SAR(1 g) = 9.53 W/kg; SAR(10 g) = 5.1 W/kg**

Maximum value of SAR (measured) = 12.0 W/kg

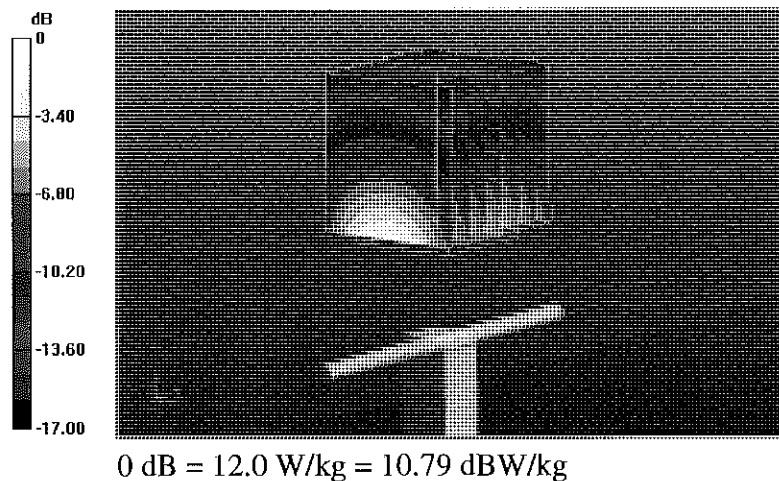

## Impedance Measurement Plot for Body TSL

13 May 2013 15:25:53  
[CH1] S11 1 U FS 1: 43.775  $\Omega$  -6.1426  $\Omega$  14.806 pF 1 750.000 000 MHz


\*

De1

Cor

Avg  
16

H1d

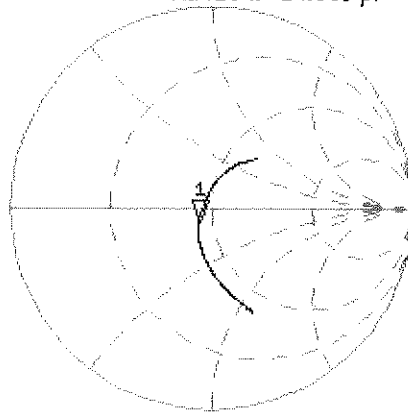


CH2 S11 LOG 5 dB/REF -20 dB 1:-20.627 dB 1 750.000 000 MHz

Cor

Avg  
16

H1d

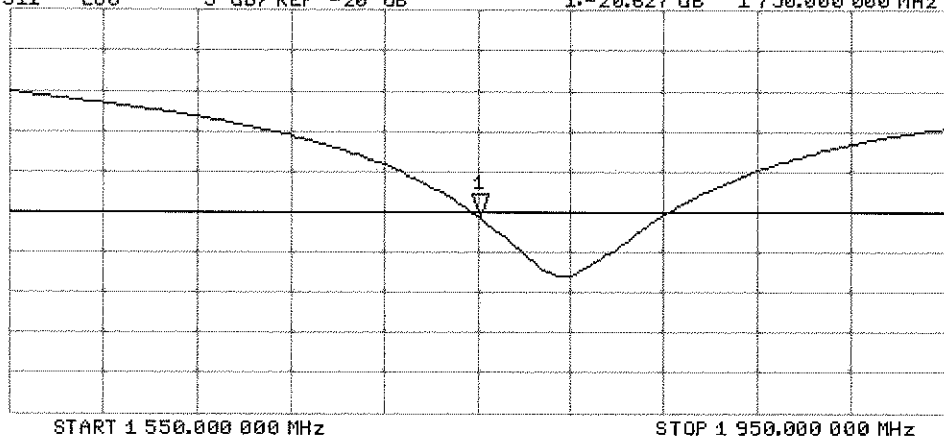



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Client **PC Test**

Certificate No: **D1900V2-5d141\_May13**

## CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d141**

Calibration procedure(s) **QA CAL-05.v9**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **May 02, 2013**

✓  
5/8/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 04-Apr-13 (No. 217-01736)         | Apr-14                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 04-Apr-13 (No. 217-01739)         | Apr-14                 |
| Reference Probe ES3DV3      | SN: 3205           | 28-Dec-12 (No. ES3-3205_Dec12)    | Dec-13                 |
| DAE4                        | SN: 601            | 25-Apr-13 (No. DAE4-601_Apr13)    | Apr-14                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

Calibrated by: **Claudio Leubler**      Name: **Claudio Leubler**      Function: **Laboratory Technician**

Approved by: **Katja Pokovic**      Name: **Katja Pokovic**      Function: **Technical Manager**

Signature

Issued: May 2, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### Additional Documentation:

- DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.6     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 1900 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 40.0           | 1.40 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 39.3 $\pm$ 6 % | 1.37 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 10.1 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 40.8 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 5.30 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 21.3 W/kg $\pm$ 16.5 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 53.3           | 1.52 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 54.0 $\pm$ 6 % | 1.51 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 10.3 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 41.5 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 5.51 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 22.1 W/kg $\pm$ 16.5 % (k=2) |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $52.6 \Omega + 4.9 j\Omega$ |
| Return Loss                          | - 25.3 dB                   |

### Antenna Parameters with Body TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $48.3 \Omega + 5.9 j\Omega$ |
| Return Loss                          | - 24.1 dB                   |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.199 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                |
|-----------------|----------------|
| Manufactured by | SPEAG          |
| Manufactured on | March 11, 2011 |

## DASY5 Validation Report for Head TSL

Date: 02.05.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d141**

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.37$  S/m;  $\epsilon_r = 39.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.98, 4.98, 4.98); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

### **Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.124 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 18.2 W/kg

**SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.3 W/kg**

Maximum value of SAR (measured) = 12.5 W/kg

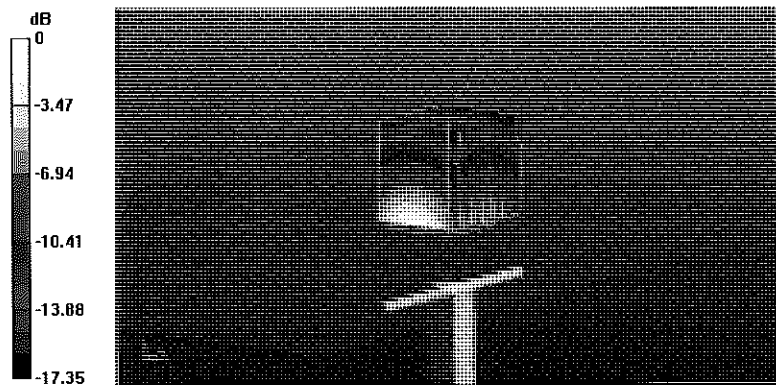

0 dB = 12.5 W/kg = 10.97 dBW/kg

## Impedance Measurement Plot for Head TSL

2 May 2013 15:38:50  
[CH1] S11 1 U FS 1: 52.600  $\Omega$  4.9375  $\Omega$  413.59  $\mu\text{H}$  1 900.000 000 MHz


\*

De1

Cor

Avg  
4

H1d

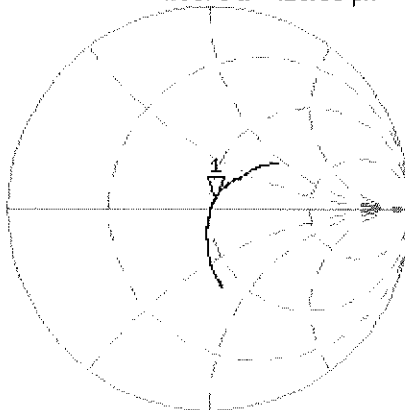


CH2 S11 LOG 5 dB/REF -20 dB 1:-25.293 dB 1 900.000 000 MHz

Cor

Avg  
4

H1d

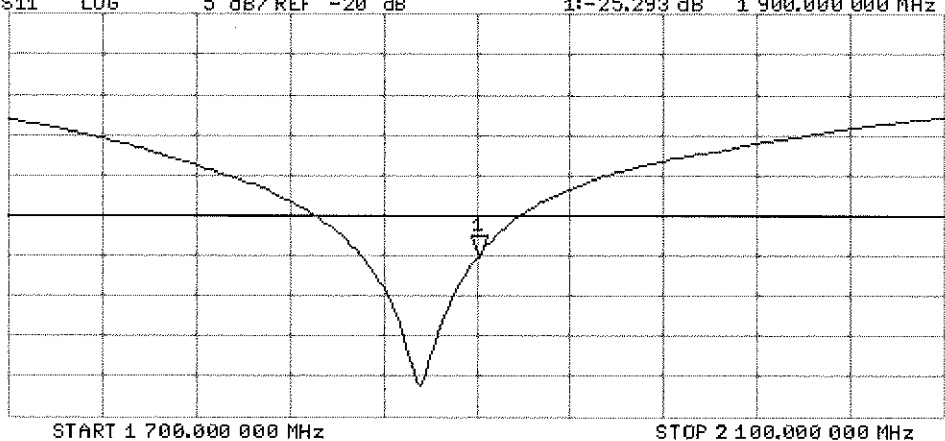

## DASY5 Validation Report for Body TSL

Date: 02.05.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d141**

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.51$  S/m;  $\epsilon_r = 54$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.6, 4.6, 4.6); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.124 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 17.6 W/kg

**SAR(1 g) = 10.3 W/kg; SAR(10 g) = 5.51 W/kg**

Maximum value of SAR (measured) = 13.0 W/kg

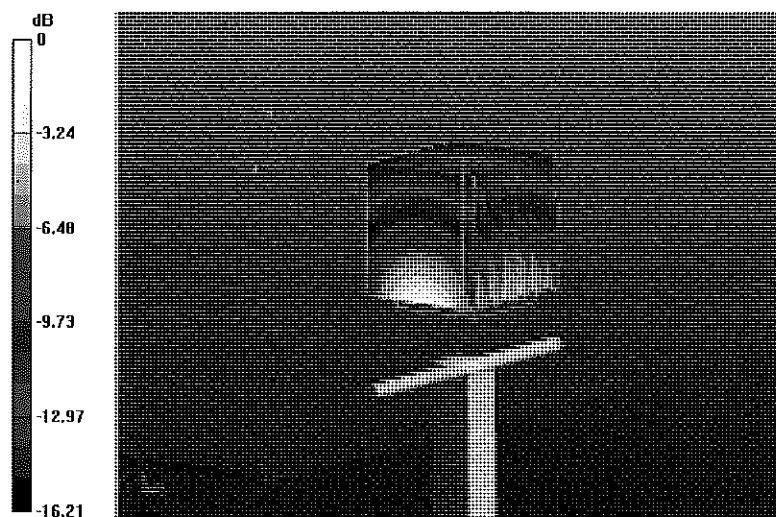

0 dB = 13.0 W/kg = 11.14 dBW/kg

# Impedance Measurement Plot for Body TSL

2 May 2013 15:38:04  
 [CH1] S11 1 U FS 1: 48.273  $\Omega$  5.9121  $\Omega$  495.23  $\mu$ H 1 900.000 000 MHz


\*

De1

Cor

Avg  
16

H1d

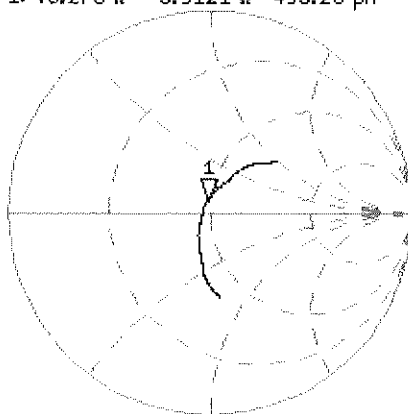


CH2 S11 LOG 5 dB/REF -20 dB 1:-24.074 dB 1 900.000 000 MHz

Cor

Avg  
16

H1d

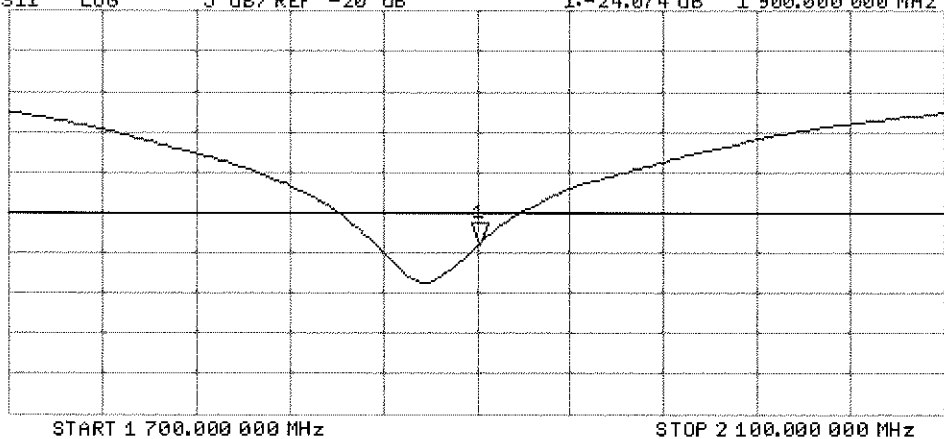



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D1900V2-5d149\_Jul13**

## CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d149**

Calibration procedure(s) **QA CAL-05.v9**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **July 22, 2013**

✓  
 KOK  
 8/19/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 04-Apr-13 (No. 217-01736)         | Apr-14                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 04-Apr-13 (No. 217-01739)         | Apr-14                 |
| Reference Probe ES3DV3      | SN: 3205           | 28-Dec-12 (No. ES3-3205_Dec12)    | Dec-13                 |
| DAE4                        | SN: 601            | 25-Apr-13 (No. DAE4-601_Apr13)    | Apr-14                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                |                |                       |           |
|----------------|----------------|-----------------------|-----------|
|                | Name           | Function              | Signature |
| Calibrated by: | Jeton Kastrati | Laboratory Technician |           |
| Approved by:   | Katja Pokovic  | Technical Manager     |           |

Issued: July 22, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                        |             |
|-------------------------------------|------------------------|-------------|
| <b>DASY Version</b>                 | DASY5                  | V52.8.7     |
| <b>Extrapolation</b>                | Advanced Extrapolation |             |
| <b>Phantom</b>                      | Modular Flat Phantom   |             |
| <b>Distance Dipole Center - TSL</b> | 10 mm                  | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm      |             |
| <b>Frequency</b>                    | 1900 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 40.0           | 1.40 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 38.9 $\pm$ 6 % | 1.36 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 9.99 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>40.4 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 5.28 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>21.3 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Body TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Body TSL parameters</b>             | 22.0 °C             | 53.3           | 1.52 mho/m           |
| <b>Measured Body TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 53.4 $\pm$ 6 % | 1.49 mho/m $\pm$ 6 % |
| <b>Body TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 10.0 W/kg                                      |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>40.5 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 5.36 W/kg                                      |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>21.6 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                               |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | $52.9\ \Omega + 6.0\ j\Omega$ |
| Return Loss                          | - 23.8 dB                     |

### Antenna Parameters with Body TSL

|                                      |                               |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | $48.5\ \Omega + 6.4\ j\Omega$ |
| Return Loss                          | - 23.5 dB                     |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.196 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                |
|-----------------|----------------|
| Manufactured by | SPEAG          |
| Manufactured on | March 11, 2011 |

## DASY5 Validation Report for Head TSL

Date: 22.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d149**

Communication System: UID 0 - CW ; Frequency: 1900 MHz

Medium parameters used:  $f = 1900 \text{ MHz}$ ;  $\sigma = 1.36 \text{ S/m}$ ;  $\epsilon_r = 38.9$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.98, 4.98, 4.98); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

### **Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**



Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 96.173 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 18.0 W/kg

**SAR(1 g) = 9.99 W/kg; SAR(10 g) = 5.28 W/kg**

Maximum value of SAR (measured) = 12.4 W/kg

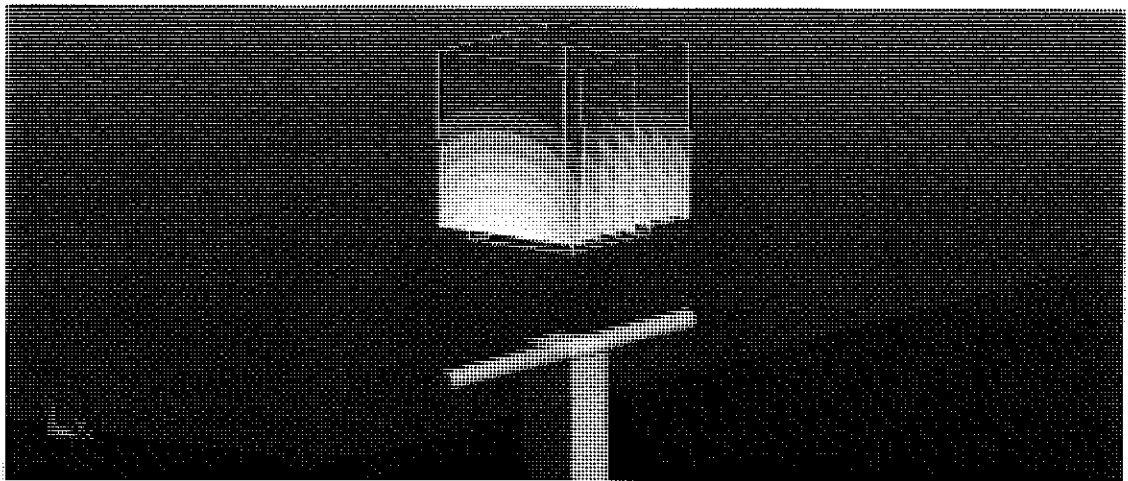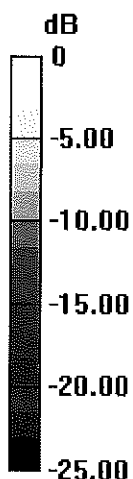


0 dB = 12.4 W/kg = 10.93 dBW/kg

# Impedance Measurement Plot for Head TSL


22 Jul 2013 11:59:34  
 CH1 S11 1 U FS 1: 52.941  $\Omega$  6.0059  $\Omega$  503.09  $\mu$ H 1 900.000 000 MHz

\*  
 Del  
 CA  
 Avg  
 16  
 H1d

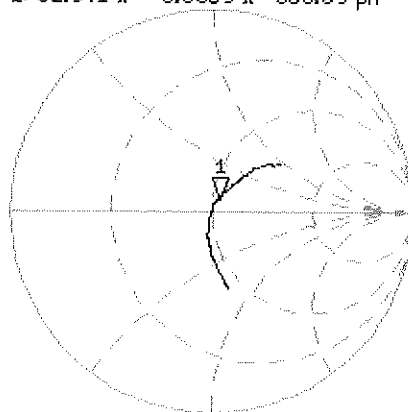

CH2 S11 LOG 5 dB/REF -20 dB 1:-23.758 dB 1 900.000 000 MHz

CA  
 Avg  
 16  
 H1d

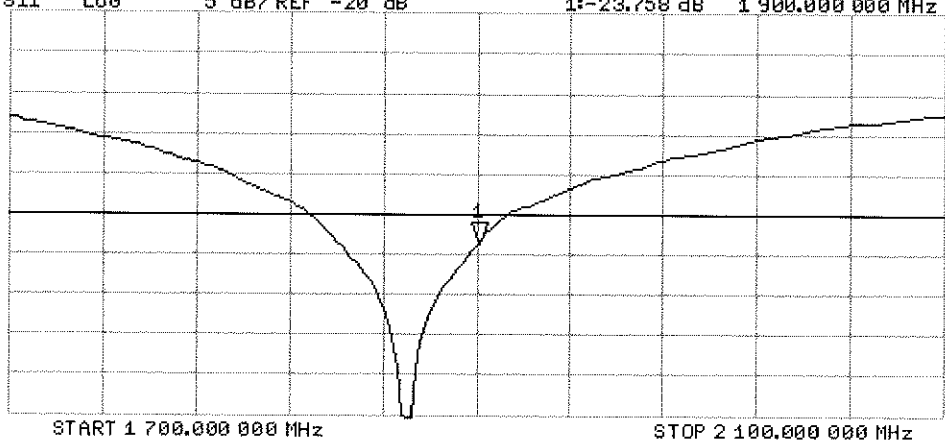

## DASY5 Validation Report for Body TSL

Date: 22.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d149**

Communication System: UID 0 - CW ; Frequency: 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.49$  S/m;  $\epsilon_r = 53.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.6, 4.6, 4.6); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

### **Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.173 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 17.0 W/kg

**SAR(1 g) = 10 W/kg; SAR(10 g) = 5.36 W/kg**

Maximum value of SAR (measured) = 12.6 W/kg

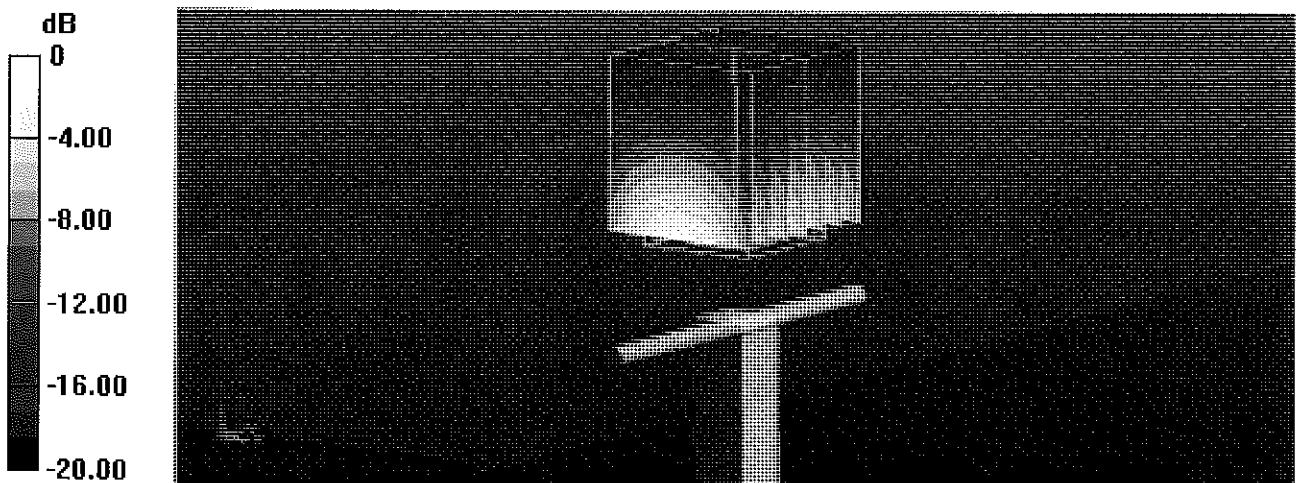


0 dB = 12.6 W/kg = 11.00 dBW/kg

## Impedance Measurement Plot for Body TSL

22 Jul 2013 11:32:14  
CH1 S11 1 U FS 1: 48.525  $\Delta$  6.3906  $\Delta$  535.32 pF 1 900.000 000 MHz

\*  
De1  
CA

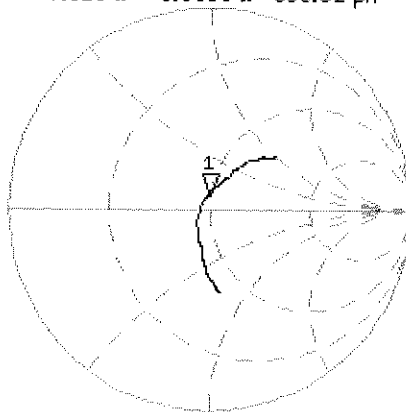

Avg  
16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 1: -23.547 dB 1 900.000 000 MHz

CA

Avg  
16

H1d

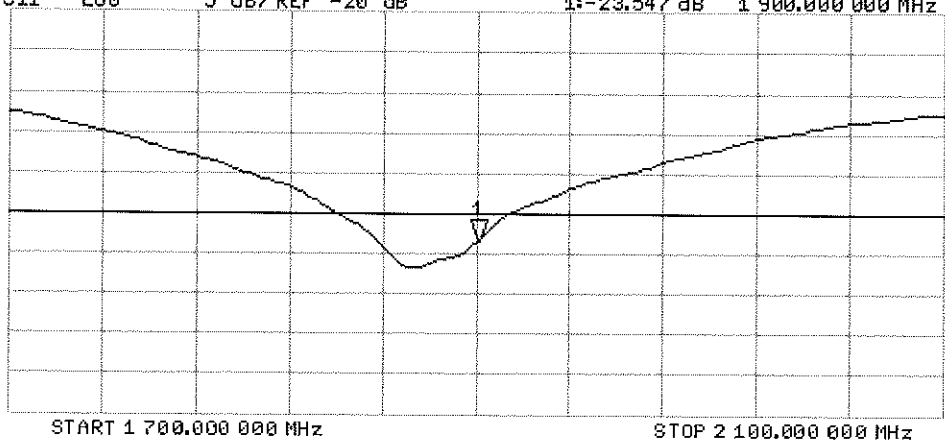



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D5GHzV2-1120\_Feb13**

## CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN: 1120**

Calibration procedure(s) **QA CAL-22.v2**  
**Calibration procedure for dipole validation kits between 3-6 GHz**

Calibration date: **February 14, 2013**

✓  
Kok  
2/2/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 27-Mar-12 (No. 217-01530)         | Apr-13                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 27-Mar-12 (No. 217-01533)         | Apr-13                 |
| Reference Probe EX3DV4      | SN: 3503           | 28-Dec-12 (No. EX3-3503_Dec12)    | Dec-13                 |
| DAE4                        | SN: 601            | 27-Jun-12 (No. DAE4-601_Jun12)    | Jun-13                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

Calibrated by: **Israe El-Naouq** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature

*Israe El-Naouq*  
*Katja Pokovic*

Issued: February 14, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- a) IEC 62209-2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", March 2010
- b) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                                                                                                                      |                                  |
|-------------------------------------|----------------------------------------------------------------------------------------------------------------------|----------------------------------|
| <b>DASY Version</b>                 | DASY5                                                                                                                | V52.8.5                          |
| <b>Extrapolation</b>                | Advanced Extrapolation                                                                                               |                                  |
| <b>Phantom</b>                      | Modular Flat Phantom V5.0                                                                                            |                                  |
| <b>Distance Dipole Center - TSL</b> | 10 mm                                                                                                                | with Spacer                      |
| <b>Zoom Scan Resolution</b>         | dx, dy = 4.0 mm, dz = 1.4 mm                                                                                         | Graded Ratio = 1.4 (Z direction) |
| <b>Frequency</b>                    | 5200 MHz $\pm$ 1 MHz<br>5300 MHz $\pm$ 1 MHz<br>5500 MHz $\pm$ 1 MHz<br>5600 MHz $\pm$ 1 MHz<br>5800 MHz $\pm$ 1 MHz |                                  |

## Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 36.0           | 4.66 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 34.7 $\pm$ 6 % | 4.47 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL at 5200 MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| SAR measured                                                | 100 mW input power | 7.67 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>76.0 W/kg <math>\pm</math> 19.9 % (k=2)</b> |

| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| SAR measured                                                  | 100 mW input power | 2.18 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>21.5 W/kg <math>\pm</math> 19.5 % (k=2)</b> |

### Head TSL parameters at 5300 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.9         | 4.76 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.5 ± 6 %   | 4.57 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5300 MHz

|                                                             |                    |                                   |
|-------------------------------------------------------------|--------------------|-----------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                   |
| SAR measured                                                | 100 mW input power | 7.94 W/kg                         |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>78.7 W / kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.27 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>22.4 W/kg ± 19.5 % (k=2)</b> |

### Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.6         | 4.96 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.2 ± 6 %   | 4.74 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5500 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.09 W/kg                       |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>80.1 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.29 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>22.6 W/kg ± 19.5 % (k=2)</b> |

### Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.5         | 5.07 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.1 ± 6 %   | 4.83 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5600 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.08 W/kg                       |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>79.9 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.28 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>22.5 W/kg ± 19.5 % (k=2)</b> |

### Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.3         | 5.27 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 33.9 ± 6 %   | 5.05 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5800 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 7.57 W/kg                       |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>74.9 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.13 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>21.0 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 49.0         | 5.30 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 46.9 ± 6 %   | 5.36 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5200 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 7.73 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>76.6 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.17 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>21.5 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5300 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.9         | 5.42 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 46.7 ± 6 %   | 5.48 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5300 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 7.75 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>76.8 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.18 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>21.5 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.6         | 5.65 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 46.3 ± 6 %   | 5.71 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5500 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.06 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>79.8 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.24 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>22.1 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5600 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.5         | 5.77 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 46.2 ± 6 %   | 5.83 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5600 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.15 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>80.7 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.26 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>22.3 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.2         | 6.00 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 45.9 ± 6 %   | 6.12 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5800 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 7.62 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>75.5 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.12 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>20.9 W/kg ± 19.5 % (k=2)</b> |

## Appendix

### Antenna Parameters with Head TSL at 5200 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $53.8 \Omega - 6.3 j\Omega$ |
| Return Loss                          | - 23.0 dB                   |

### Antenna Parameters with Head TSL at 5300 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $50.1 \Omega + 0.5 j\Omega$ |
| Return Loss                          | - 45.3 dB                   |

### Antenna Parameters with Head TSL at 5500 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $51.0 \Omega - 0.9 j\Omega$ |
| Return Loss                          | - 37.9 dB                   |

### Antenna Parameters with Head TSL at 5600 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $55.3 \Omega - 0.9 j\Omega$ |
| Return Loss                          | - 25.8 dB                   |

### Antenna Parameters with Head TSL at 5800 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $53.5 \Omega + 3.3 j\Omega$ |
| Return Loss                          | - 26.7 dB                   |

### Antenna Parameters with Body TSL at 5200 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $53.7 \Omega - 4.8 j\Omega$ |
| Return Loss                          | - 24.8 dB                   |

### Antenna Parameters with Body TSL at 5300 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $50.2 \Omega + 2.4 j\Omega$ |
| Return Loss                          | - 32.5 dB                   |

### Antenna Parameters with Body TSL at 5500 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $51.6 \Omega - 1.5 j\Omega$ |
| Return Loss                          | - 33.3 dB                   |

### Antenna Parameters with Body TSL at 5600 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $57.4 \Omega + 0.9 j\Omega$ |
| Return Loss                          | - 23.2 dB                   |



## Antenna Parameters with Body TSL at 5800 MHz

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $53.5 \Omega + 3.2 j\Omega$ |
| Return Loss                          | - 26.7 dB                   |

## General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.206 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

|                 |                    |
|-----------------|--------------------|
| Manufactured by | SPEAG              |
| Manufactured on | September 08, 2011 |

## DASY5 Validation Report for Head TSL

Date: 08.02.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1120**

Communication System: CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 4.47$  S/m;  $\epsilon_r = 34.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5300$  MHz;  $\sigma = 4.57$  S/m;  $\epsilon_r = 34.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5500$  MHz;  $\sigma = 4.74$  S/m;  $\epsilon_r = 34.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5600$  MHz;  $\sigma = 4.83$  S/m;  $\epsilon_r = 34.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.05$  S/m;  $\epsilon_r = 33.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.41, 5.41, 5.41); Calibrated: 28.12.2012, ConvF(5.1, 5.1, 5.1); Calibrated: 28.12.2012, ConvF(4.91, 4.91, 4.91); Calibrated: 28.12.2012, ConvF(4.76, 4.76, 4.76); Calibrated: 28.12.2012, ConvF(4.81, 4.81, 4.81); Calibrated: 28.12.2012;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.5(1059); SEMCAD X 14.6.8(7028)

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.561 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 28.8 W/kg

**SAR(1 g) = 7.67 W/kg; SAR(10 g) = 2.18 W/kg**

Maximum value of SAR (measured) = 17.7 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 62.429 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 30.3 W/kg

**SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg**

Maximum value of SAR (measured) = 18.5 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.998 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 32.7 W/kg

**SAR(1 g) = 8.09 W/kg; SAR(10 g) = 2.29 W/kg**

Maximum value of SAR (measured) = 19.3 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 62.540 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 33.3 W/kg

**SAR(1 g) = 8.08 W/kg; SAR(10 g) = 2.28 W/kg**

Maximum value of SAR (measured) = 19.5 W/kg


**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.600 V/m; Power Drift = 0.09 dB


Peak SAR (extrapolated) = 32.9 W/kg

**SAR(1 g) = 7.57 W/kg; SAR(10 g) = 2.13 W/kg**

Maximum value of SAR (measured) = 18.8 W/kg

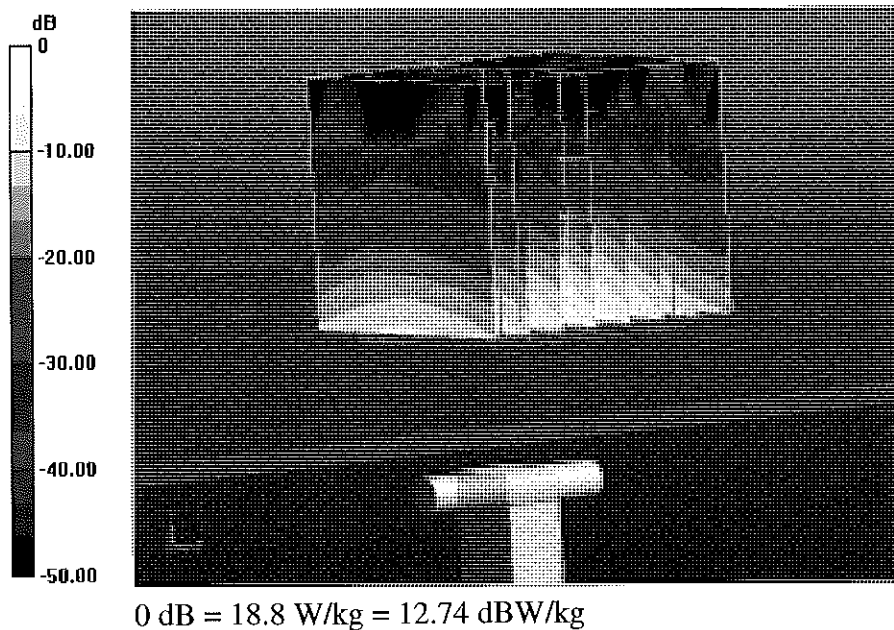

Impedance Measurement Plot for Head TSL

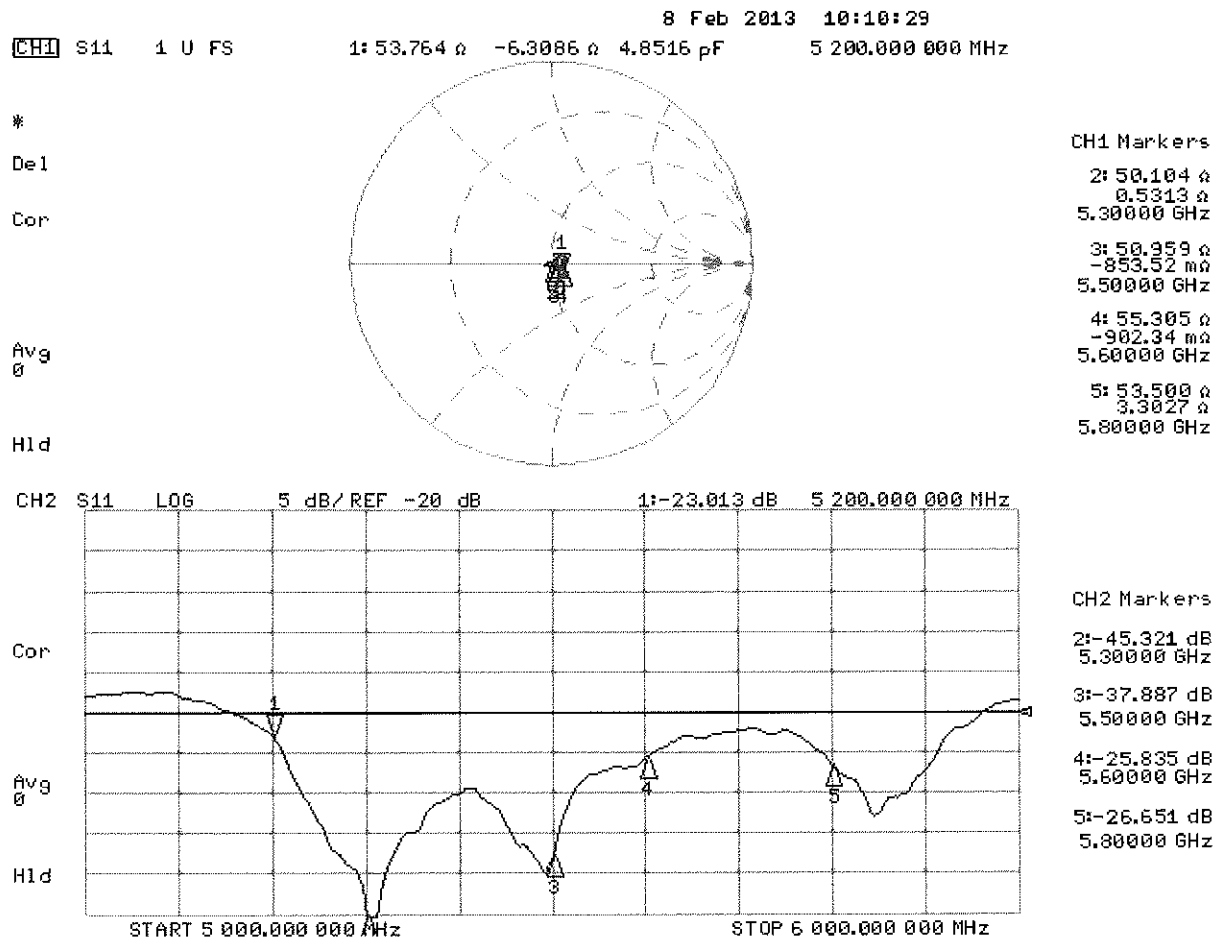

## DASY5 Validation Report for Body TSL

Date: 14.02.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1120**

Communication System: CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 5.36$  S/m;  $\epsilon_r = 46.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5300$  MHz;  $\sigma = 5.48$  S/m;  $\epsilon_r = 46.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5500$  MHz;  $\sigma = 5.71$  S/m;  $\epsilon_r = 46.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5600$  MHz;  $\sigma = 5.83$  S/m;  $\epsilon_r = 46.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5800$  MHz;  $\sigma = 6.12$  S/m;  $\epsilon_r = 45.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.91, 4.91, 4.91); Calibrated: 28.12.2012, ConvF(4.67, 4.67, 4.67); Calibrated: 28.12.2012, ConvF(4.43, 4.43, 4.43); Calibrated: 28.12.2012, ConvF(4.22, 4.22, 4.22); Calibrated: 28.12.2012, ConvF(4.38, 4.38, 4.38); Calibrated: 28.12.2012;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.5(1059); SEMCAD X 14.6.8(7028)

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.053 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 31.1 W/kg

**SAR(1 g) = 7.73 W/kg; SAR(10 g) = 2.17 W/kg**

Maximum value of SAR (measured) = 18.2 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 60.021 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 32.1 W/kg

**SAR(1 g) = 7.75 W/kg; SAR(10 g) = 2.18 W/kg**

Maximum value of SAR (measured) = 18.5 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 59.894 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 35.3 W/kg

**SAR(1 g) = 8.06 W/kg; SAR(10 g) = 2.24 W/kg**

Maximum value of SAR (measured) = 19.4 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 59.730 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 36.8 W/kg

**SAR(1 g) = 8.15 W/kg; SAR(10 g) = 2.26 W/kg**

Maximum value of SAR (measured) = 19.9 W/kg


**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 56.663 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 36.4 W/kg

**SAR(1 g) = 7.62 W/kg; SAR(10 g) = 2.12 W/kg**

Maximum value of SAR (measured) = 19.0 W/kg

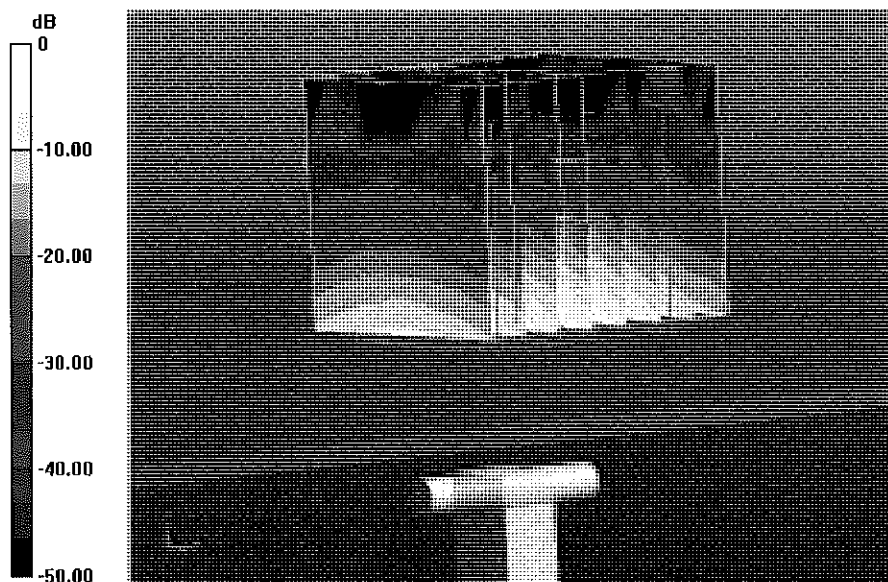


0 dB = 19.0 W/kg = 12.79 dBW/kg

# Impedance Measurement Plot for Body TSL

14 Feb 2013 15:47:05  
 CH1 S11 1 U F8 1: 53.672  $\Omega$  -4.7539  $\Omega$  6.4382 pF 5 200.000 000 MHz


\*  
 Del  
 Cor  
 Avg  
 16  
 H1d

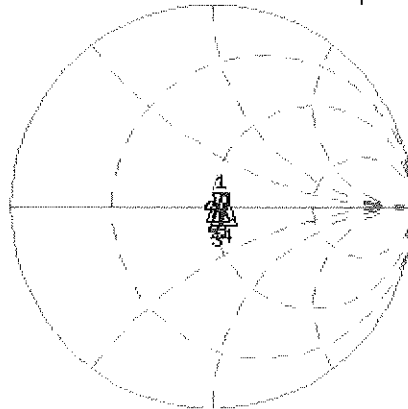

CH1 Markers  
 2: 50.250  $\Omega$   
 2.3555  $\Omega$   
 5.30000 GHz  
 3: 51.629  $\Omega$   
 -1.4824  $\Omega$   
 5.50000 GHz  
 4: 57.389  $\Omega$   
 0.9180  $\Omega$   
 5.60000 GHz  
 5: 53.543  $\Omega$   
 3.2441  $\Omega$   
 5.80000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 1:-24.750 dB 5 200.000 000 MHz

Cor  
 Avg  
 16  
 H1d

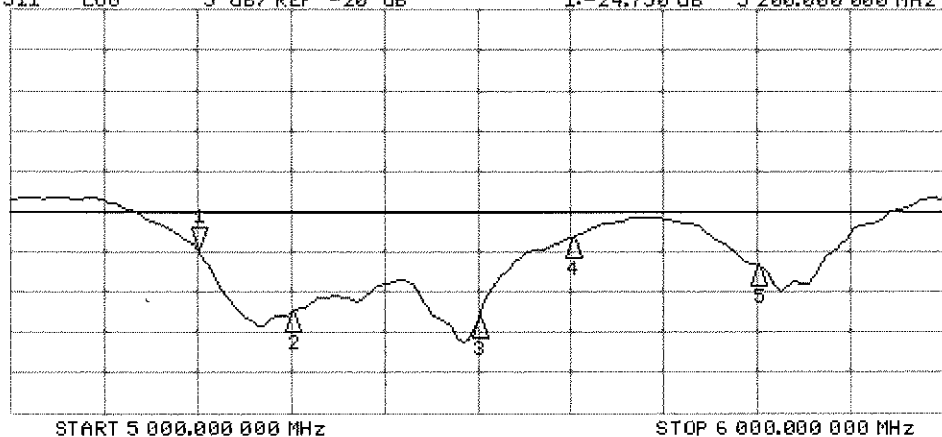

CH2 Markers  
 2:-32.508 dB  
 5.30000 GHz  
 3:-33.267 dB  
 5.50000 GHz  
 4:-23.183 dB  
 5.60000 GHz  
 5:-26.672 dB  
 5.80000 GHz



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **PC Test**

Certificate No: **D5GHzV2-1057\_Jan14**

## CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN: 1057**

Calibration procedure(s) **QA CAL-22.v2**  
**Calibration procedure for dipole validation kits between 3-6 GHz**

Calibration date: **January 27, 2014**

CC  
2/5/14 ✓

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 09-Oct-13 (No. 217-01827)         | Oct-14                 |
| Power sensor HP 8481A       | US37292783         | 09-Oct-13 (No. 217-01827)         | Oct-14                 |
| Power sensor HP 8481A       | MY41092317         | 09-Oct-13 (No. 217-01828)         | Oct-14                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 04-Apr-13 (No. 217-01736)         | Apr-14                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 04-Apr-13 (No. 217-01739)         | Apr-14                 |
| Reference Probe EX3DV4      | SN: 3503           | 30-Dec-13 (No. EX3-3503_Dec13)    | Dec-14                 |
| DAE4                        | SN: 601            | 25-Apr-13 (No. DAE4-601_Apr13)    | Apr-14                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-13) | In house check: Oct-16 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

Calibrated by: **Israe El-Naouq** **Laboratory Technician**

Approved by: **Kalja Pokovic** **Technical Manager**

Signature

*Israe El-Naouq*  
*Kalja Pokovic*

Issued: January 27, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEC 62209-2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"
- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

### Additional Documentation:

- DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                                                                                                                      |                                  |
|-------------------------------------|----------------------------------------------------------------------------------------------------------------------|----------------------------------|
| <b>DASY Version</b>                 | DASY5                                                                                                                | V52.8.7                          |
| <b>Extrapolation</b>                | Advanced Extrapolation                                                                                               |                                  |
| <b>Phantom</b>                      | Modular Flat Phantom V5.0                                                                                            |                                  |
| <b>Distance Dipole Center - TSL</b> | 10 mm                                                                                                                | with Spacer                      |
| <b>Zoom Scan Resolution</b>         | dx, dy = 4.0 mm, dz = 1.4 mm                                                                                         | Graded Ratio = 1.4 (Z direction) |
| <b>Frequency</b>                    | 5200 MHz $\pm$ 1 MHz<br>5300 MHz $\pm$ 1 MHz<br>5500 MHz $\pm$ 1 MHz<br>5600 MHz $\pm$ 1 MHz<br>5800 MHz $\pm$ 1 MHz |                                  |

## Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 36.0           | 4.66 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 35.0 $\pm$ 6 % | 4.45 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL at 5200 MHz

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                | 100 mW input power | 7.85 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>78.0 W/kg <math>\pm</math> 19.9 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
| SAR measured                                                  | 100 mW input power | 2.25 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>22.3 W/kg <math>\pm</math> 19.5 % (k=2)</b> |

### Head TSL parameters at 5300 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.9         | 4.76 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.9 ± 6 %   | 4.54 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5300 MHz

|                                                             |                    |                                   |
|-------------------------------------------------------------|--------------------|-----------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                   |
| SAR measured                                                | 100 mW input power | 8.36 W/kg                         |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>83.0 W / kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.40 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>23.8 W/kg ± 19.5 % (k=2)</b> |

### Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.6         | 4.96 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.6 ± 6 %   | 4.74 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5500 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.50 W/kg                       |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>84.3 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.42 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>24.0 W/kg ± 19.5 % (k=2)</b> |

### Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.5         | 5.07 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.5 ± 6 %   | 4.86 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5600 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.42 W/kg                       |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>83.5 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.40 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>23.8 W/kg ± 19.5 % (k=2)</b> |

### Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.3         | 5.27 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.2 ± 6 %   | 5.07 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Head TSL at 5800 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.00 W/kg                       |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>79.3 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.28 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>22.6 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 49.0         | 5.30 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 47.3 ± 6 %   | 5.44 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5200 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                 |
|-------------------------------------------------------|--------------------|---------------------------------|
| SAR measured                                          | 100 mW input power | 7.58 W/kg                       |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | <b>75.3 W/kg ± 19.9 % (k=2)</b> |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                 |
|---------------------------------------------------------|--------------------|---------------------------------|
| SAR measured                                            | 100 mW input power | 2.12 W/kg                       |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | <b>21.0 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5300 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.9         | 5.42 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 47.2 ± 6 %   | 5.57 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5300 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                 |
|-------------------------------------------------------|--------------------|---------------------------------|
| SAR measured                                          | 100 mW input power | 7.79 W/kg                       |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | <b>77.4 W/kg ± 19.9 % (k=2)</b> |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                 |
|---------------------------------------------------------|--------------------|---------------------------------|
| SAR measured                                            | 100 mW input power | 2.17 W/kg                       |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | <b>21.5 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.6         | 5.65 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 46.8 ± 6 %   | 5.84 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5500 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 7.96 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>79.1 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.22 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>22.0 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5600 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.5         | 5.77 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 46.6 ± 6 %   | 5.98 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5600 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 8.07 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>80.2 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.24 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>22.2 W/kg ± 19.5 % (k=2)</b> |

### Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 48.2         | 6.00 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 46.3 ± 6 %   | 6.23 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

### SAR result with Body TSL at 5800 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 7.48 W/kg                       |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>74.3 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.06 W/kg                       |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>20.4 W/kg ± 19.5 % (k=2)</b> |

## Appendix

### Antenna Parameters with Head TSL at 5200 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 43.1 $\Omega$ - 4.6 j $\Omega$ |
| Return Loss                          | - 21.0 dB                      |

### Antenna Parameters with Head TSL at 5300 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 46.5 $\Omega$ - 1.3 j $\Omega$ |
| Return Loss                          | - 28.1 dB                      |

### Antenna Parameters with Head TSL at 5500 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 46.2 $\Omega$ - 2.5 j $\Omega$ |
| Return Loss                          | - 26.4 dB                      |

### Antenna Parameters with Head TSL at 5600 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.9 $\Omega$ - 5.7 j $\Omega$ |
| Return Loss                          | - 24.6 dB                      |

### Antenna Parameters with Head TSL at 5800 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.7 $\Omega$ - 3.1 j $\Omega$ |
| Return Loss                          | - 29.5 dB                      |

### Antenna Parameters with Body TSL at 5200 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 49.4 $\Omega$ - 7.7 j $\Omega$ |
| Return Loss                          | - 22.2 dB                      |

### Antenna Parameters with Body TSL at 5300 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 49.6 $\Omega$ - 3.0 j $\Omega$ |
| Return Loss                          | - 30.3 dB                      |

### Antenna Parameters with Body TSL at 5500 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.8 $\Omega$ - 3.9 j $\Omega$ |
| Return Loss                          | - 28.0 dB                      |



### Antenna Parameters with Body TSL at 5600 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 55.4 $\Omega$ - 2.5 j $\Omega$ |
| Return Loss                          | - 25.0 dB                      |

### Antenna Parameters with Body TSL at 5800 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 52.3 $\Omega$ - 0.7 j $\Omega$ |
| Return Loss                          | - 32.5 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.186 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                   |
|-----------------|-------------------|
| Manufactured by | SPEAG             |
| Manufactured on | November 27, 2006 |

## DASY5 Validation Report for Head TSL

Date: 27.01.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1057**

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 4.45$  S/m;  $\epsilon_r = 35$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5300$  MHz;  $\sigma = 4.54$  S/m;  $\epsilon_r = 34.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5500$  MHz;  $\sigma = 4.74$  S/m;  $\epsilon_r = 34.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5600$  MHz;  $\sigma = 4.86$  S/m;  $\epsilon_r = 34.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.07$  S/m;  $\epsilon_r = 34.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.52, 5.52, 5.52); Calibrated: 30.12.2013, ConvF(5.2, 5.2, 5.2); Calibrated: 30.12.2013, ConvF(5.01, 5.01, 5.01); Calibrated: 30.12.2013, ConvF(4.86, 4.86, 4.86); Calibrated: 30.12.2013, ConvF(4.91, 4.91, 4.91); Calibrated: 30.12.2013;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 63.497 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 28.2 W/kg

**SAR(1 g) = 7.85 W/kg; SAR(10 g) = 2.25 W/kg**

Maximum value of SAR (measured) = 18.6 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.444 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 31.2 W/kg

**SAR(1 g) = 8.36 W/kg; SAR(10 g) = 2.4 W/kg**

Maximum value of SAR (measured) = 20.1 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 63.807 V/m; Power Drift = 0.07 dB


Peak SAR (extrapolated) = 33.0 W/kg

**SAR(1 g) = 8.5 W/kg; SAR(10 g) = 2.42 W/kg**

Maximum value of SAR (measured) = 20.8 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 63.194 V/m; Power Drift = 0.06 dB  
Peak SAR (extrapolated) = 33.2 W/kg  
SAR(1 g) = 8.42 W/kg; SAR(10 g) = 2.4 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 60.646 V/m; Power Drift = 0.08 dB  
Peak SAR (extrapolated) = 32.9 W/kg  
SAR(1 g) = 8 W/kg; SAR(10 g) = 2.28 W/kg  
Maximum value of SAR (measured) = 19.9 W/kg

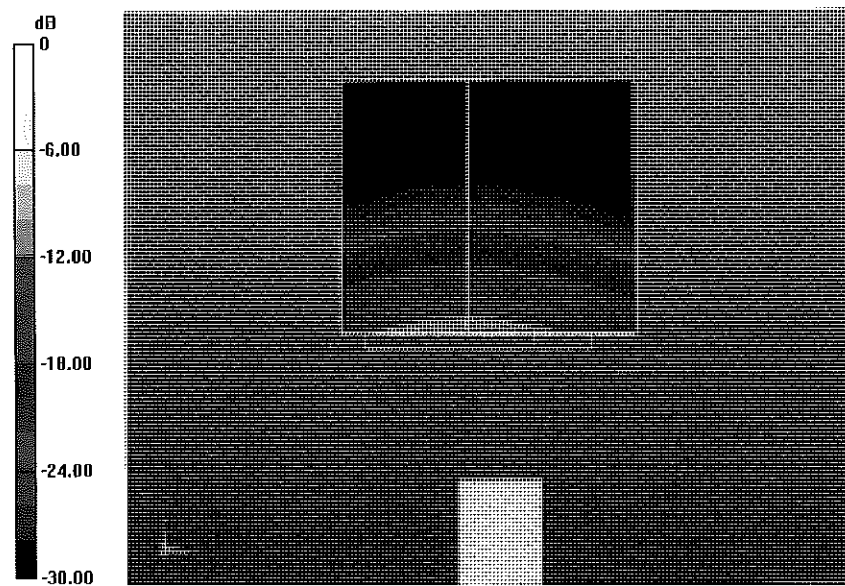


0 dB = 19.9 W/kg = 12.99 dBW/kg

# Impedance Measurement Plot for Head TSL

27 Jan 2014 17:12:04  
 CH1 S11 1 U FS 1: 43.092  $\Omega$  -4.5938  $\Omega$  6.6627 pF 5 200.000 000 MHz

\*  
 Del  
 Cor  
 Avg  
 16  
 H1d

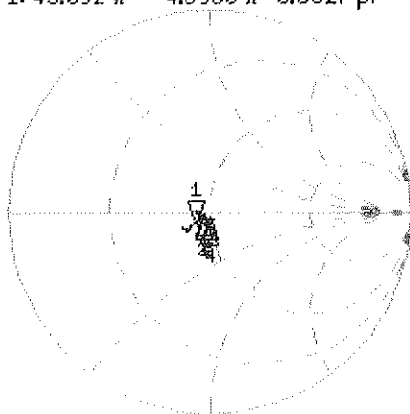


CH1 Markers

2: 46.475  $\Omega$   
 -1.3496  $\Omega$   
 5.30000 GHz  
 3: 46.150  $\Omega$   
 -2.5078  $\Omega$   
 5.50000 GHz  
 4: 48.900  $\Omega$   
 -5.6932  $\Omega$   
 5.60000 GHz  
 5: 48.734  $\Omega$   
 -3.0762  $\Omega$   
 5.80000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 1:-21.014 dB 5 200.000 000 MHz

Del  
 Cor  
 Avg  
 16  
 H1d

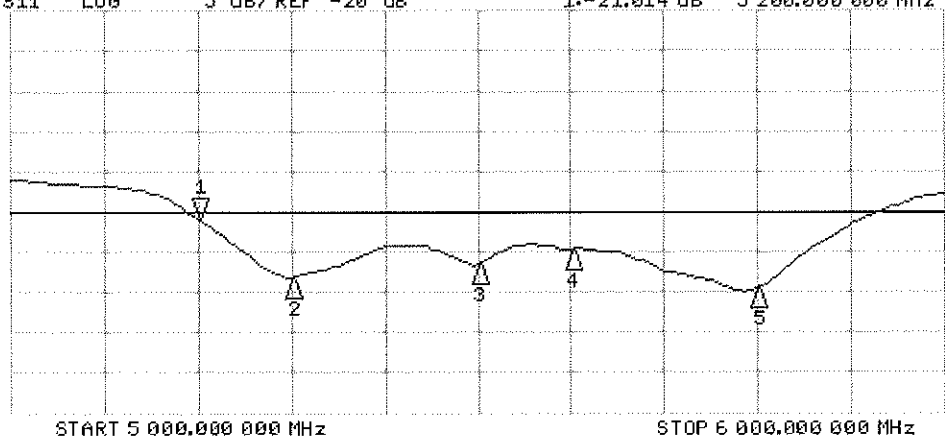

CH2 Markers

2:-28.145 dB  
 5.30000 GHz  
 3:-26.415 dB  
 5.50000 GHz  
 4:-24.640 dB  
 5.60000 GHz  
 5:-29.464 dB  
 5.80000 GHz

## DASY5 Validation Report for Body TSL

Date: 24.01.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1057**

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 5.44$  S/m;  $\epsilon_r = 47.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5300$  MHz;  $\sigma = 5.57$  S/m;  $\epsilon_r = 47.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5500$  MHz;  $\sigma = 5.84$  S/m;  $\epsilon_r = 46.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5600$  MHz;  $\sigma = 5.98$  S/m;  $\epsilon_r = 46.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5800$  MHz;  $\sigma = 6.23$  S/m;  $\epsilon_r = 46.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.01, 5.01, 5.01); Calibrated: 30.12.2013, ConvF(4.76, 4.76, 4.76); Calibrated: 30.12.2013, ConvF(4.52, 4.52, 4.52); Calibrated: 30.12.2013, ConvF(4.3, 4.3, 4.3); Calibrated: 30.12.2013, ConvF(4.47, 4.47, 4.47); Calibrated: 30.12.2013;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.809 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 30.1 W/kg

**SAR(1 g) = 7.58 W/kg; SAR(10 g) = 2.12 W/kg**

Maximum value of SAR (measured) = 18.2 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.585 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 32.2 W/kg

**SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.17 W/kg**

Maximum value of SAR (measured) = 19.1 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.364 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 34.4 W/kg

**SAR(1 g) = 7.96 W/kg; SAR(10 g) = 2.22 W/kg**

Maximum value of SAR (measured) = 19.4 W/kg

**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 57.864 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 35.8 W/kg

**SAR(1 g) = 8.07 W/kg; SAR(10 g) = 2.24 W/kg**

Maximum value of SAR (measured) = 19.8 W/kg


**Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 54.817 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 35.1 W/kg

**SAR(1 g) = 7.48 W/kg; SAR(10 g) = 2.06 W/kg**

Maximum value of SAR (measured) = 18.8 W/kg

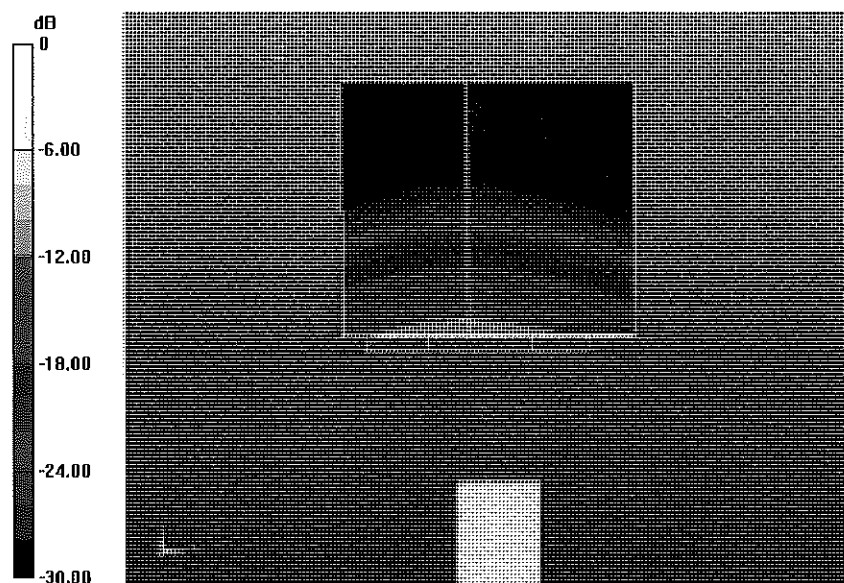


0 dB = 18.8 W/kg = 12.74 dBW/kg

# Impedance Measurement Plot for Body TSL

24 Jan 2014 15:50:22  
**CH1** S11 1 U FS 1: 49.354  $\Omega$  -7.7188  $\Omega$  3.9652 pF 5 200.000 000 MHz


\*  
 Del  
 Cor  
 Avg  
 16  
 H1d

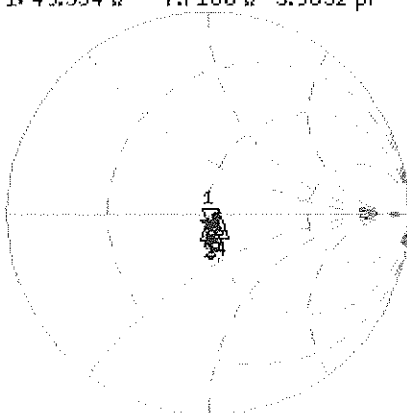

CH1 Markers  
 2: 49.559  $\Omega$   
 -3.0176  $\Omega$   
 5.30000 GHz  
 3: 50.793  $\Omega$   
 -3.9160  $\Omega$   
 5.50000 GHz  
 4: 55.393  $\Omega$   
 -2.5176  $\Omega$   
 5.60000 GHz  
 5: 52.320  $\Omega$   
 -716.80 m $\Omega$   
 5.80000 GHz

CH2 S11 L06 5 dB/REF -20 dB 1:-22.190 dB 5 200.000 000 MHz

Cor  
 Avg  
 16  
 H1d

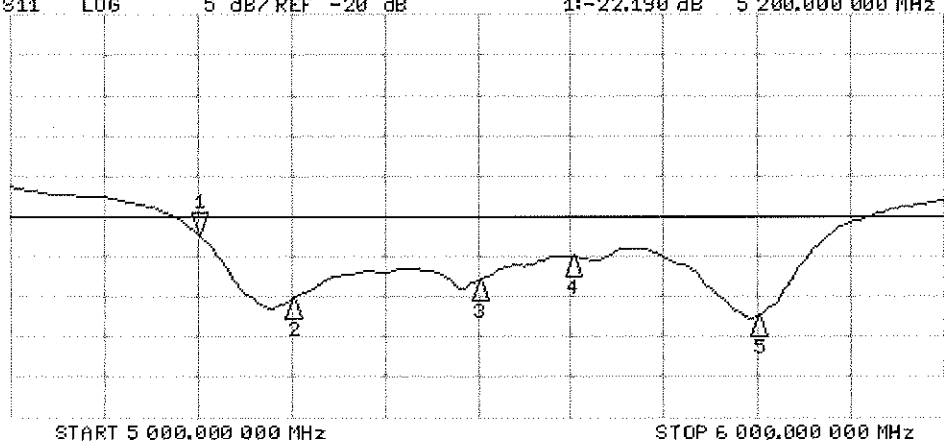

CH2 Markers  
 2:-30.277 dB  
 5.30000 GHz  
 3:-28.039 dB  
 5.50000 GHz  
 4:-24.960 dB  
 5.60000 GHz  
 5:-32.401 dB  
 5.80000 GHz



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D750V3-1046\_Feb13**

## CALIBRATION CERTIFICATE

Object **D750V3 - SN: 1046**

Calibration procedure(s) **QA CAL-05.v9**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **February 13, 2013**

✓  
KOK  
2/21/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)     | Scheduled Calibration |
|-----------------------------|--------------------|--------------------------------|-----------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)      | Oct-13                |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)      | Oct-13                |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 27-Mar-12 (No. 217-01530)      | Apr-13                |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 27-Mar-12 (No. 217-01533)      | Apr-13                |
| Reference Probe ES3DV3      | SN: 3205           | 28-Dec-12 (No. ES3-3205_Dec12) | Dec-13                |
| DAE4                        | SN: 601            | 27-Jun-12 (No. DAE4-601_Jun12) | Jun-13                |

| Secondary Standards       | ID #             | Check Date (in house)             | Scheduled Check        |
|---------------------------|------------------|-----------------------------------|------------------------|
| Power sensor HP 8481A     | MY41092317       | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06   | 100005           | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                |               |                       |           |
|----------------|---------------|-----------------------|-----------|
|                | Name          | Function              | Signature |
| Calibrated by: | Leif Klysner  | Laboratory Technician |           |
| Approved by:   | Katja Pokovic | Technical Manager     |           |

Issued: February 13, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.5     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 15 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 750 MHz $\pm$ 1 MHz    |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 41.9           | 0.89 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 41.2 $\pm$ 6 % | 0.91 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                       |                    |                                                |
|-------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                                |
| SAR measured                                          | 250 mW input power | 2.17 W/kg                                      |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | <b>8.50 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                         |                    |                                                |
|---------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                                |
| SAR measured                                            | 250 mW input power | 1.41 W/kg                                      |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | <b>5.55 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 55.5           | 0.96 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 54.8 $\pm$ 6 % | 0.99 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                       |                    |                                                |
|-------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                                |
| SAR measured                                          | 250 mW input power | 2.25 W/kg                                      |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | <b>8.77 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                         |                    |                                                |
|---------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                                |
| SAR measured                                            | 250 mW input power | 1.49 W/kg                                      |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | <b>5.84 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $56.3 \Omega + 1.4 j\Omega$ |
| Return Loss                          | - 24.3 dB                   |

### Antenna Parameters with Body TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $52.0 \Omega - 1.1 j\Omega$ |
| Return Loss                          | - 32.9 dB                   |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.038 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                    |
|-----------------|--------------------|
| Manufactured by | SPEAG              |
| Manufactured on | September 02, 2011 |

## DASY5 Validation Report for Head TSL

Date: 13.02.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1046**

Communication System: CW; Frequency: 750 MHz

Medium parameters used:  $f = 750 \text{ MHz}$ ;  $\sigma = 0.91 \text{ S/m}$ ;  $\epsilon_r = 41.2$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.28, 6.28, 6.28); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.5(1059); SEMCAD X 14.6.8(7028)

### **Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 52.942 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 3.32 W/kg

**SAR(1 g) = 2.17 W/kg; SAR(10 g) = 1.41 W/kg**


Maximum value of SAR (measured) = 2.55 W/kg

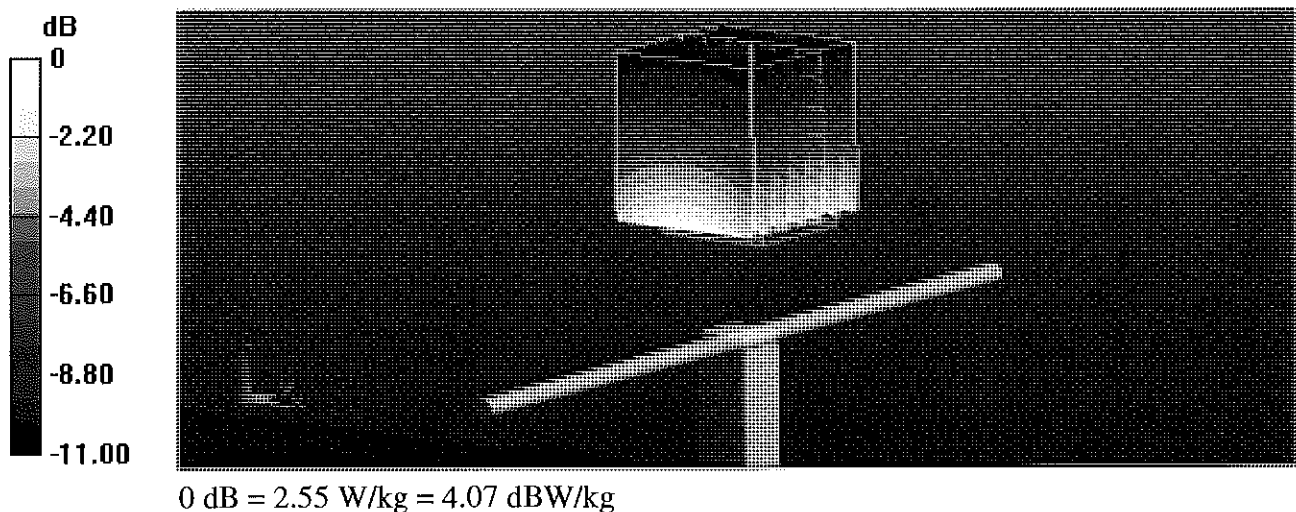

# Impedance Measurement Plot for Head TSL


13 Feb 2013 16:15:52  
 CH1 S11 1 U FS 1: 56.305  $\Omega$  1.4043  $\Omega$  298.00 pF 750.000 000 MHz

\*  
 Del  
 Cor  
 Avg  
 16  
 H1d

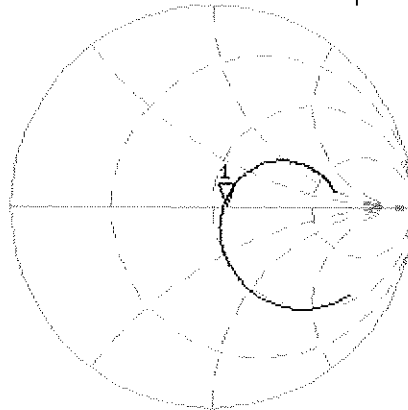

CH2 S11 LOG 5 dB/REF -20 dB 1: -24.327 dB 750.000 000 MHz

Cor  
 Avg  
 16  
 H1d

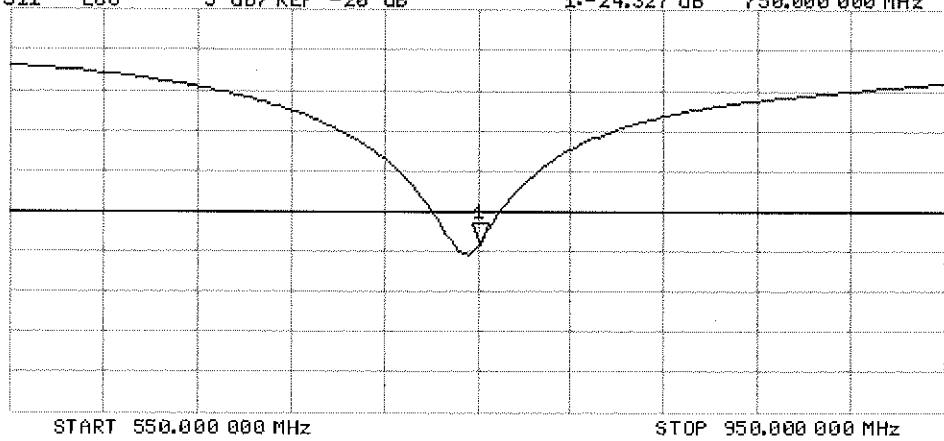

## DASY5 Validation Report for Body TSL

Date: 13.02.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1046**

Communication System: CW; Frequency: 750 MHz

Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.99$  S/m;  $\epsilon_r = 54.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.11, 6.11, 6.11); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.5(1059); SEMCAD X 14.6.8(7028)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 52.942 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 3.29 W/kg

**SAR(1 g) = 2.25 W/kg; SAR(10 g) = 1.49 W/kg**

Maximum value of SAR (measured) = 2.61 W/kg

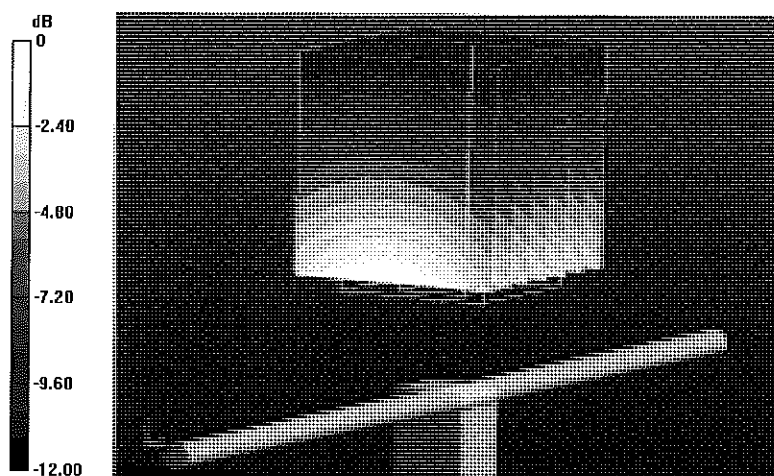


0 dB = 2.61 W/kg = 4.17 dBW/kg

# Impedance Measurement Plot for Body TSL

13 Feb 2013 10:40:44  
 CH1 S11 1 U FS 1: 52.045  $\Omega$  -1.0898  $\Omega$  194.71 pF 750.000 000 MHz

#  
 Del  
 CA

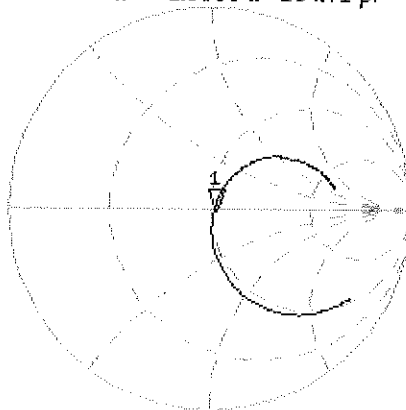

Avg  
 16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 1: -32.864 dB 750.000 000 MHz

CA

Avg  
 16

H1d

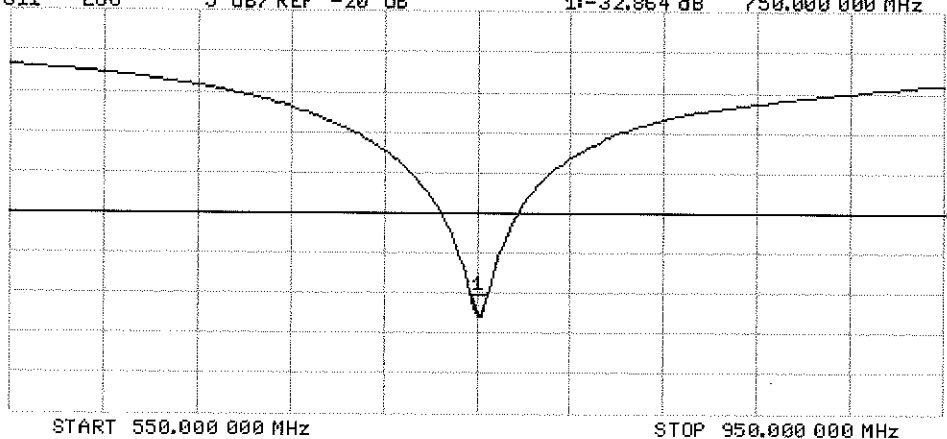



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D750V3-1054\_Mar13**

## CALIBRATION CERTIFICATE

Object **D750V3 - SN: 1054**

Calibration procedure(s) **QA CAL-05.v9**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **March 18, 2013**

✓ KOK  
3/22/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 27-Mar-12 (No. 217-01530)         | Apr-13                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 27-Mar-12 (No. 217-01533)         | Apr-13                 |
| Reference Probe ES3DV3      | SN: 3205           | 28-Dec-12 (No. ES3-3205_Dec12)    | Dec-13                 |
| DAE4                        | SN: 601            | 27-Jun-12 (No. DAE4-601_Jun12)    | Jun-13                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

Calibrated by: **Israe El-Naouq** **Israe El-Naouq** **Israe El-Naouq**  
 Name Function Laboratory Technician

Approved by: **Katja Pokovic** **Katja Pokovic** **Katja Pokovic**  
 Name Function Technical Manager

Signature

Issued: March 18, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                        |             |
|-------------------------------------|------------------------|-------------|
| <b>DASY Version</b>                 | DASY5                  | V52.8.5     |
| <b>Extrapolation</b>                | Advanced Extrapolation |             |
| <b>Phantom</b>                      | Modular Flat Phantom   |             |
| <b>Distance Dipole Center - TSL</b> | 15 mm                  | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm      |             |
| <b>Frequency</b>                    | 750 MHz $\pm$ 1 MHz    |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 41.9           | 0.89 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 41.1 $\pm$ 6 % | 0.92 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 2.19 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>8.50 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 1.42 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>5.55 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Body TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Body TSL parameters</b>             | 22.0 °C             | 55.5           | 0.96 mho/m           |
| <b>Measured Body TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 54.2 $\pm$ 6 % | 1.00 mho/m $\pm$ 6 % |
| <b>Body TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 2.26 W/kg                                      |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>8.72 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 1.48 W/kg                                      |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>5.75 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 54.4 $\Omega$ - 0.9 j $\Omega$ |
| Return Loss                          | - 27.2 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 49.7 $\Omega$ - 2.7 j $\Omega$ |
| Return Loss                          | - 31.4 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.034 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                   |
|-----------------|-------------------|
| Manufactured by | SPEAG             |
| Manufactured on | November 08, 2011 |

## DASY5 Validation Report for Head TSL

Date: 18.03.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1054**

Communication System: CW; Frequency: 750 MHz

Medium parameters used:  $f = 750 \text{ MHz}$ ;  $\sigma = 0.92 \text{ S/m}$ ;  $\epsilon_r = 41.1$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.28, 6.28, 6.28); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.5(1059); SEMCAD X 14.6.8(7028)

### **Dipole Calibration for Head Tissue/ $P_{in}=250 \text{ mW}$ , $d=15\text{mm}$ /Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value =  $52.772 \text{ V/m}$ ; Power Drift =  $0.03 \text{ dB}$

Peak SAR (extrapolated) =  $3.33 \text{ W/kg}$

**SAR(1 g) =  $2.19 \text{ W/kg}$ ; SAR(10 g) =  $1.42 \text{ W/kg}$**

Maximum value of SAR (measured) =  $2.55 \text{ W/kg}$

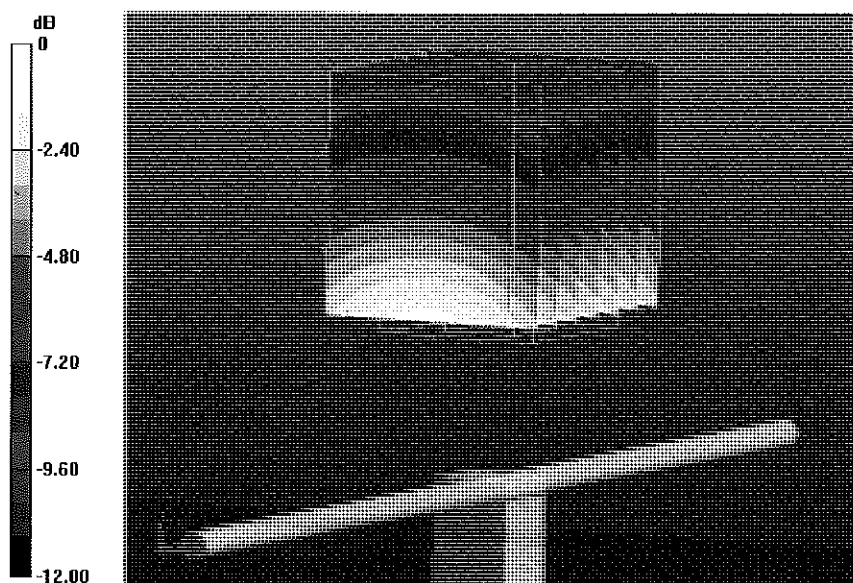


0 dB =  $2.55 \text{ W/kg}$  =  $4.07 \text{ dBW/kg}$

# Impedance Measurement Plot for Head TSL


18 Mar 2013 13:14:09  
**CH1** S11 1 U FS 1: 54.449  $\Omega$  -917.97 m $\Omega$  231.17 pF 750.000 000 MHz

\*  
 Del  
 CA  
 Avg  
 16  
 H1 d

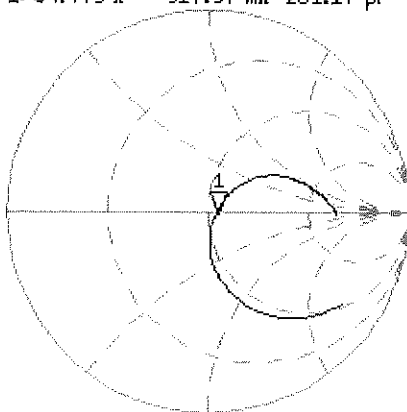

CH2 S11 LOG 5 dB/REF -20 dB 1:-27.227 dB 750.000 000 MHz

CA  
 Avg  
 16  
 H1 d

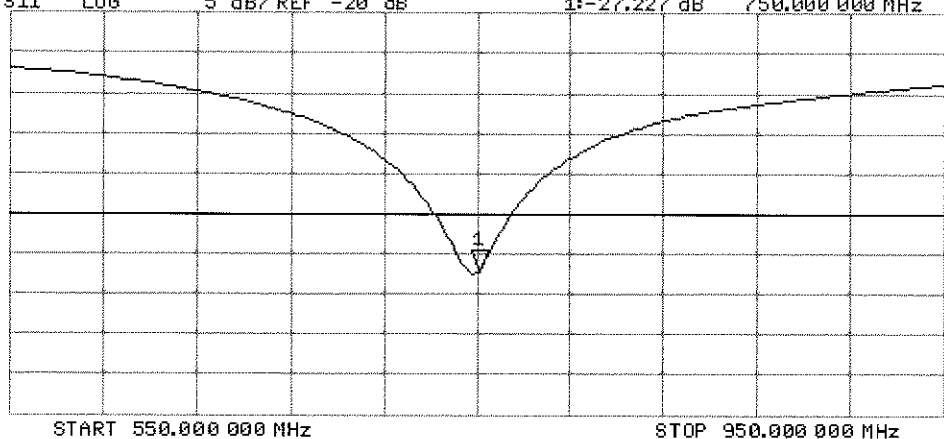

## DASY5 Validation Report for Body TSL

Date: 18.03.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1054**

Communication System: CW; Frequency: 750 MHz

Medium parameters used:  $f = 750 \text{ MHz}$ ;  $\sigma = 1 \text{ S/m}$ ;  $\epsilon_r = 54.2$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.11, 6.11, 6.11); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.5(1059); SEMCAD X 14.6.8(7028)

### **Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 52.772 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.32 W/kg

**SAR(1 g) = 2.26 W/kg; SAR(10 g) = 1.48 W/kg**


Maximum value of SAR (measured) = 2.61 W/kg

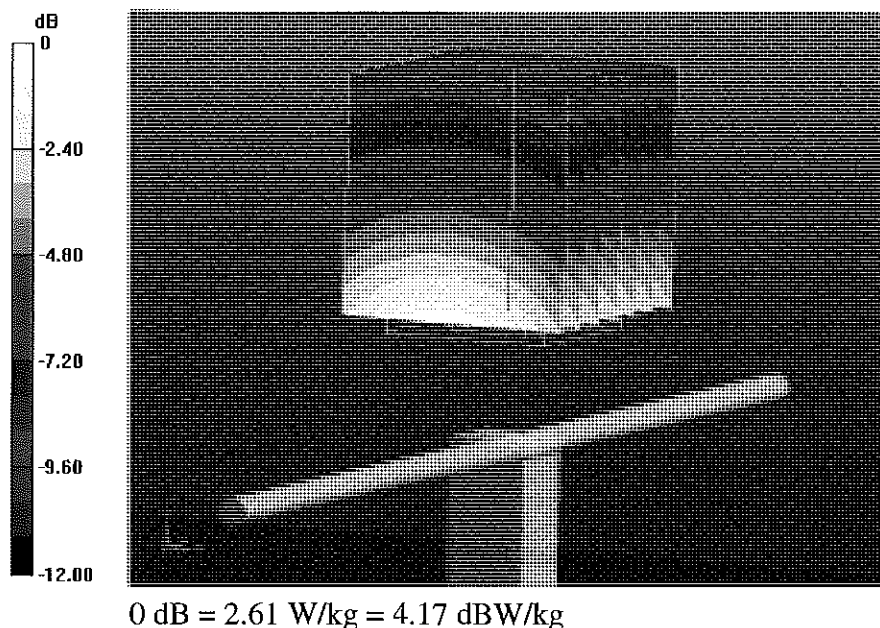

# Impedance Measurement Plot for Body TSL

18 Mar 2013 12:24:11  
 CH1 S11 1 U FS 1: 49.717  $\Delta$  -2.6553  $\Delta$  79.890 pF 750.000 000 MHz


\*  
 De1  
 CA

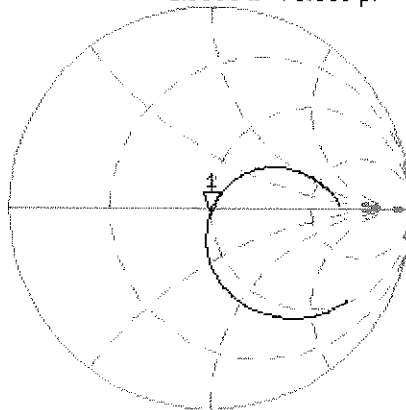

Av9  
 16  
 H1d

CH2 S11 LOG 5 dB/REF -20 dB 1: -31.444 dB 750.000 000 MHz

CA  
 Av9  
 16  
 H1d

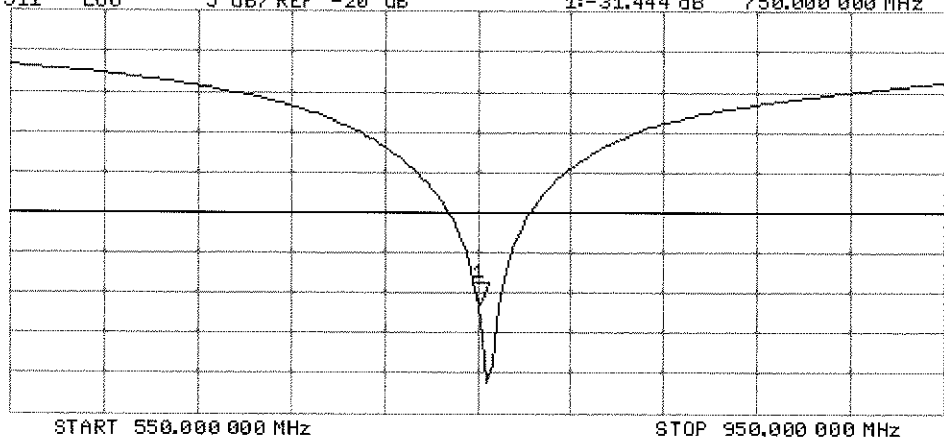



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D835V2-4d119\_Apr13**

## CALIBRATION CERTIFICATE

Object **D835V2 - SN: 4d119**

Calibration procedure(s) **QA CAL-05.v9**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **April 25, 2013**

✓  
KOK  
5/8/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 04-Apr-13 (No. 217-01736)         | Apr-14                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 04-Apr-13 (No. 217-01739)         | Apr-14                 |
| Reference Probe ES3DV3      | SN: 3205           | 28-Dec-12 (No. ES3-3205_Dec12)    | Dec-13                 |
| DAE4                        | SN: 909            | 11-Sep-12 (No. DAE4-909_Sep12)    | Sep-13                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

Calibrated by: **Claudio Leubler** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature

Issued: April 26, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### Additional Documentation:

- DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.6     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 15 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 835 MHz $\pm$ 1 MHz    |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 41.5           | 0.90 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 40.8 $\pm$ 6 % | 0.94 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 2.51 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 9.68 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 1.62 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 6.30 W/kg $\pm$ 16.5 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 55.2           | 0.97 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 54.0 $\pm$ 6 % | 1.01 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 2.47 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 9.54 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 1.62 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 6.31 W/kg $\pm$ 16.5 % (k=2) |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.1 $\Omega$ - 4.7 j $\Omega$ |
| Return Loss                          | - 26.6 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 45.8 $\Omega$ - 6.3 j $\Omega$ |
| Return Loss                          | - 22.1 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.385 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |               |
|-----------------|---------------|
| Manufactured by | SPEAG         |
| Manufactured on | June 29, 2010 |

## DASY5 Validation Report for Head TSL

Date: 25.04.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d119**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.94$  S/m;  $\epsilon_r = 40.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.05, 6.05, 6.05); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 11.09.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

### **Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.387 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.86 W/kg

**SAR(1 g) = 2.51 W/kg; SAR(10 g) = 1.62 W/kg**

Maximum value of SAR (measured) = 2.93 W/kg

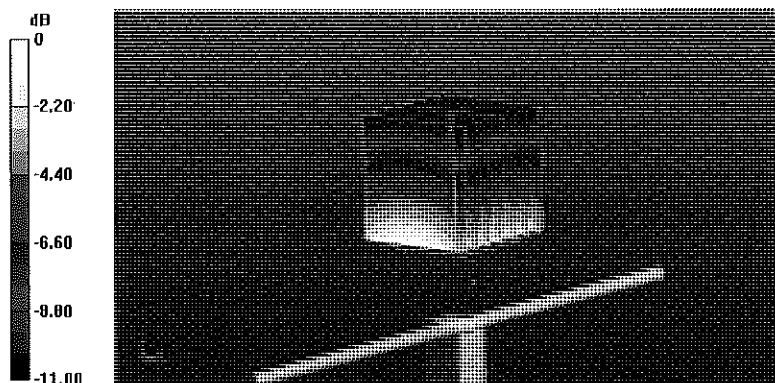

0 dB = 2.93 W/kg = 4.67 dBW/kg

# Impedance Measurement Plot for Head TSL

25 Apr 2013 09:11:06  
 CH1 S11 1 U FS 1: 50.061  $\Omega$  -4.6621  $\Omega$  40.884 pF 835.000 000 MHz


\*

Del

CA

Avg  
16

H1 d

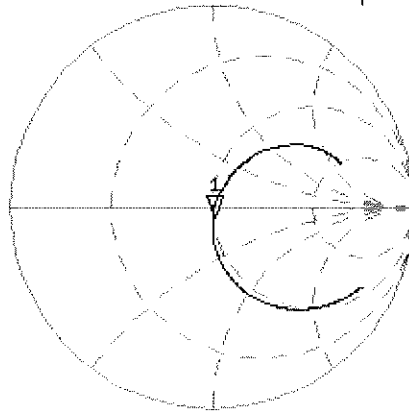


CH2 S11 LOG 5 dB/REF -20 dB 1:-26.641 dB 835.000 000 MHz

CA

Avg  
16

H1 d

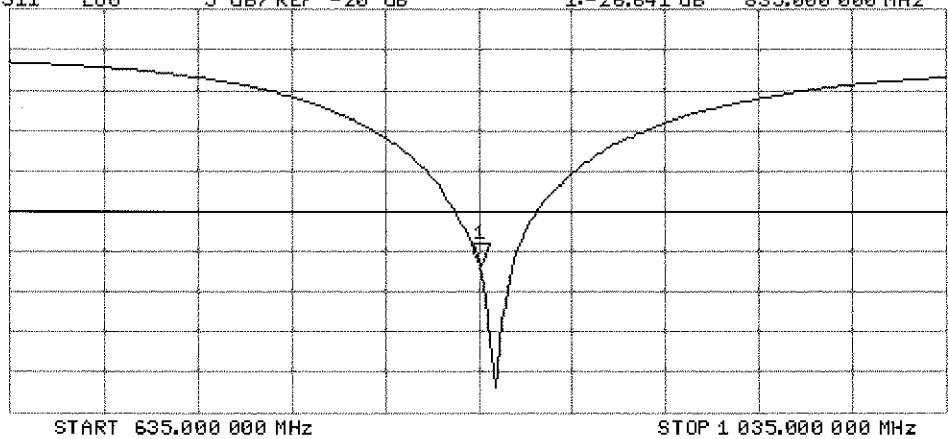

## DASY5 Validation Report for Body TSL

Date: 24.04.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d119**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 1.01 \text{ S/m}$ ;  $\epsilon_r = 54$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.04, 6.04, 6.04); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 11.09.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.178 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.68 W/kg


**SAR(1 g) = 2.47 W/kg; SAR(10 g) = 1.62 W/kg**

Maximum value of SAR (measured) = 2.89 W/kg

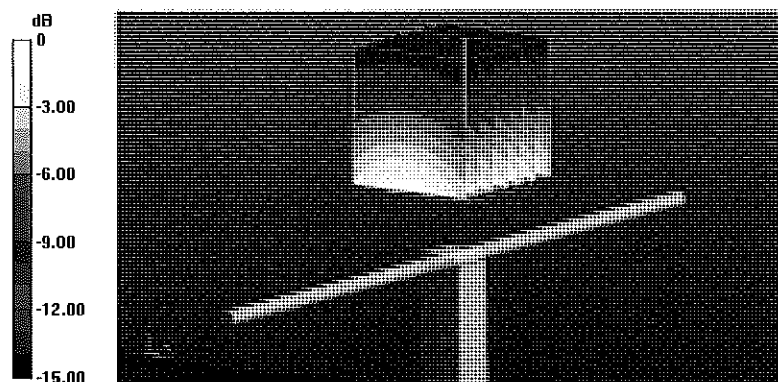

0 dB = 2.89 W/kg = 4.61 dBW/kg

Impedance Measurement Plot for Body TSL

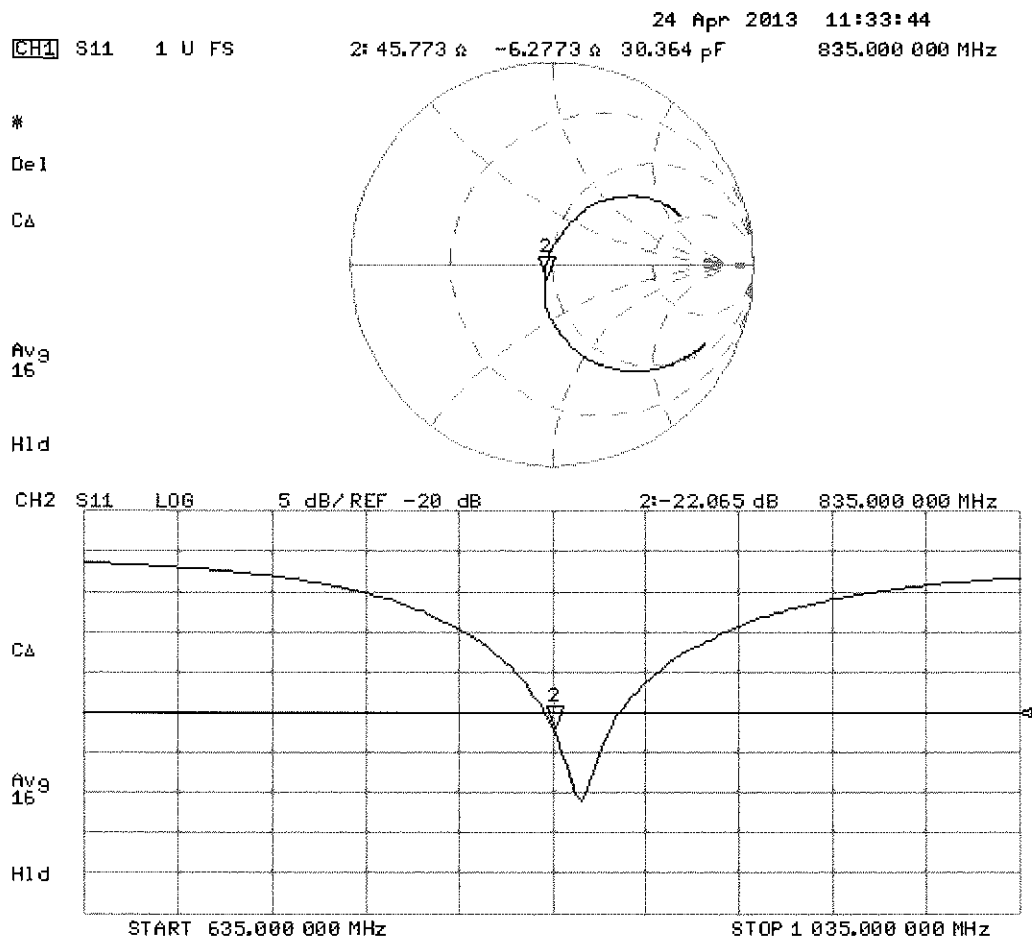



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D835V2-4d133\_Jul13**

## CALIBRATION CERTIFICATE

Object **D835V2 - SN: 4d133**

Calibration procedure(s) **QA CAL-05.v9  
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **July 17, 2013**

✓  
KOK  
8/12/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Power sensor HP 8481A       | US37292783         | 01-Nov-12 (No. 217-01640)         | Oct-13                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 04-Apr-13 (No. 217-01736)         | Apr-14                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 04-Apr-13 (No. 217-01739)         | Apr-14                 |
| Reference Probe ES3DV3      | SN: 3205           | 28-Dec-12 (No. ES3-3205_Dec12)    | Dec-13                 |
| DAE4                        | SN: 601            | 25-Apr-13 (No. DAE4-601_Apr13)    | Apr-14                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                |               |                       |           |
|----------------|---------------|-----------------------|-----------|
|                | Name          | Function              | Signature |
| Calibrated by: | Leif Klysner  | Laboratory Technician |           |
| Approved by:   | Katja Pokovic | Technical Manager     |           |

Issued: July 18, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.7     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 15 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 835 MHz $\pm$ 1 MHz    |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 41.5           | 0.90 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 41.8 $\pm$ 6 % | 0.92 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 2.44 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>9.62 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 1.59 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>6.28 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 55.2           | 0.97 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 54.9 $\pm$ 6 % | 1.00 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b> | Condition          |                                                |
| SAR measured                                                | 250 mW input power | 2.46 W/kg                                      |
| SAR for nominal Body TSL parameters                         | normalized to 1W   | <b>9.61 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b> | condition          |                                                |
| SAR measured                                                  | 250 mW input power | 1.62 W/kg                                      |
| SAR for nominal Body TSL parameters                           | normalized to 1W   | <b>6.36 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 52.0 $\Omega$ - 1.8 j $\Omega$ |
| Return Loss                          | - 31.8 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.2 $\Omega$ - 3.6 j $\Omega$ |
| Return Loss                          | - 27.7 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.395 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |               |
|-----------------|---------------|
| Manufactured by | SPEAG         |
| Manufactured on | July 22, 2011 |

## DASY5 Validation Report for Head TSL

Date: 17.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d133**

Communication System: UID 0 - CW ; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.92 \text{ S/m}$ ;  $\epsilon_r = 41.8$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.05, 6.05, 6.05); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

### **Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 57.188 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.66 W/kg

**SAR(1 g) = 2.44 W/kg; SAR(10 g) = 1.59 W/kg**

Maximum value of SAR (measured) = 2.84 W/kg

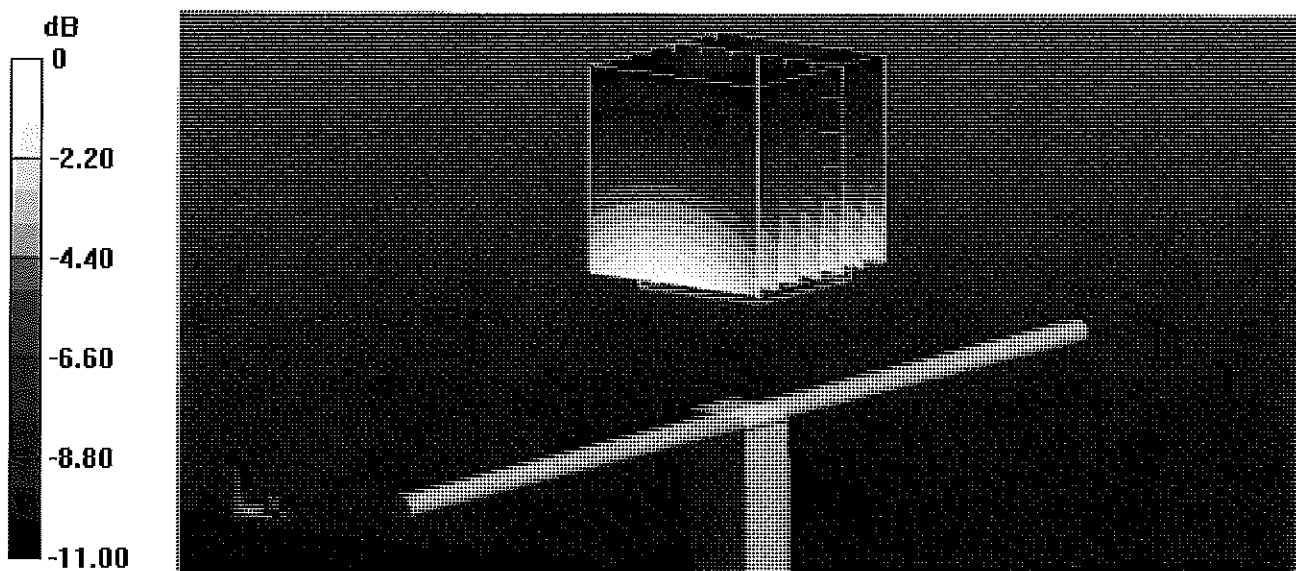


0 dB = 2.84 W/kg = 4.53 dBW/kg

Impedance Measurement Plot for Head TSL


18 Jul 2013 09:49:17  
[CH1] S11 1 U FS 1: 51.957  $\angle$  -1.7539  $\angle$  108.67 pF 835.000 000 MHz

\*  
De1  
CA  
Avg  
16  
H1d

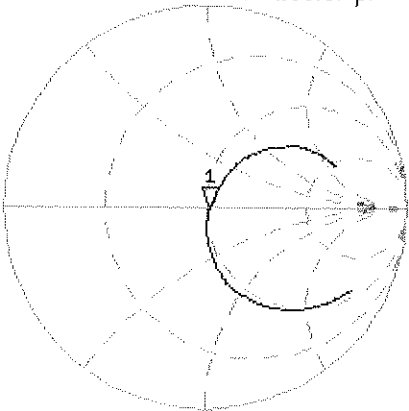

CH2 S11 L00 5 dB/REF -20 dB 1:-31.772 dB 835.000 000 MHz

CA  
Avg  
16  
H1d

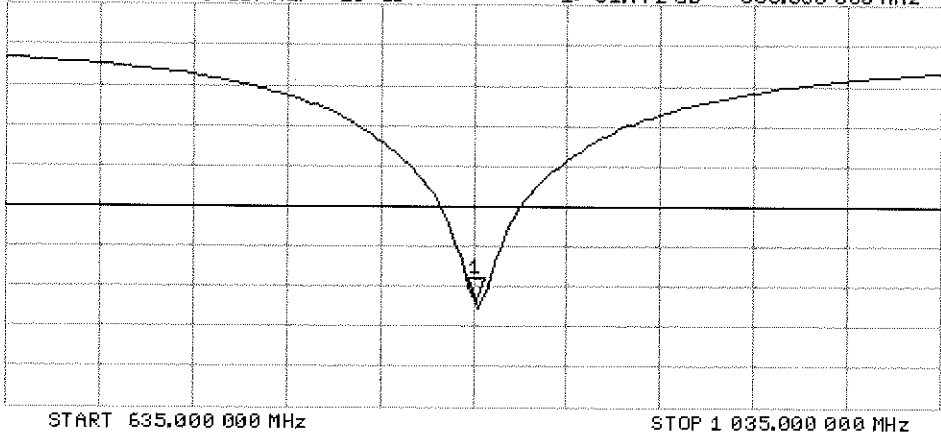

## DASY5 Validation Report for Body TSL

Date: 17.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d133**

Communication System: UID 0 - CW ; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 1 \text{ S/m}$ ;  $\epsilon_r = 54.9$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.04, 6.04, 6.04); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

### **Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 55.351 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.59 W/kg

**SAR(1 g) = 2.46 W/kg; SAR(10 g) = 1.62 W/kg**

Maximum value of SAR (measured) = 2.86 W/kg

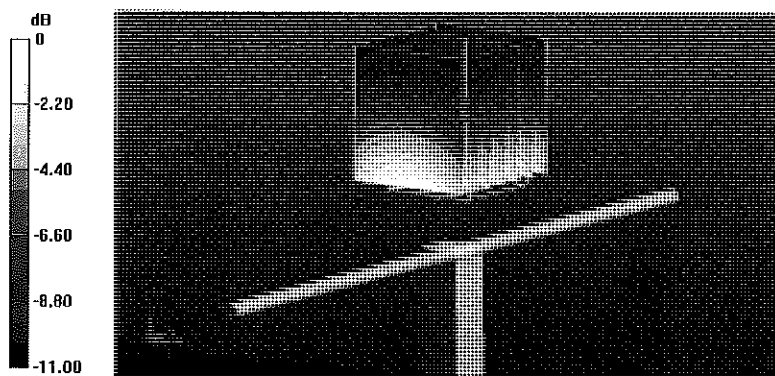


0 dB = 2.86 W/kg = 4.56 dBW/kg

# Impedance Measurement Plot for Body TSL

18 Jul 2013 09:11:04  
 CH1 S11 1 U FS 1: 48.184  $\Omega$  -3.6035  $\Omega$  52.894 pF 835.000 000 MHz

\*  
 Del  
 CA

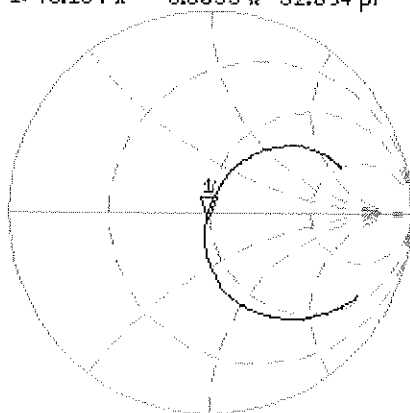

Avg  
 16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 1: -27.734 dB 835.000 000 MHz

CA

Avg  
 16

H1d

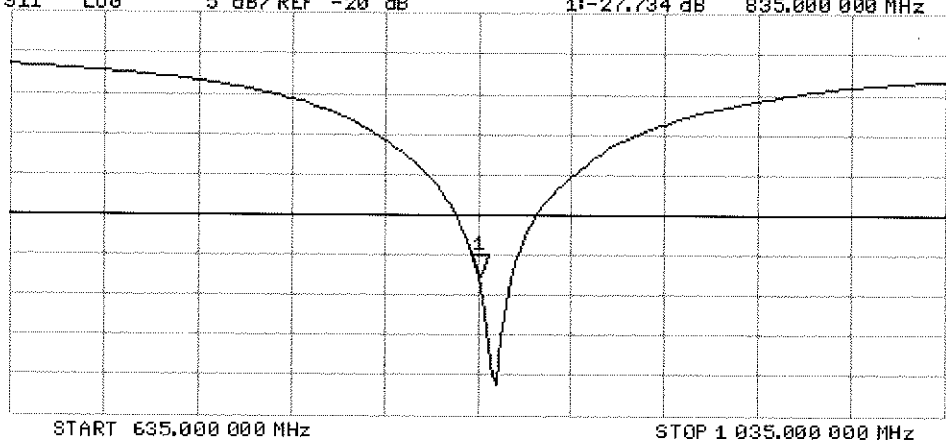



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D2450V2-719\_Aug12**

## CALIBRATION CERTIFICATE

Object **D2450V2 - SN: 719**

Calibration procedure(s) **QA CAL-05.v8**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **August 23, 2012**

✓ KOK  
9/17/12

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 05-Oct-11 (No. 217-01451)         | Oct-12                 |
| Power sensor HP 8481A       | US37292783         | 05-Oct-11 (No. 217-01451)         | Oct-12                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 27-Mar-12 (No. 217-01530)         | Apr-13                 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 27-Mar-12 (No. 217-01533)         | Apr-13                 |
| Reference Probe ES3DV3      | SN: 3205           | 30-Dec-11 (No. ES3-3205_Dec11)    | Dec-12                 |
| DAE4                        | SN: 601            | 27-Jun-12 (No. DAE4-601_Jun12)    | Jun-13                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-11) | In house check: Oct-12 |

Calibrated by: **Israe El-Naouq**      Name: **Israe El-Naouq**      Function: **Laboratory Technician**

Approved by: **Katja Pokovic**      Technical Manager

Signature

*Israe El-Naouq*  
*Katja Pokovic*

Issued: August 23, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.2     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 2450 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 39.2           | 1.80 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 39.2 $\pm$ 6 % | 1.81 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                       |                    |                                |
|-------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                |
| SAR measured                                          | 250 mW input power | 13.2 mW / g                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 52.7 mW / g $\pm$ 17.0 % (k=2) |

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                |
| SAR measured                                            | 250 mW input power | 6.19 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.7 mW / g $\pm$ 16.5 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 52.7           | 1.95 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 51.3 $\pm$ 6 % | 1.99 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                       |                    |                                |
|-------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                |
| SAR measured                                          | 250 mW input power | 13.1 mW / g                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 51.6 mW / g $\pm$ 17.0 % (k=2) |

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                |
| SAR measured                                            | 250 mW input power | 6.16 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 24.4 mW / g $\pm$ 16.5 % (k=2) |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $54.4 \Omega + 3.8 j\Omega$ |
| Return Loss                          | - 25.1 dB                   |

### Antenna Parameters with Body TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $50.7 \Omega + 5.9 j\Omega$ |
| Return Loss                          | - 24.6 dB                   |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.150 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                    |
|-----------------|--------------------|
| Manufactured by | SPEAG              |
| Manufactured on | September 10, 2002 |

## DASY5 Validation Report for Head TSL

Date: 23.08.2012

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 719**

Communication System: CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.81$  mho/m;  $\epsilon_r = 39.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 99.219 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 26.633 mW/g

**SAR(1 g) = 13.2 mW/g; SAR(10 g) = 6.19 mW/g**

Maximum value of SAR (measured) = 16.5 W/kg

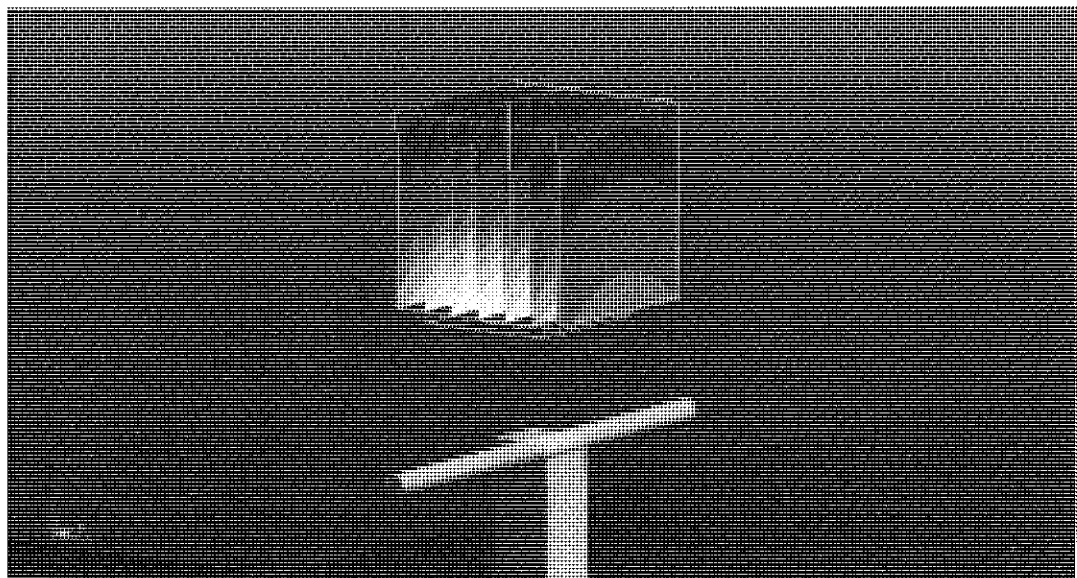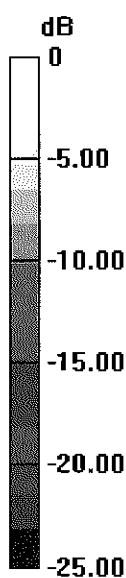


0 dB = 16.5 W/kg = 24.35 dB W/kg

# Impedance Measurement Plot for Head TSL

22 Aug 2012 15:39:08  
 CH1 S11 1 U FS 3: 54.416  $\Omega$  3.7656  $\Omega$  244.62 pH 2 450.000 000 MHz

\*  
 Del  
 CA

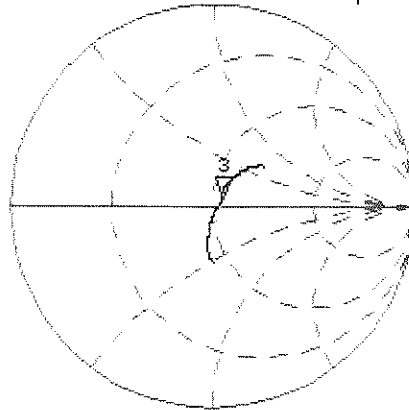

Avg  
 16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 3: -25.109 dB 2 450.000 000 MHz

CA

Avg  
 16

H1d

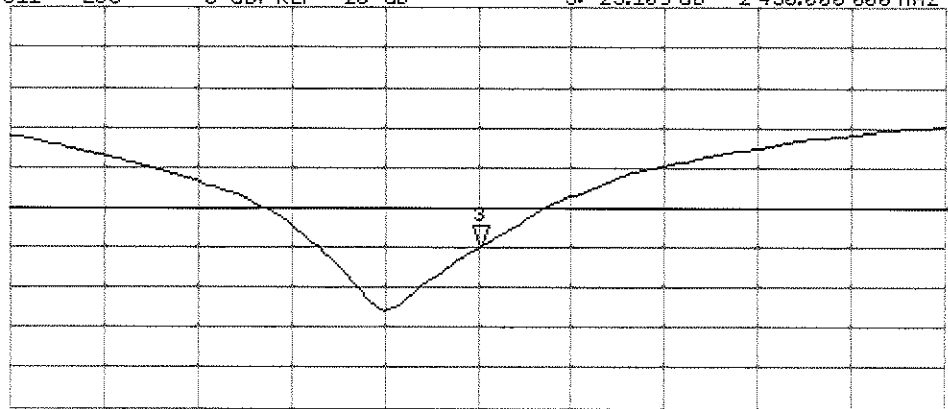

START 2 250.000 000 MHz

STOP 2 650.000 000 MHz

## DASY5 Validation Report for Body TSL

Date: 22.08.2012

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 719**

Communication System: CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 51.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.26, 4.26, 4.26); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.970 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 26.692 mW/g

**SAR(1 g) = 13.1 mW/g; SAR(10 g) = 6.16 mW/g**

Maximum value of SAR (measured) = 17.1 W/kg

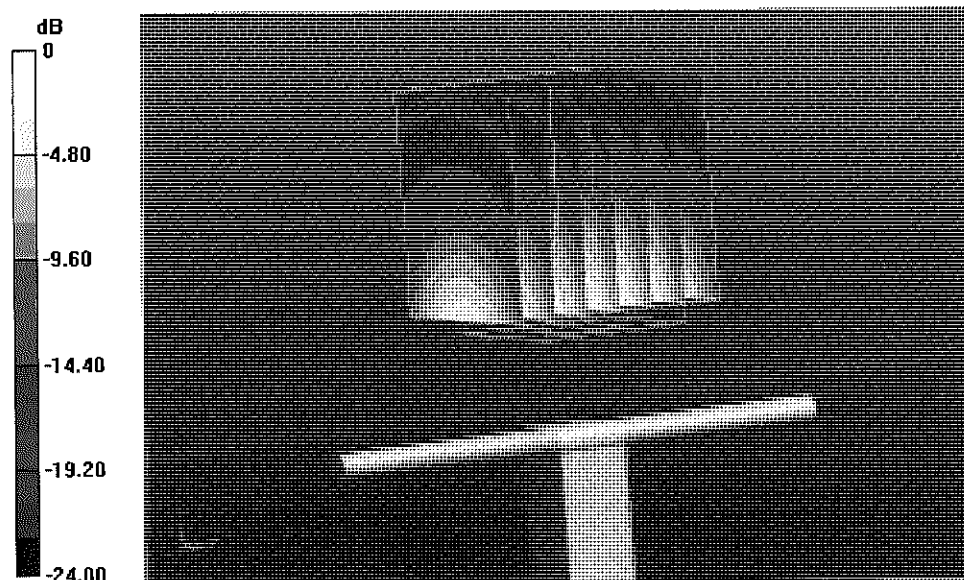


0 dB = 17.1 W/kg = 24.66 dB W/kg

Impedance Measurement Plot for Body TSL


22 Aug 2012 15:38:22  
[CH1] S11 1 U FS 3: 50.709  $\Omega$  5.8906  $\Omega$  382.66 pF 2 450.000 000 MHz

\*  
Del  
CA  
Avg  
16  
H1d

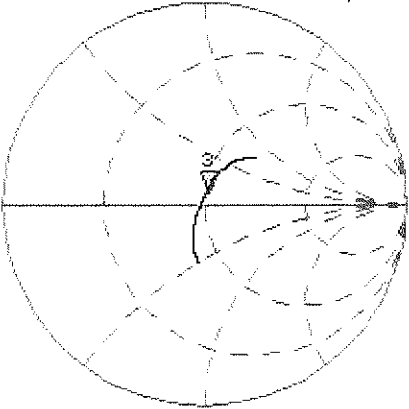

CH2 S11 LOG 5 dB/REF -20 dB 3:-24.605 dB 2 450.000 000 MHz

CA  
Avg  
16  
H1d

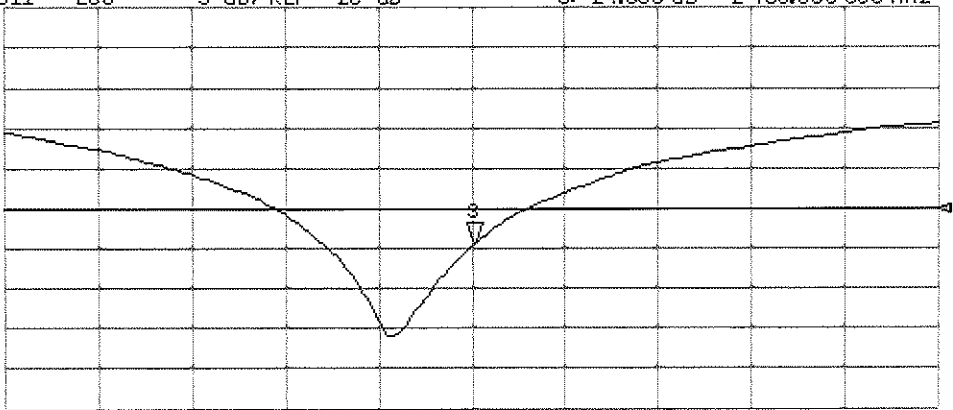

START 2 250.000 000 MHz STOP 2 650.000 000 MHz



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Client **PC Test**

Certificate No: **ES3-3318\_Apr13**

## CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3318**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-23.v4, QA CAL-25.v4**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **April 29, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 28-Dec-12 (No. ES3-3013_Dec12)    | Dec-13                 |
| DAE4                       | SN: 660         | 31-Jan-13 (No. DAE4-660_Jan13)    | Jan-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-15 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                                                                                                                 | Name          | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|---------------|-----------------------|-----------|
| Calibrated by:                                                                                                  | Dimce Iliev   | Laboratory Technician |           |
| Approved by:                                                                                                    | Katja Pokovic | Technical Manager     |           |
| Issued: April 29, 2013                                                                                          |               |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |               |                       |           |





Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C, D               | modulation dependent linearization parameters                                                                                                           |
| Polarization $\phi$      | $\phi$ rotation around probe axis                                                                                                                       |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

# Probe ES3DV3

## SN:3318

Manufactured: January 10, 2012  
Calibrated: April 29, 2013

**Calibrated for DASY/EASY Systems**  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3318

### Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|-----------------------------------------------------------|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 1.15     | 0.92     | 1.29     | ± 10.1 %  |
| DCP (mV) <sup>B</sup>                                     | 102.6    | 105.4    | 100.8    |           |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB/ $\mu\text{V}$ | C   | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----|---------------------------|---|---------|------------------------|-----|---------|----------|---------------------------|
| 0   | CW                        | X | 0.0     | 0.0                    | 1.0 | 0.00    | 153.6    | ±3.5 %                    |
|     |                           | Y | 0.0     | 0.0                    | 1.0 |         | 133.8    |                           |
|     |                           | Z | 0.0     | 0.0                    | 1.0 |         | 154.8    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3318

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 41.9                               | 0.89                            | 6.59    | 6.59    | 6.59    | 0.25  | 2.12       | ± 12.0 %    |
| 850                  | 41.5                               | 0.92                            | 6.33    | 6.33    | 6.33    | 0.57  | 1.25       | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 5.22    | 5.22    | 5.22    | 0.79  | 1.25       | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 4.59    | 4.59    | 4.59    | 0.80  | 1.30       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3318

### Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 55.5                               | 0.96                            | 6.35    | 6.35    | 6.35    | 0.53  | 1.42       | ± 12.0 %    |
| 850                  | 55.2                               | 0.99                            | 6.21    | 6.21    | 6.21    | 0.57  | 1.38       | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 4.79    | 4.79    | 4.79    | 0.46  | 1.77       | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 4.31    | 4.31    | 4.31    | 0.80  | 1.09       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

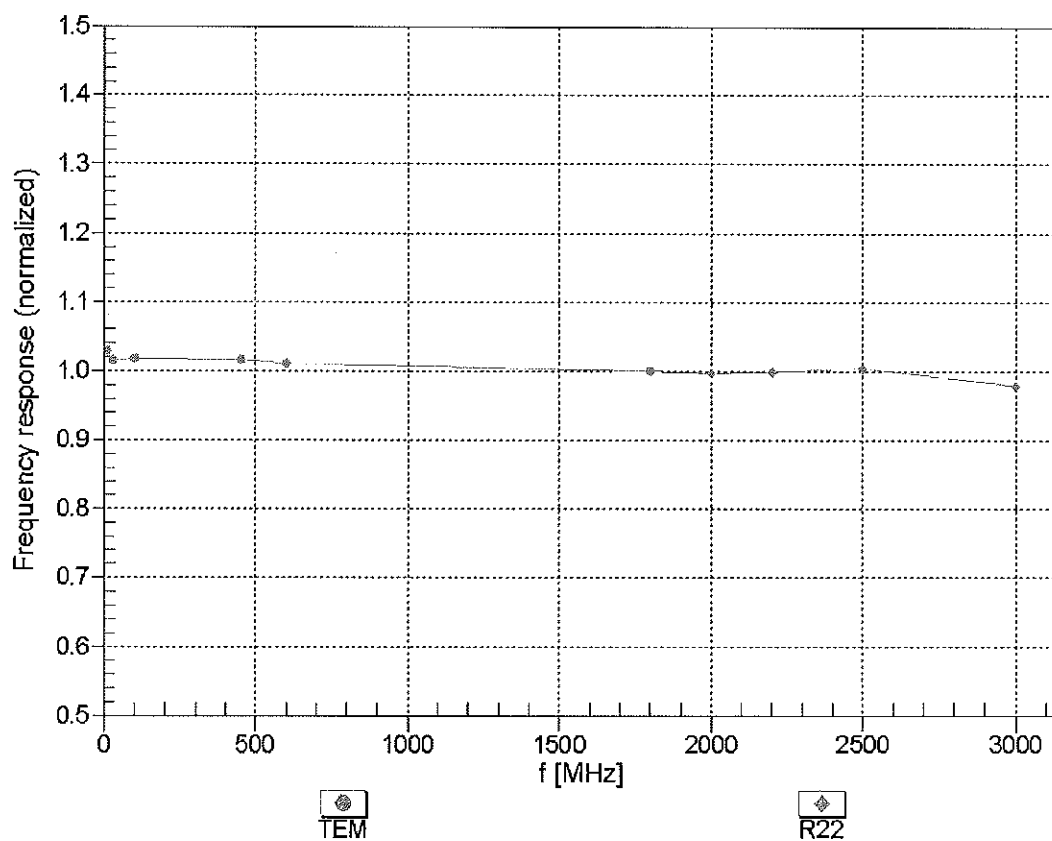



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)

## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

f=600 MHz, TEM

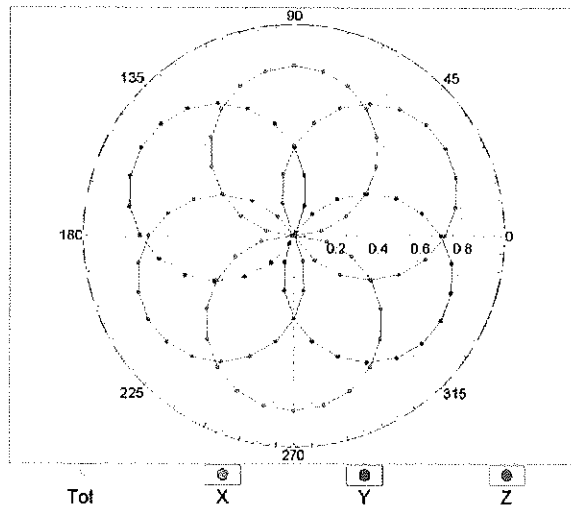


f=1800 MHz, R22

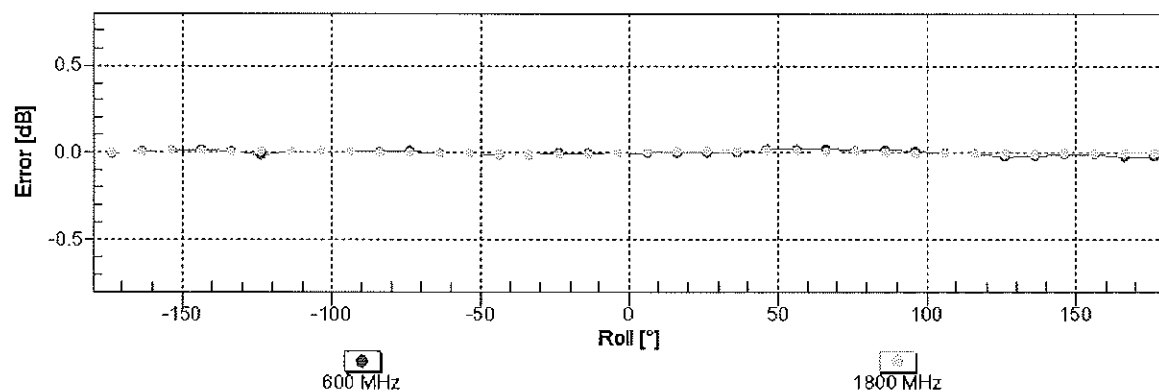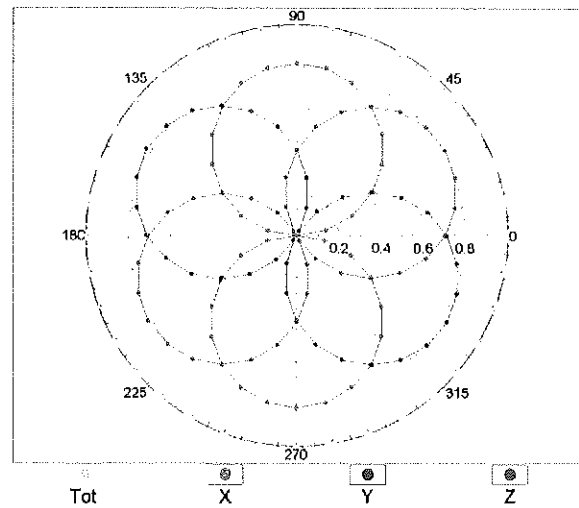

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )


# Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f = 900 \text{ MHz}$ )

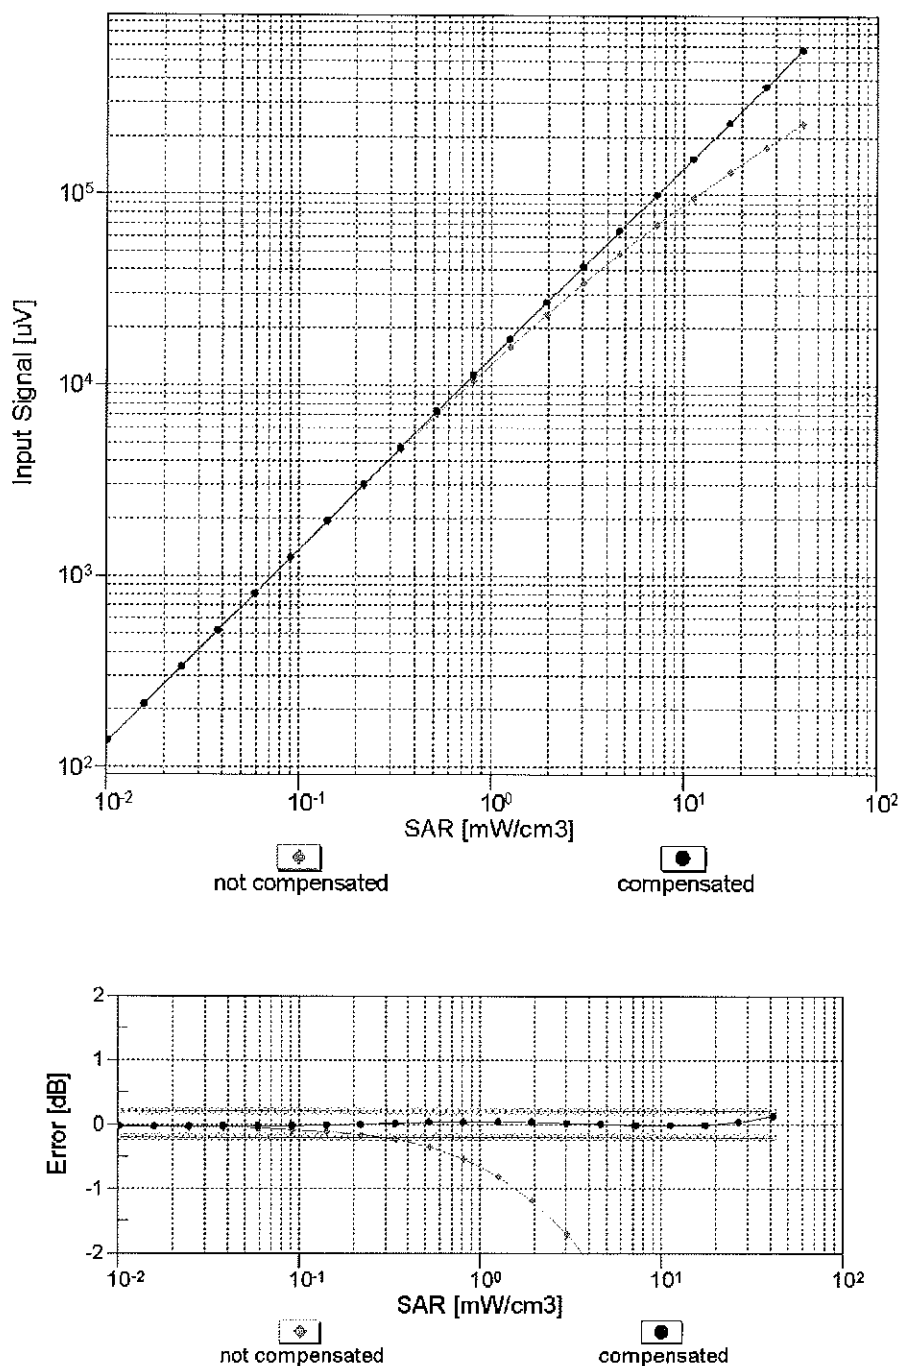

Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )





## Conversion Factor Assessment

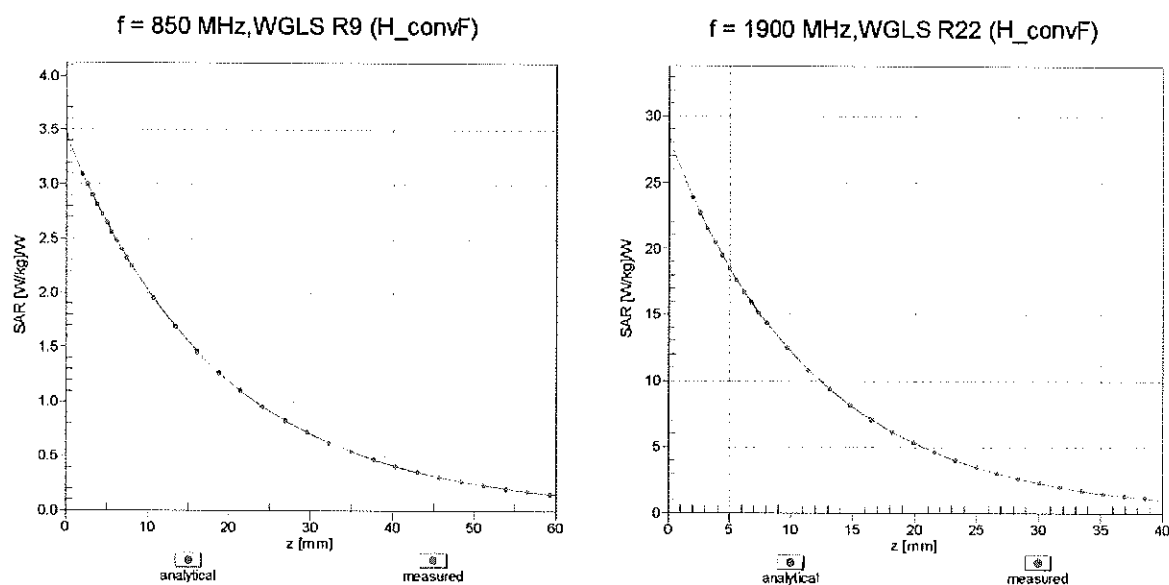

## Deviation from Isotropy in Liquid

Error ( $\phi$ ,  $\theta$ ),  $f = 900 \text{ MHz}$

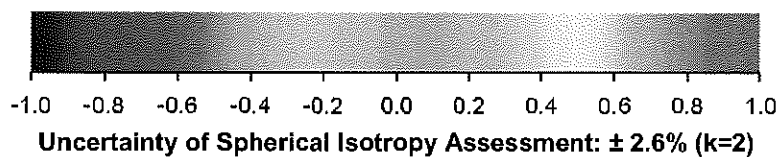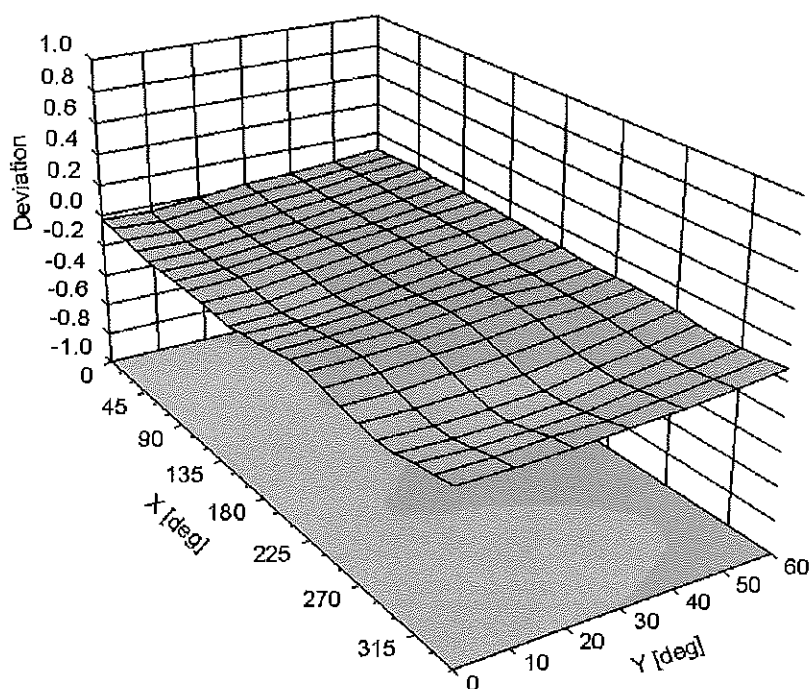

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3318

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -103.8     |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 10 mm      |
| Tip Diameter                                  | 4 mm       |
| Probe Tip to Sensor X Calibration Point       | 2 mm       |
| Probe Tip to Sensor Y Calibration Point       | 2 mm       |
| Probe Tip to Sensor Z Calibration Point       | 2 mm       |
| Recommended Measurement Distance from Surface | 3 mm       |

## **Additional Conversion Factors**

**for Dosimetric E-Field Probe**

Type:

**ES3DV3**

Serial Number:

**3318**

Place of Assessment:

**Zurich**

Date of Assessment:

**June 19, 2013**


Probe Calibration Date:

**April 29, 2013**

✓  
Kox  
6/25/13

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. The evaluation is coupled with measured conversion factors (probe calibration date indicated above). The uncertainty of the numerical assessment is based on the extrapolation from measured value at 835 MHz or at 1900 MHz.

Assessed by:



## Dosimetric E-Field Probe ES3DV3 SN:3318

Conversion factor ( $\pm$  standard deviation)

1750  $\pm$  50 MHz      *ConvF*      5.59  $\pm$  7%

$\epsilon_r = 40.1 \pm 5\%$   
 $\sigma = 1.37 \pm 5\%$  mho/m  
(head tissue)

1750  $\pm$  50 MHz      *ConvF*      5.22  $\pm$  7%

$\epsilon_r = 53.4 \pm 5\%$   
 $\sigma = 1.49 \pm 5\%$  mho/m  
(body tissue)

### Important Note:

For numerically assessed probe conversion factors, parameters Alpha and Delta in the DASY software must have the following entries: Alpha = 0 and Delta = 1.

Please see also DASY Manual.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Client **PC Test**

Certificate No: **ES3-3319\_Apr13**

## CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3319**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-23.v4, QA CAL-25.v4**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **April 29, 2013**

VCC  
6/14/13

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 28-Dec-12 (No. ES3-3013_Dec12)    | Dec-13                 |
| DAE4                       | SN: 660         | 31-Jan-13 (No. DAE4-660_Jan13)    | Jan-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-15 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                                                                                                                 |                     |                                   |               |
|-----------------------------------------------------------------------------------------------------------------|---------------------|-----------------------------------|---------------|
| Calibrated by:                                                                                                  | Name<br>Dimce Iliev | Function<br>Laboratory Technician | Signature<br> |
| Approved by:                                                                                                    | Katja Pokovic       | Technical Manager                 |               |
| Issued: April 29, 2013                                                                                          |                     |                                   |               |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |                     |                                   |               |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C, D               | modulation dependent linearization parameters                                                                                                           |
| Polarization $\phi$      | $\phi$ rotation around probe axis                                                                                                                       |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

# Probe ES3DV3

## SN:3319

Manufactured: January 10, 2012  
Calibrated: April 29, 2013

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

### Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|-----------------------------------------------------------|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 1.12     | 1.20     | 1.22     | ± 10.1 %  |
| DCP (mV) <sup>B</sup>                                     | 100.7    | 102.6    | 102.4    |           |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB/ $\mu\text{V}$ | C   | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----|---------------------------|---|---------|------------------------|-----|---------|----------|---------------------------|
| 0   | CW                        | X | 0.0     | 0.0                    | 1.0 | 0.00    | 152.0    | ±3.8 %                    |
|     |                           | Y | 0.0     | 0.0                    | 1.0 |         | 159.0    |                           |
|     |                           | Z | 0.0     | 0.0                    | 1.0 |         | 149.8    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 41.9                               | 0.89                            | 6.49    | 6.49    | 6.49    | 0.28  | 1.97       | ± 12.0 %    |
| 850                  | 41.5                               | 0.92                            | 6.23    | 6.23    | 6.23    | 0.42  | 1.57       | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 5.22    | 5.22    | 5.22    | 0.80  | 1.24       | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 4.57    | 4.57    | 4.57    | 0.80  | 1.32       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

### Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 55.5                               | 0.96                            | 6.30    | 6.30    | 6.30    | 0.45  | 1.53       | ± 12.0 %    |
| 850                  | 55.2                               | 0.99                            | 6.15    | 6.15    | 6.15    | 0.42  | 1.65       | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 4.85    | 4.85    | 4.85    | 0.63  | 1.49       | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 4.32    | 4.32    | 4.32    | 0.69  | 1.20       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

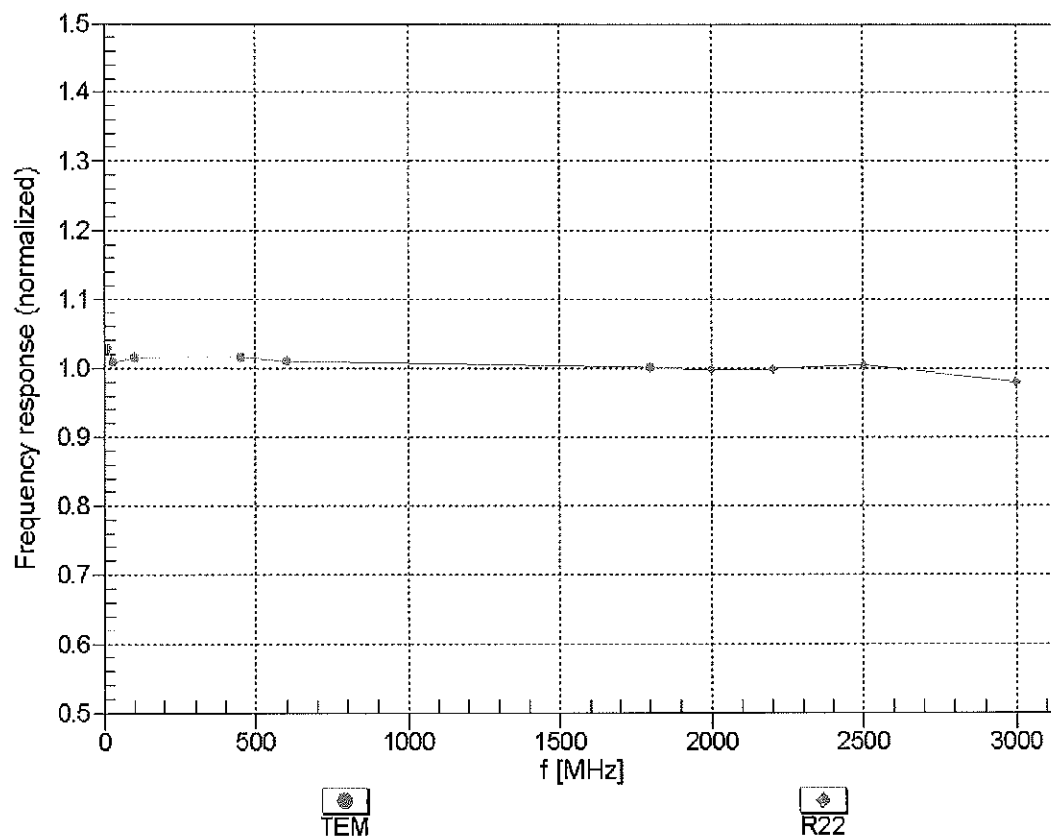



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$



f=600 MHz,TEM

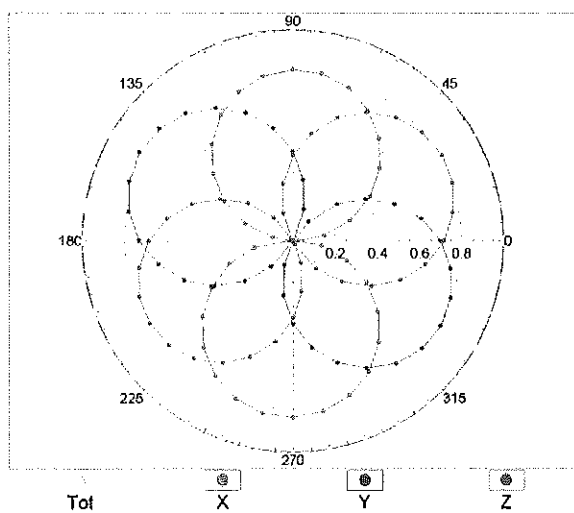

f=1800 MHz,R22

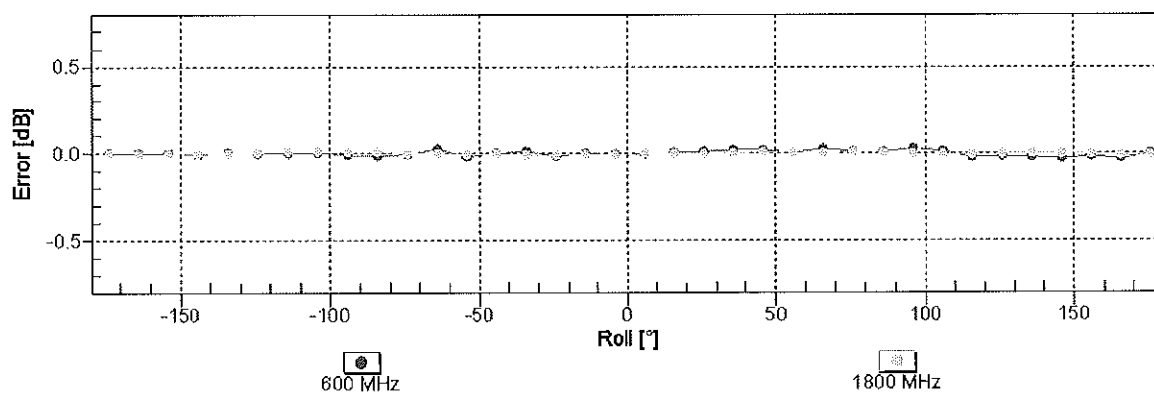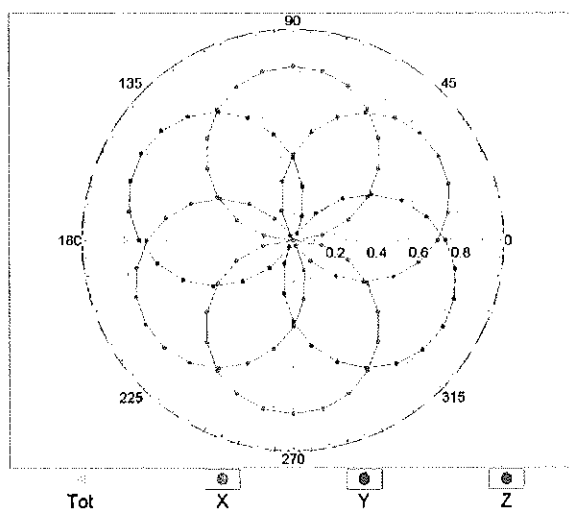
**Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )**

# Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f = 900 \text{ MHz}$ )

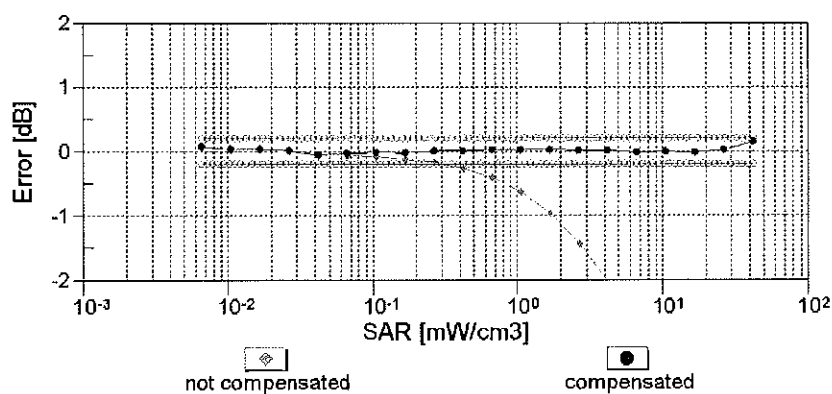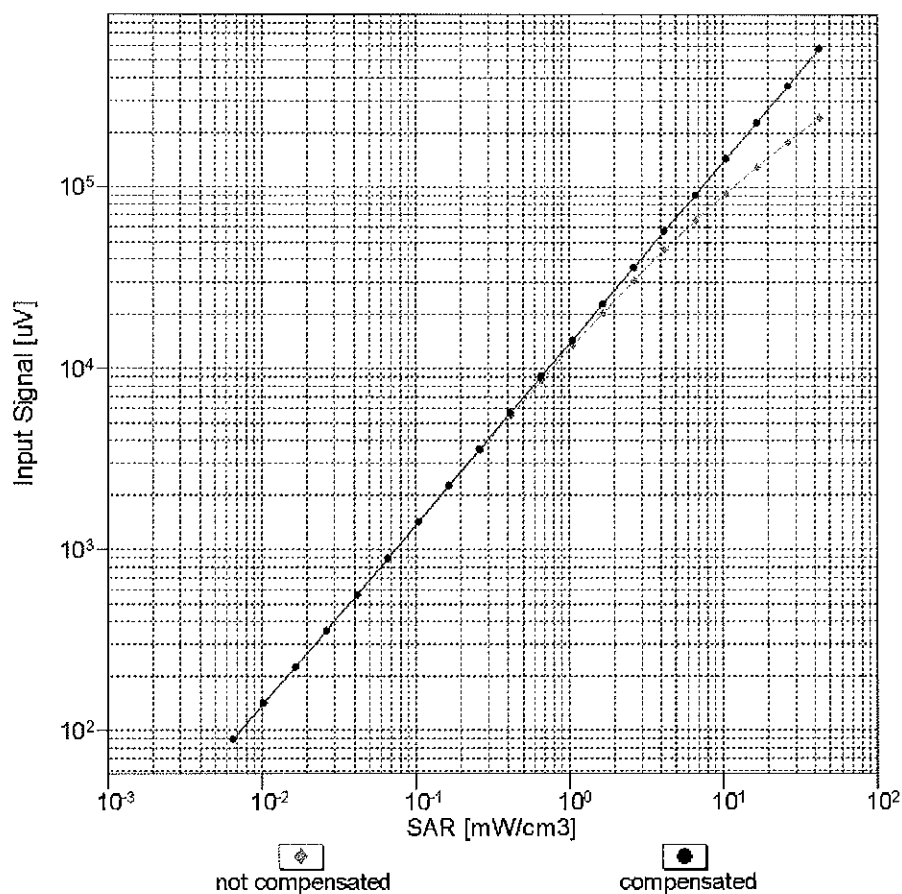



Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

## Conversion Factor Assessment

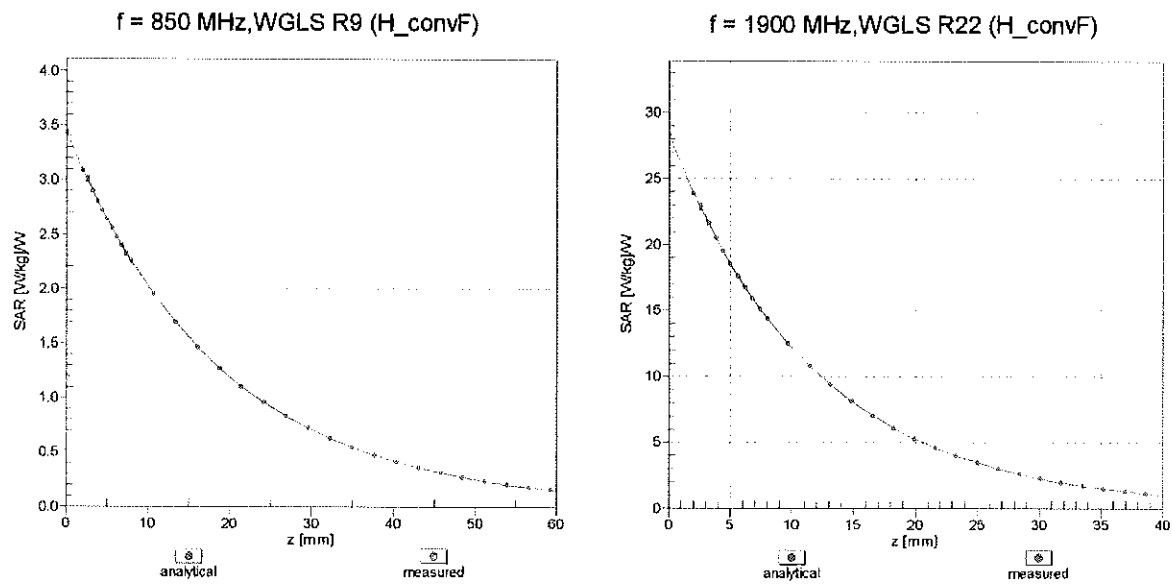

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

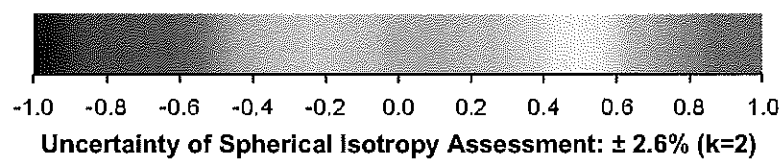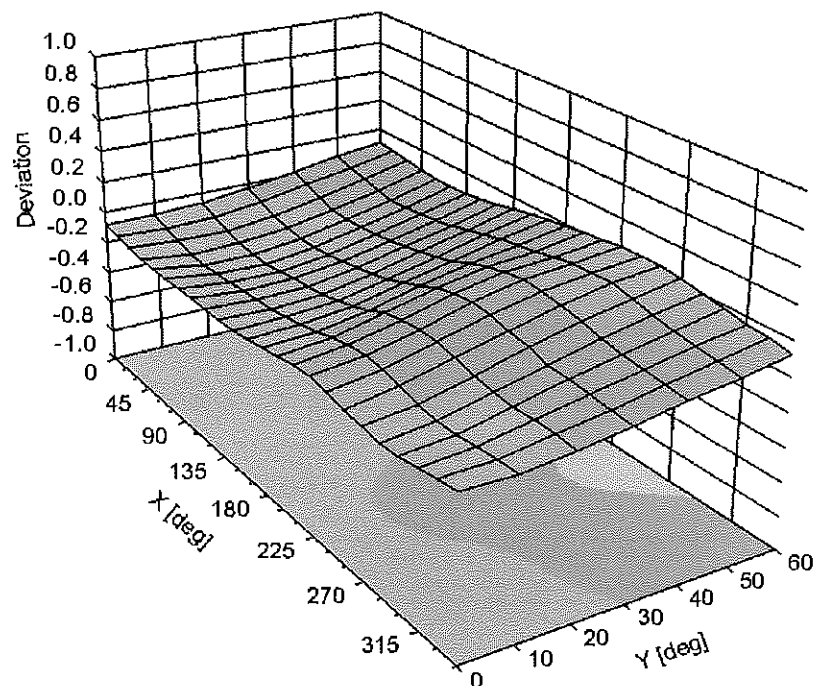

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -104.1     |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 10 mm      |
| Tip Diameter                                  | 4 mm       |
| Probe Tip to Sensor X Calibration Point       | 2 mm       |
| Probe Tip to Sensor Y Calibration Point       | 2 mm       |
| Probe Tip to Sensor Z Calibration Point       | 2 mm       |
| Recommended Measurement Distance from Surface | 3 mm       |

## **Additional Conversion Factors**

**for Dosimetric E-Field Probe**

Type:

**ES3DV3**

Serial Number:

**3319**

Place of Assessment:

**Zurich**

Date of Assessment:


**June 19, 2013**

Probe Calibration Date:

**April 29, 2013**

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. The evaluation is coupled with measured conversion factors (probe calibration date indicated above). The uncertainty of the numerical assessment is based on the extrapolation from measured value at 835 MHz or at 1900 MHz.

Assessed by:



✓  
KOK  
6/25/13



## Dosimetric E-Field Probe ES3DV3 SN:3319

Conversion factor ( $\pm$  standard deviation)

1750  $\pm$  50 MHz      *ConvF*      5.59  $\pm$  7 %

$\epsilon_r = 40.1 \pm 5\%$   
 $\sigma = 1.37 \pm 5\%$  mho/m  
(head tissue)

1750  $\pm$  50 MHz      *ConvF*      5.22  $\pm$  7 %

$\epsilon_r = 53.4 \pm 5\%$   
 $\sigma = 1.49 \pm 5\%$  mho/m  
(body tissue)

### Important Note:

For numerically assessed probe conversion factors, parameters Alpha and Delta in the DASY software must have the following entries: Alpha = 0 and Delta = 1.

Please see also DASY Manual.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Client **PC Test**

Certificate No: **ES3-3263\_May13**

## CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3263**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-23.v4, QA CAL-25.v4**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **May 16, 2013**

*✓ OK  
5/23/13*

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 28-Dec-12 (No. ES3-3013_Dec12)    | Dec-13                 |
| DAE4                       | SN: 660         | 31-Jan-13 (No. DAE4-660_Jan13)    | Jan-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-15 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                                                                                                                 | Name          | Function              | Signature            |
|-----------------------------------------------------------------------------------------------------------------|---------------|-----------------------|----------------------|
| Calibrated by:                                                                                                  | Leif Klysner  | Laboratory Technician | <i>Leif Klysner</i>  |
| Approved by:                                                                                                    | Katja Pokovic | Technical Manager     | <i>Katja Pokovic</i> |
| Issued: May 17, 2013                                                                                            |               |                       |                      |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |               |                       |                      |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C, D               | modulation dependent linearization parameters                                                                                                           |
| Polarization $\varphi$   | $\varphi$ rotation around probe axis                                                                                                                    |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* *frequency\_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

# Probe ES3DV3

## SN:3263

Manufactured: January 25, 2010  
Calibrated: May 16, 2013

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

### Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2)     |
|-----------------------------------------------------------|----------|----------|----------|---------------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 1.21     | 1.25     | 1.12     | $\pm 10.1 \%$ |
| DCP (mV) <sup>B</sup>                                     | 101.2    | 100.2    | 103.7    |               |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C   | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----|---------------------------|---|---------|------------------------------|-----|---------|----------|---------------------------|
| 0   | CW                        | X | 0.0     | 0.0                          | 1.0 | 0.00    | 156.5    | $\pm 2.5 \%$              |
|     |                           | Y | 0.0     | 0.0                          | 1.0 |         | 153.2    |                           |
|     |                           | Z | 0.0     | 0.0                          | 1.0 |         | 147.2    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 41.9                               | 0.89                            | 6.51    | 6.51    | 6.51    | 0.21  | 2.29       | ± 12.0 %    |
| 835                  | 41.5                               | 0.90                            | 6.29    | 6.29    | 6.29    | 0.50  | 1.38       | ± 12.0 %    |
| 1750                 | 40.1                               | 1.37                            | 5.30    | 5.30    | 5.30    | 0.45  | 1.54       | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 5.11    | 5.11    | 5.11    | 0.57  | 1.38       | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 4.47    | 4.47    | 4.47    | 0.59  | 1.49       | ± 12.0 %    |
| 2600                 | 39.0                               | 1.96                            | 4.31    | 4.31    | 4.31    | 0.80  | 1.28       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

### Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 55.5                               | 0.96                            | 6.37    | 6.37    | 6.37    | 0.34  | 1.82       | ± 12.0 %    |
| 835                  | 55.2                               | 0.97                            | 6.29    | 6.29    | 6.29    | 0.54  | 1.39       | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 5.01    | 5.01    | 5.01    | 0.72  | 1.27       | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 4.78    | 4.78    | 4.78    | 0.53  | 1.56       | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 4.33    | 4.33    | 4.33    | 0.80  | 1.14       | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 4.14    | 4.14    | 4.14    | 0.80  | 1.02       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

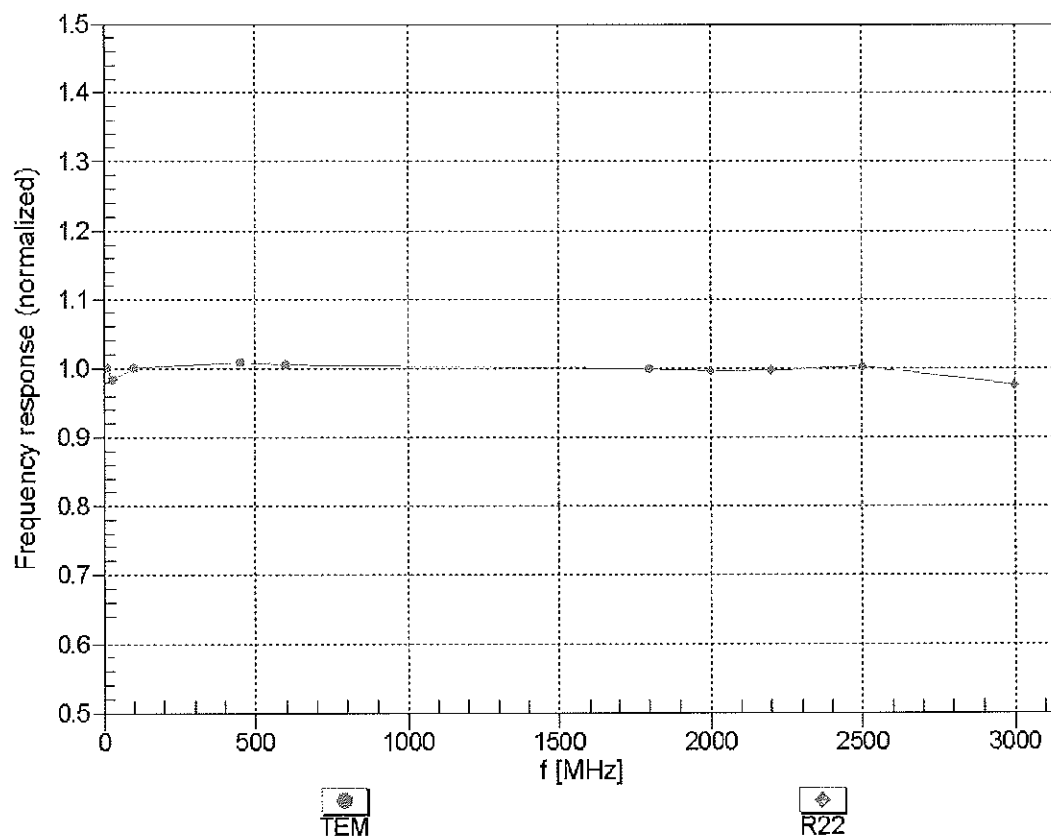


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)





## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

f=600 MHz,TEM

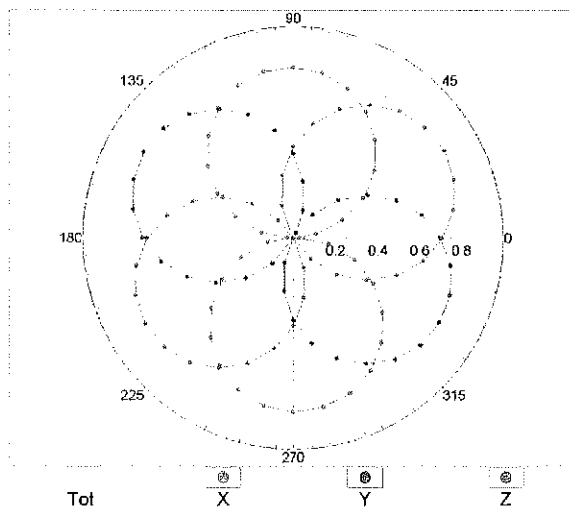


f=1800 MHz,R22

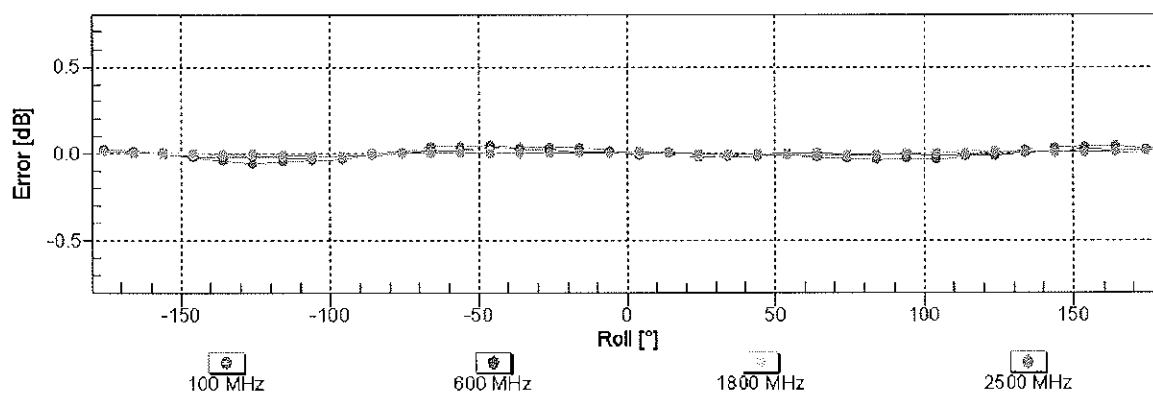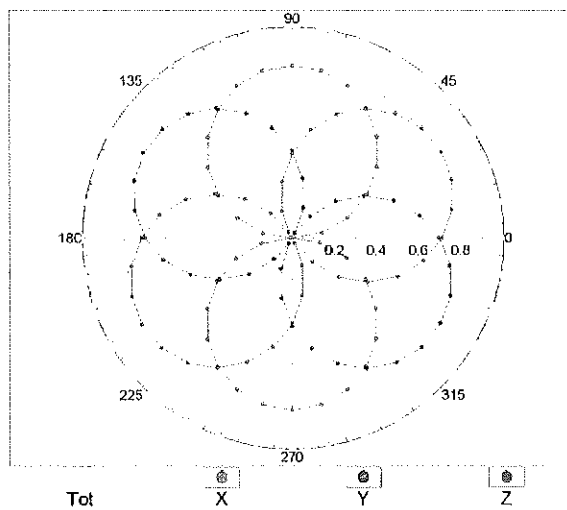


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

# Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f = 900 \text{ MHz}$ )

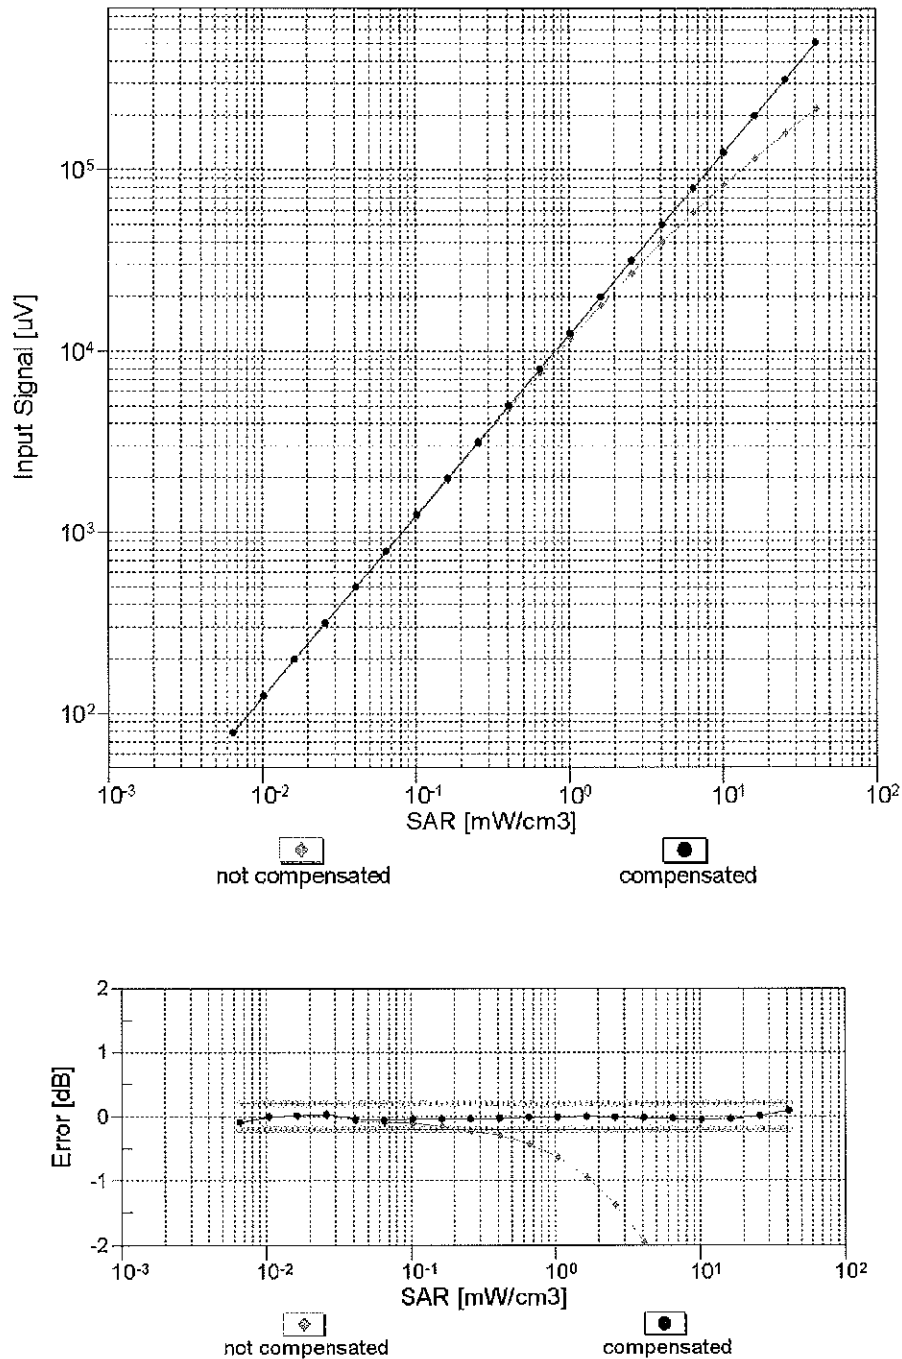



Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

## Conversion Factor Assessment

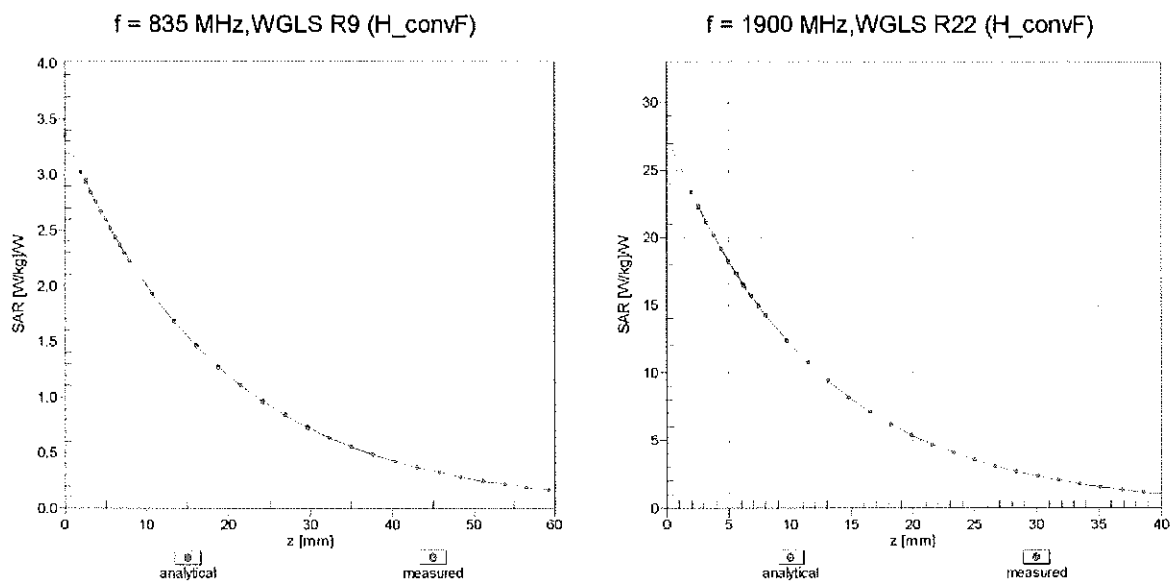

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

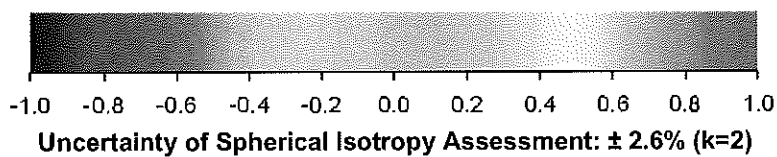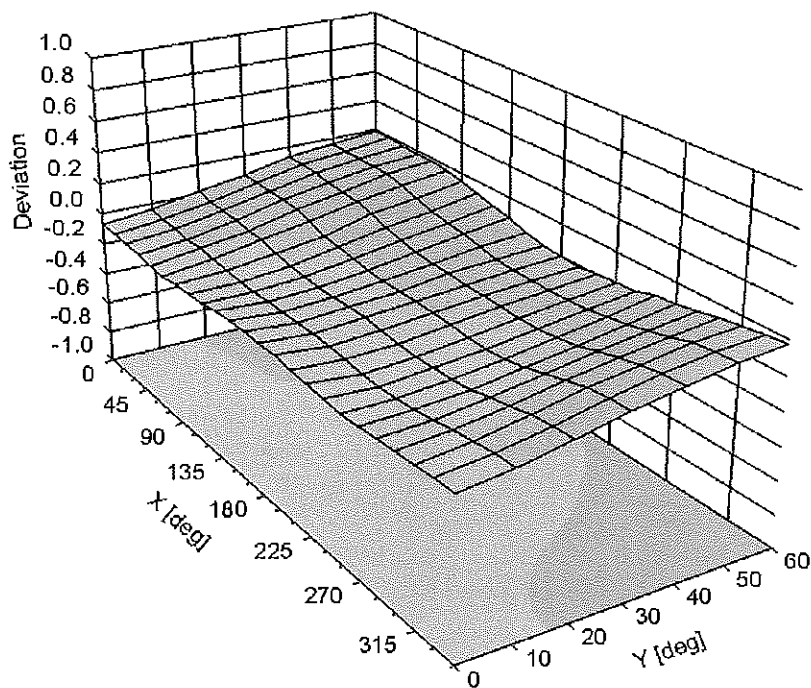

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -116       |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 10 mm      |
| Tip Diameter                                  | 4 mm       |
| Probe Tip to Sensor X Calibration Point       | 2 mm       |
| Probe Tip to Sensor Y Calibration Point       | 2 mm       |
| Probe Tip to Sensor Z Calibration Point       | 2 mm       |
| Recommended Measurement Distance from Surface | 3 mm       |



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **ES3-3287\_Nov13**

## CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3287**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **November 20, 2013**

CC  
11/20/2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 28-Dec-12 (No. ES3-3013_Dec12)    | Dec-13                 |
| DAE4                       | SN: 660         | 4-Sep-13 (No. DAE4-660_Sep13)     | Sep-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-15 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

|                                                                                                                 | Name          | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|---------------|-----------------------|-----------|
| Calibrated by:                                                                                                  | Leif Klysner  | Laboratory Technician |           |
| Approved by:                                                                                                    | Kalja Pokovic | Technical Manager     |           |
| Issued: November 20, 2013                                                                                       |               |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |               |                       |           |



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C, D               | modulation dependent linearization parameters                                                                                                           |
| Polarization $\phi$      | $\phi$ rotation around probe axis                                                                                                                       |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |
| Connector Angle          | information used in DASY system to align probe sensor X to the robot coordinate system                                                                  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

# Probe ES3DV3

## SN:3287

Manufactured: June 7, 2010  
Calibrated: November 20, 2013

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

# DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287

## Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2)     |
|-----------------------------------------------------------|----------|----------|----------|---------------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 1.31     | 1.25     | 1.25     | $\pm 10.1 \%$ |
| DCP (mV) <sup>B</sup>                                     | 102.6    | 102.5    | 100.4    |               |

## Modulation Calibration Parameters

| UID           | Communication System Name                |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C    | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|---------------|------------------------------------------|---|---------|------------------------------|------|---------|----------|---------------------------|
| 0             | CW                                       | X | 0.0     | 0.0                          | 1.0  | 0.00    | 157.3    | $\pm 2.7 \%$              |
|               |                                          | Y | 0.0     | 0.0                          | 1.0  |         | 159.9    |                           |
|               |                                          | Z | 0.0     | 0.0                          | 1.0  |         | 152.5    |                           |
| 10010-<br>CAA | SAR Validation (Square, 100ms, 10ms)     | X | 2.23    | 57.9                         | 9.9  | 10.00   | 45.7     | $\pm 1.4 \%$              |
|               |                                          | Y | 2.13    | 57.6                         | 9.8  |         | 46.6     |                           |
|               |                                          | Z | 3.31    | 61.1                         | 11.8 |         | 47.6     |                           |
| 10011-<br>CAA | UMTS-FDD (WCDMA)                         | X | 3.25    | 66.3                         | 17.9 | 2.91    | 124.8    | $\pm 0.5 \%$              |
|               |                                          | Y | 3.16    | 65.7                         | 17.4 |         | 127.4    |                           |
|               |                                          | Z | 3.15    | 65.5                         | 17.4 |         | 122.8    |                           |
| 10012-<br>CAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps) | X | 3.08    | 68.7                         | 18.3 | 1.87    | 127.2    | $\pm 0.7 \%$              |
|               |                                          | Y | 3.03    | 68.2                         | 17.9 |         | 129.4    |                           |
|               |                                          | Z | 2.87    | 67.0                         | 17.3 |         | 126.5    |                           |
| 10021-<br>DAA | GSM-FDD (TDMA, GMSK)                     | X | 15.99   | 90.6                         | 25.0 | 9.39    | 99.9     | $\pm 1.2 \%$              |
|               |                                          | Y | 12.41   | 86.6                         | 23.6 |         | 101.5    |                           |
|               |                                          | Z | 29.18   | 99.9                         | 28.5 |         | 109.2    |                           |
| 10023-<br>DAA | GPRS-FDD (TDMA, GMSK, TN 0)              | X | 25.67   | 98.9                         | 27.8 | 9.57    | 97.9     | $\pm 1.7 \%$              |
|               |                                          | Y | 14.20   | 88.5                         | 24.3 |         | 100.6    |                           |
|               |                                          | Z | 27.68   | 99.8                         | 28.8 |         | 107.7    |                           |
| 10024-<br>DAA | GPRS-FDD (TDMA, GMSK, TN 0-1)            | X | 42.95   | 99.6                         | 24.9 | 6.56    | 124.4    | $\pm 1.4 \%$              |
|               |                                          | Y | 45.27   | 99.9                         | 24.8 |         | 128.8    |                           |
|               |                                          | Z | 42.64   | 99.6                         | 25.5 |         | 135.7    |                           |
| 10027-<br>DAA | GPRS-FDD (TDMA, GMSK, TN 0-1-2)          | X | 27.78   | 91.3                         | 21.1 | 4.80    | 136.0    | $\pm 1.4 \%$              |
|               |                                          | Y | 32.74   | 93.9                         | 21.9 |         | 146.6    |                           |
|               |                                          | Z | 23.93   | 89.5                         | 21.1 |         | 144.8    |                           |
| 10028-<br>DAA | GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)        | X | 59.17   | 99.6                         | 22.4 | 3.55    | 142.5    | $\pm 1.2 \%$              |
|               |                                          | Y | 78.76   | 99.7                         | 21.7 |         | 104.9    |                           |
|               |                                          | Z | 38.06   | 94.2                         | 21.4 |         | 148.8    |                           |
| 10032-<br>CAA | IEEE 802.15.1 Bluetooth (GFSK, DH5)      | X | 93.35   | 99.7                         | 19.5 | 1.16    | 108.1    | $\pm 0.9 \%$              |
|               |                                          | Y | 96.67   | 94.0                         | 16.9 |         | 114.7    |                           |
|               |                                          | Z | 98.17   | 96.2                         | 18.2 |         | 108.9    |                           |
| 10039-<br>CAA | CDMA2000 (1xRTT, RC1)                    | X | 4.84    | 66.7                         | 18.8 | 4.57    | 126.5    | $\pm 0.9 \%$              |
|               |                                          | Y | 4.83    | 66.6                         | 18.6 |         | 134.4    |                           |
|               |                                          | Z | 4.76    | 66.0                         | 18.3 |         | 125.9    |                           |
| 10081-<br>CAA | CDMA2000 (1xRTT, RC3)                    | X | 4.00    | 66.2                         | 18.5 | 3.97    | 121.9    | $\pm 0.7 \%$              |
|               |                                          | Y | 3.91    | 65.5                         | 17.9 |         | 128.9    |                           |
|               |                                          | Z | 3.88    | 65.2                         | 17.8 |         | 120.7    |                           |



|           |                                          |   |       |      |      |      |       |        |
|-----------|------------------------------------------|---|-------|------|------|------|-------|--------|
| 10098-CAA | UMTS-FDD (HSUPA, Subtest 2)              | X | 4.66  | 66.6 | 18.4 | 3.98 | 132.5 | ±0.7 % |
|           |                                          | Y | 4.66  | 66.5 | 18.2 |      | 141.3 |        |
|           |                                          | Z | 4.54  | 65.9 | 17.9 |      | 130.7 |        |
| 10100-CAB | LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK) | X | 6.65  | 68.3 | 20.1 | 5.67 | 139.5 | ±1.4 % |
|           |                                          | Y | 6.69  | 68.3 | 19.9 |      | 148.9 |        |
|           |                                          | Z | 6.60  | 67.9 | 19.8 |      | 137.5 |        |
| 10108-CAB | LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK) | X | 6.52  | 67.8 | 20.0 | 5.80 | 137.3 | ±1.4 % |
|           |                                          | Y | 6.53  | 67.6 | 19.7 |      | 147.5 |        |
|           |                                          | Z | 6.51  | 67.6 | 19.8 |      | 135.3 |        |
| 10110-CAB | LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)  | X | 6.19  | 67.2 | 19.7 | 5.75 | 134.3 | ±1.2 % |
|           |                                          | Y | 6.24  | 67.3 | 19.6 |      | 142.9 |        |
|           |                                          | Z | 6.23  | 67.1 | 19.6 |      | 132.3 |        |
| 10151-CAB | LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)  | X | 11.56 | 79.1 | 27.9 | 9.28 | 130.1 | ±3.0 % |
|           |                                          | Y | 11.01 | 76.8 | 26.2 |      | 141.9 |        |
|           |                                          | Z | 12.98 | 81.2 | 28.7 |      | 135.7 |        |
| 10154-CAB | LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)  | X | 6.25  | 67.4 | 19.8 | 5.75 | 135.1 | ±1.2 % |
|           |                                          | Y | 6.17  | 66.9 | 19.3 |      | 143.6 |        |
|           |                                          | Z | 6.16  | 66.8 | 19.4 |      | 132.8 |        |
| 10160-CAB | LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)  | X | 6.66  | 67.8 | 20.0 | 5.82 | 140.3 | ±1.4 % |
|           |                                          | Y | 6.72  | 67.9 | 19.9 |      | 148.8 |        |
|           |                                          | Z | 6.66  | 67.6 | 19.8 |      | 137.4 |        |
| 10169-CAB | LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)    | X | 5.05  | 66.7 | 19.5 | 5.73 | 117.8 | ±0.9 % |
|           |                                          | Y | 4.93  | 66.0 | 18.9 |      | 125.0 |        |
|           |                                          | Z | 5.08  | 66.3 | 19.3 |      | 116.3 |        |
| 10172-CAB | LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)    | X | 8.47  | 76.8 | 26.9 | 9.21 | 100.3 | ±2.2 % |
|           |                                          | Y | 8.06  | 74.6 | 25.3 |      | 107.5 |        |
|           |                                          | Z | 9.43  | 78.2 | 27.4 |      | 102.5 |        |
| 10175-CAB | LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)    | X | 4.98  | 66.3 | 19.3 | 5.72 | 118.2 | ±0.9 % |
|           |                                          | Y | 4.96  | 66.1 | 19.0 |      | 119.9 |        |
|           |                                          | Z | 5.03  | 66.1 | 19.1 |      | 116.1 |        |
| 10181-CAB | LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)    | X | 5.06  | 66.7 | 19.6 | 5.72 | 118.7 | ±0.9 % |
|           |                                          | Y | 4.97  | 66.2 | 19.1 |      | 120.0 |        |
|           |                                          | Z | 5.03  | 66.1 | 19.1 |      | 116.3 |        |
| 10225-CAA | UMTS-FDD (HSPA+)                         | X | 6.78  | 66.1 | 18.9 | 5.97 | 105.3 | ±1.2 % |
|           |                                          | Y | 6.68  | 65.7 | 18.6 |      | 106.8 |        |
|           |                                          | Z | 7.32  | 67.6 | 19.7 |      | 148.0 |        |
| 10237-CAB | LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)    | X | 8.56  | 77.1 | 27.1 | 9.21 | 100.8 | ±1.9 % |
|           |                                          | Y | 8.33  | 75.8 | 26.1 |      | 103.8 |        |
|           |                                          | Z | 9.39  | 78.0 | 27.3 |      | 101.9 |        |
| 10252-CAB | LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)  | X | 10.58 | 77.8 | 27.4 | 9.24 | 123.3 | ±2.5 % |
|           |                                          | Y | 10.48 | 76.9 | 26.5 |      | 128.1 |        |
|           |                                          | Z | 11.79 | 79.6 | 28.0 |      | 127.0 |        |
| 10267-CAB | LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK) | X | 11.52 | 79.1 | 27.9 | 9.30 | 130.1 | ±2.7 % |
|           |                                          | Y | 11.24 | 77.7 | 26.9 |      | 136.0 |        |
|           |                                          | Z | 12.96 | 81.2 | 28.8 |      | 134.8 |        |

|           |                                                           |   |      |      |      |      |       |        |
|-----------|-----------------------------------------------------------|---|------|------|------|------|-------|--------|
| 10274-CAA | UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)                 | X | 6.14 | 67.4 | 19.0 | 4.87 | 145.5 | ±1.2 % |
|           |                                                           | Y | 6.19 | 67.4 | 19.0 |      | 149.2 |        |
|           |                                                           | Z | 6.10 | 66.9 | 18.8 |      | 142.3 |        |
| 10275-CAA | UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)                  | X | 4.41 | 66.4 | 18.3 | 3.96 | 126.4 | ±0.7 % |
|           |                                                           | Y | 4.43 | 66.3 | 18.2 |      | 130.4 |        |
|           |                                                           | Z | 4.36 | 65.9 | 18.0 |      | 123.8 |        |
| 10291-AAA | CDMA2000, RC3, SO55, Full Rate                            | X | 3.57 | 65.9 | 17.9 | 3.46 | 120.0 | ±0.5 % |
|           |                                                           | Y | 3.55 | 65.6 | 17.6 |      | 121.7 |        |
|           |                                                           | Z | 3.50 | 65.1 | 17.5 |      | 117.2 |        |
| 10292-AAA | CDMA2000, RC3, SO32, Full Rate                            | X | 3.55 | 66.1 | 18.0 | 3.39 | 121.3 | ±0.5 % |
|           |                                                           | Y | 3.54 | 66.0 | 17.8 |      | 123.6 |        |
|           |                                                           | Z | 3.45 | 65.2 | 17.4 |      | 118.9 |        |
| 10297-AAA | LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)                   | X | 6.53 | 67.8 | 20.0 | 5.81 | 136.2 | ±1.2 % |
|           |                                                           | Y | 6.48 | 67.5 | 19.6 |      | 139.3 |        |
|           |                                                           | Z | 6.52 | 67.6 | 19.8 |      | 134.1 |        |
| 10311-AAA | LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)                  | X | 7.12 | 68.4 | 20.4 | 6.06 | 141.7 | ±1.4 % |
|           |                                                           | Y | 7.11 | 68.3 | 20.1 |      | 145.3 |        |
|           |                                                           | Z | 7.14 | 68.4 | 20.3 |      | 139.8 |        |
| 10315-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle) | X | 2.79 | 67.6 | 18.0 | 1.71 | 125.5 | ±0.5 % |
|           |                                                           | Y | 2.71 | 66.9 | 17.3 |      | 128.2 |        |
|           |                                                           | Z | 2.64 | 66.2 | 17.0 |      | 123.5 |        |
| 10403-AAA | CDMA2000 (1xEV-DO, Rev. 0)                                | X | 4.78 | 67.5 | 18.3 | 3.76 | 130.6 | ±0.5 % |
|           |                                                           | Y | 4.77 | 67.5 | 18.2 |      | 133.8 |        |
|           |                                                           | Z | 4.65 | 66.5 | 17.8 |      | 130.0 |        |
| 10404-AAA | CDMA2000 (1xEV-DO, Rev. A)                                | X | 4.83 | 68.2 | 18.6 | 3.77 | 129.2 | ±0.7 % |
|           |                                                           | Y | 4.68 | 67.4 | 18.0 |      | 131.9 |        |
|           |                                                           | Z | 4.52 | 66.3 | 17.7 |      | 128.7 |        |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 7 and 8).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 41.9                               | 0.89                            | 6.52    | 6.52    | 6.52    | 0.47               | 1.46                    | ± 12.0 %    |
| 835                  | 41.5                               | 0.90                            | 6.30    | 6.30    | 6.30    | 0.40               | 1.59                    | ± 12.0 %    |
| 1750                 | 40.1                               | 1.37                            | 5.27    | 5.27    | 5.27    | 0.63               | 1.34                    | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 5.08    | 5.08    | 5.08    | 0.62               | 1.37                    | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 4.43    | 4.43    | 4.43    | 0.79               | 1.28                    | ± 12.0 %    |
| 2600                 | 39.0                               | 1.96                            | 4.29    | 4.29    | 4.29    | 0.77               | 1.38                    | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287

### Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 55.5                               | 0.96                            | 6.09    | 6.09    | 6.09    | 0.55               | 1.37                    | ± 12.0 %    |
| 835                  | 55.2                               | 0.97                            | 6.04    | 6.04    | 6.04    | 0.55               | 1.39                    | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 4.93    | 4.93    | 4.93    | 0.39               | 1.73                    | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 4.67    | 4.67    | 4.67    | 0.38               | 1.75                    | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 4.17    | 4.17    | 4.17    | 0.60               | 1.20                    | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 4.00    | 4.00    | 4.00    | 0.60               | 1.10                    | ± 12.0 %    |


<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

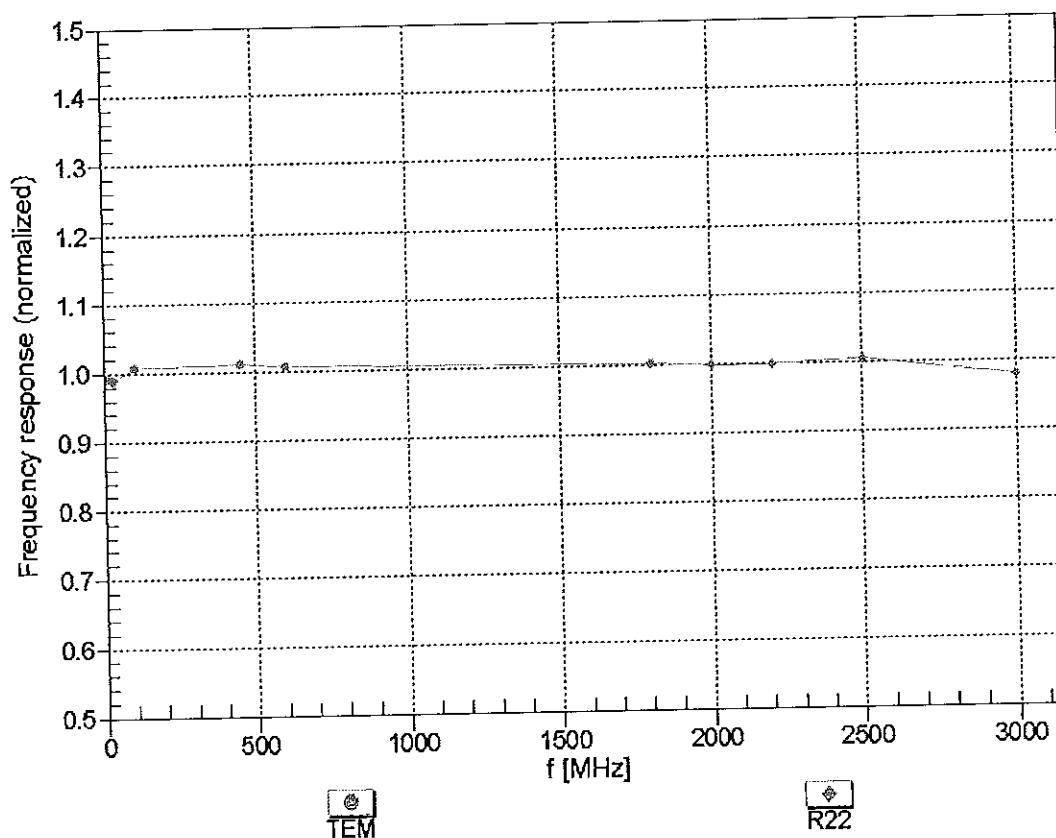



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

f=600 MHz,TEM

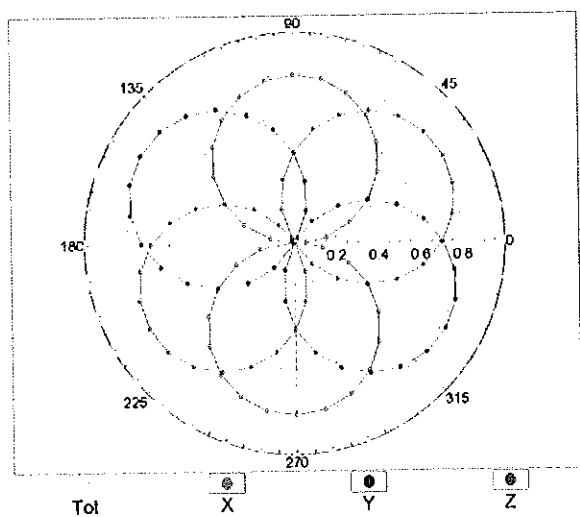



f=1800 MHz,R22

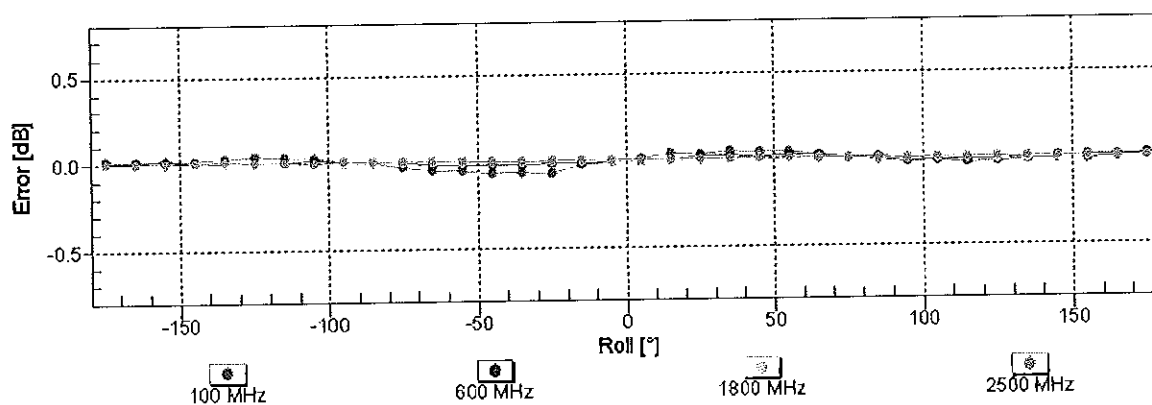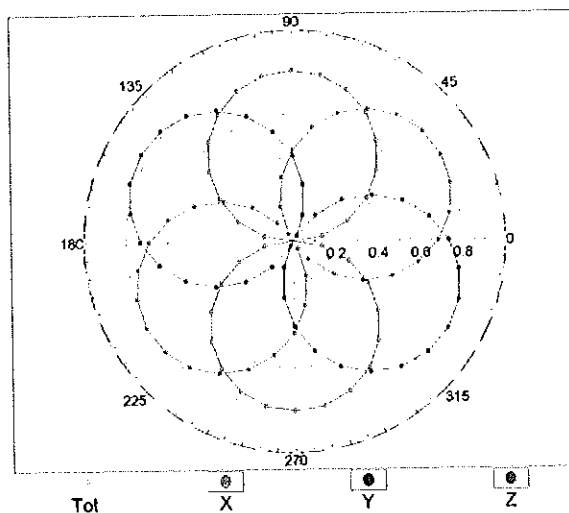

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )


# Dynamic Range f(SAR<sub>head</sub>)

(TEM cell , f = 900 MHz)

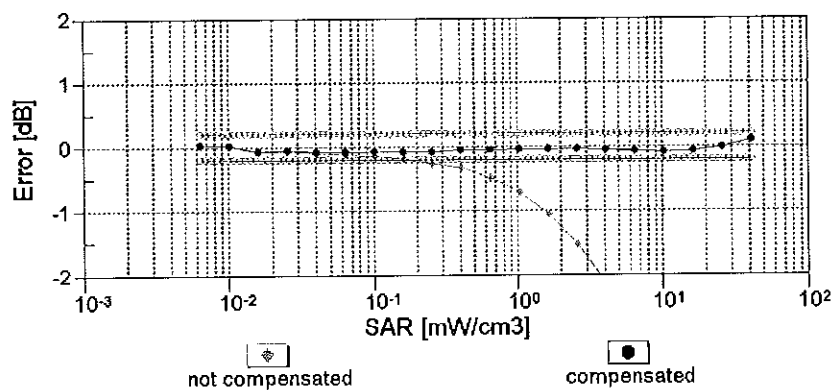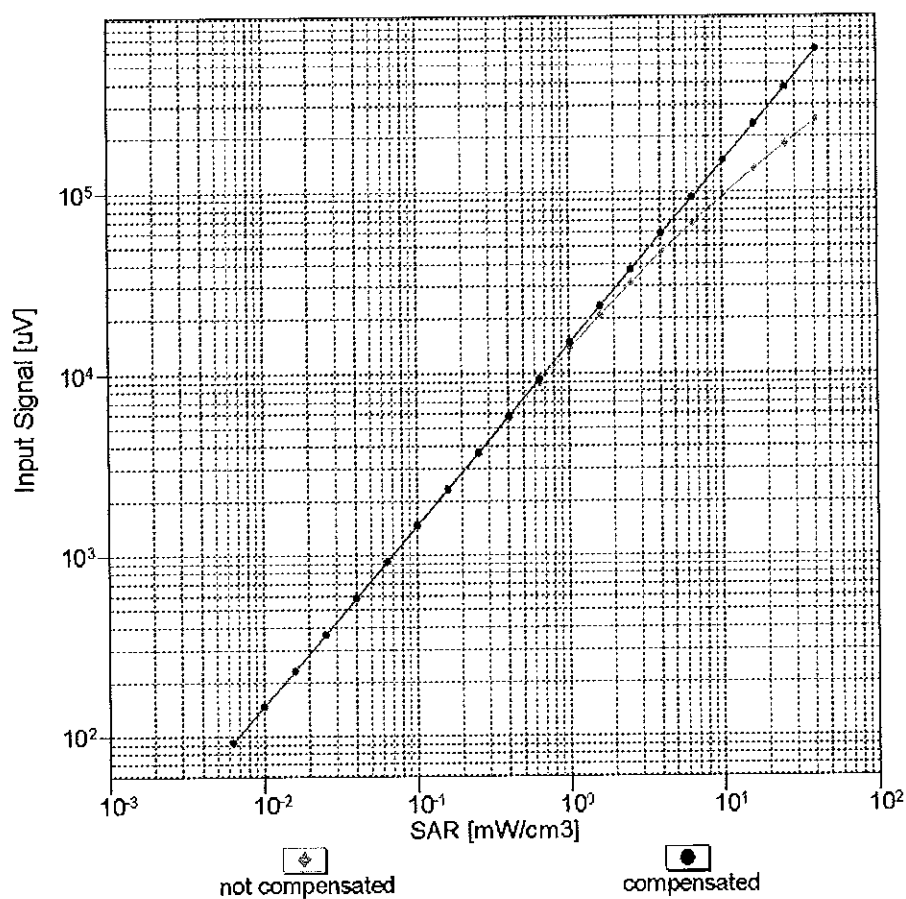



Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

## Conversion Factor Assessment

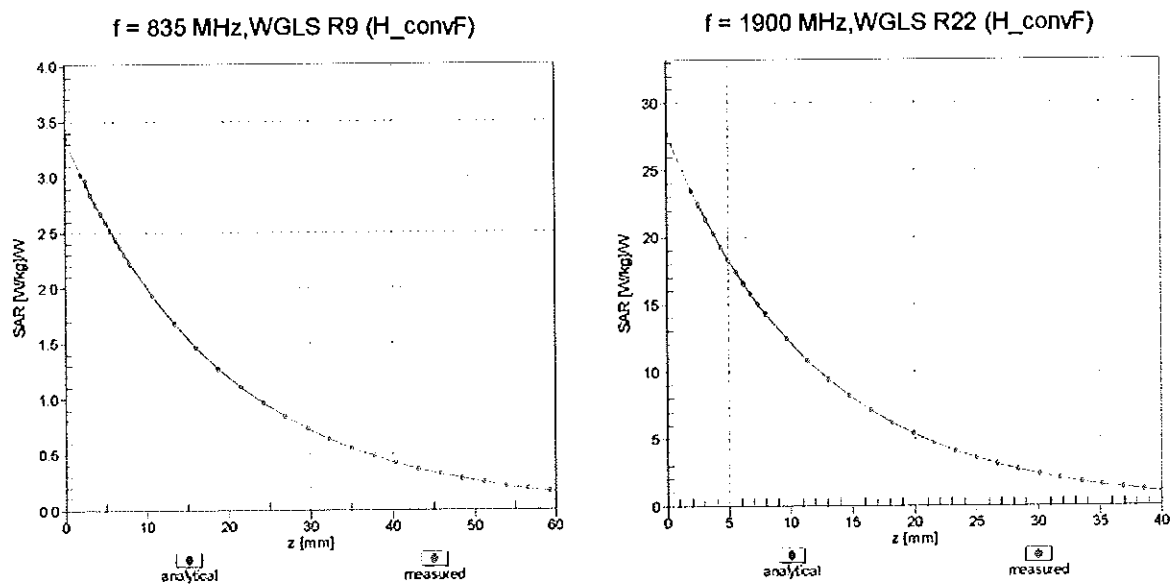

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

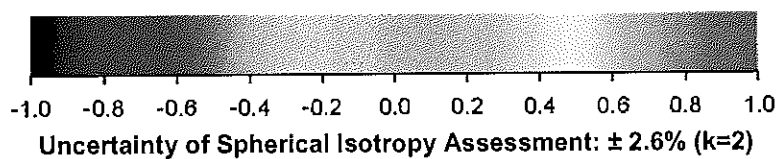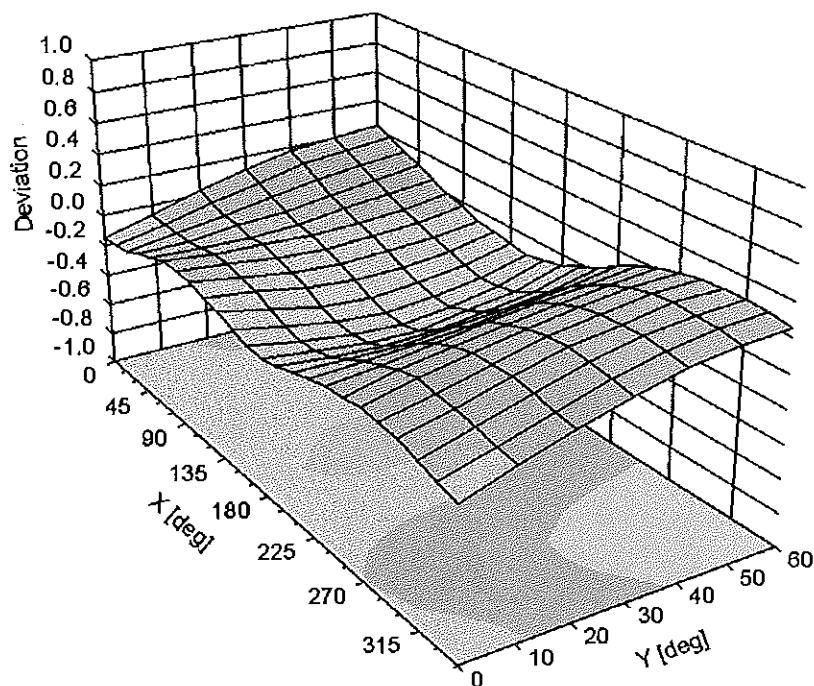



**DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287****Other Probe Parameters**

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -15        |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 10 mm      |
| Tip Diameter                                  | 4 mm       |
| Probe Tip to Sensor X Calibration Point       | 2 mm       |
| Probe Tip to Sensor Y Calibration Point       | 2 mm       |
| Probe Tip to Sensor Z Calibration Point       | 2 mm       |
| Recommended Measurement Distance from Surface | 3 mm       |



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **ES3-3288\_Sep13/2**

## **CALIBRATION CERTIFICATE (Replacement of No: ES3-3288\_Sep13)**

Object **ES3DV3 - SN:3288**

CCV  
10/4/13

Calibration procedure(s) **QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **September 23, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 28-Dec-12 (No. ES3-3013_Dec12)    | Dec-13                 |
| DAE4                       | SN: 660         | 4-Sep-13 (No. DAE4-660_Sep13)     | Apr-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-15 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-12) | In house check: Oct-13 |

|                                                                                                                 | Name           | Function              | Signature               |
|-----------------------------------------------------------------------------------------------------------------|----------------|-----------------------|-------------------------|
| Calibrated by:                                                                                                  | Jeton Kastrati | Laboratory Technician |                         |
| Approved by:                                                                                                    | Katja Pokovic  | Technical Manager     |                         |
|                                                                                                                 |                |                       | Issued: October 4, 2013 |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |                |                       |                         |

# Probe ES3DV3

## SN:3288

Manufactured: July 6, 2010  
Calibrated: September 23, 2013

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C, D               | modulation dependent linearization parameters                                                                                                           |
| Polarization $\phi$      | $\phi$ rotation around probe axis                                                                                                                       |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288

### Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|-----------------------------------------------------------|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.87     | 0.97     | 0.75     | ± 10.1 %  |
| DCP (mV) <sup>B</sup>                                     | 103.3    | 103.2    | 100.2    |           |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C   | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----|---------------------------|---|---------|------------------------------|-----|---------|----------|---------------------------|
| 0   | CW                        | X | 0.0     | 0.0                          | 1.0 | 0.00    | 171.1    | ±3.5 %                    |
|     |                           | Y | 0.0     | 0.0                          | 1.0 |         | 135.0    |                           |
|     |                           | Z | 0.0     | 0.0                          | 1.0 |         | 154.3    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 41.9                               | 0.89                            | 6.56    | 6.56    | 6.56    | 0.32  | 1.89       | ± 12.0 %    |
| 835                  | 41.5                               | 0.90                            | 6.37    | 6.37    | 6.37    | 0.34  | 1.82       | ± 12.0 %    |
| 1750                 | 40.1                               | 1.37                            | 5.67    | 5.67    | 5.67    | 0.56  | 1.51       | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 5.47    | 5.47    | 5.47    | 0.80  | 1.29       | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 4.63    | 4.63    | 4.63    | 0.80  | 1.34       | ± 12.0 %    |
| 2600                 | 39.0                               | 1.96                            | 4.55    | 4.55    | 4.55    | 0.80  | 1.41       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288


### Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 55.5                               | 0.96                            | 6.25    | 6.25    | 6.25    | 0.70  | 1.27       | ± 12.0 %    |
| 835                  | 55.2                               | 0.97                            | 6.27    | 6.27    | 6.27    | 0.75  | 1.22       | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 5.10    | 5.10    | 5.10    | 0.59  | 1.46       | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 4.82    | 4.82    | 4.82    | 0.53  | 1.54       | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 4.37    | 4.37    | 4.37    | 0.80  | 1.02       | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 4.14    | 4.14    | 4.14    | 0.64  | 0.94       | ± 12.0 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

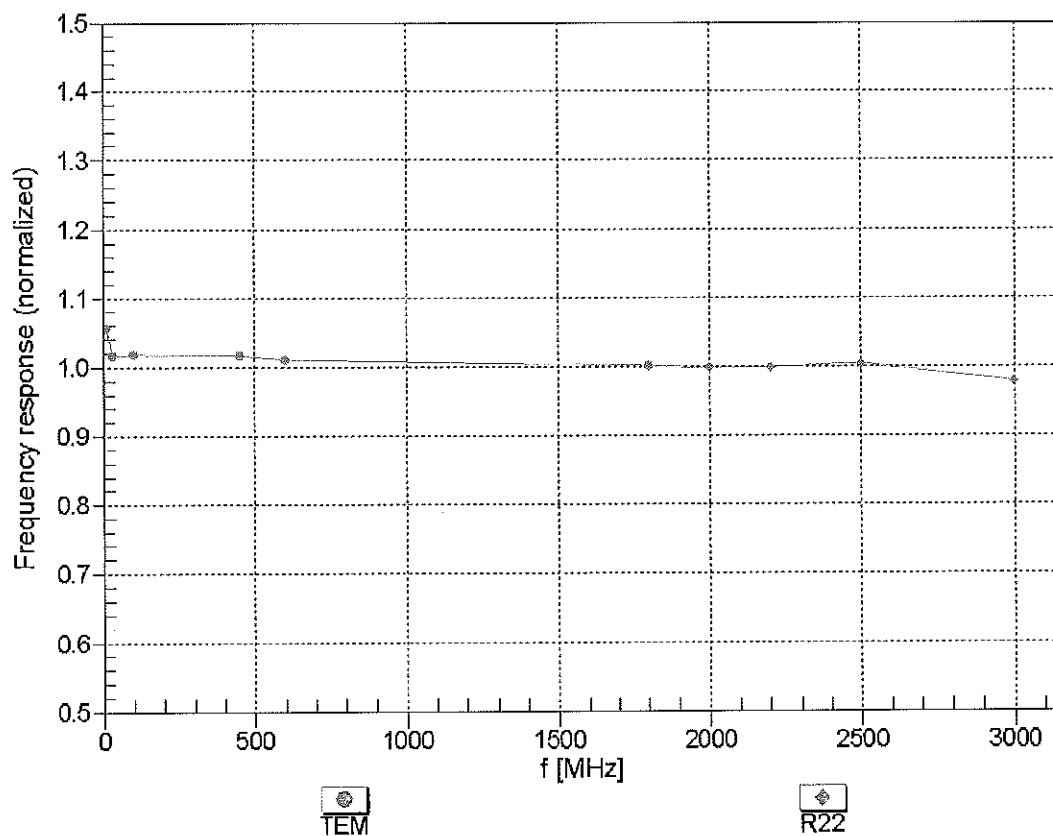


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )





## Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

f=600 MHz,TEM

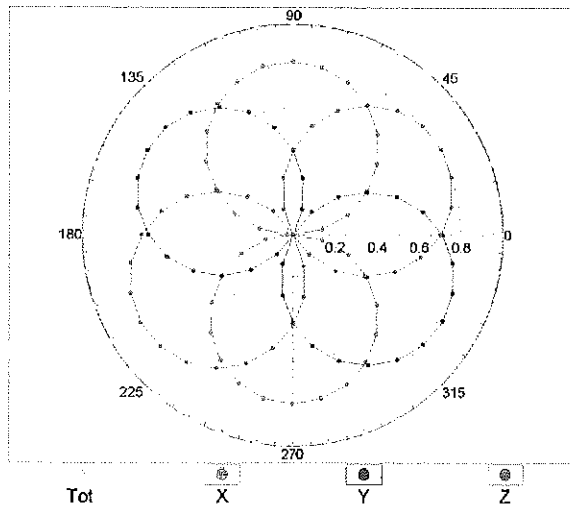


f=1800 MHz,R22

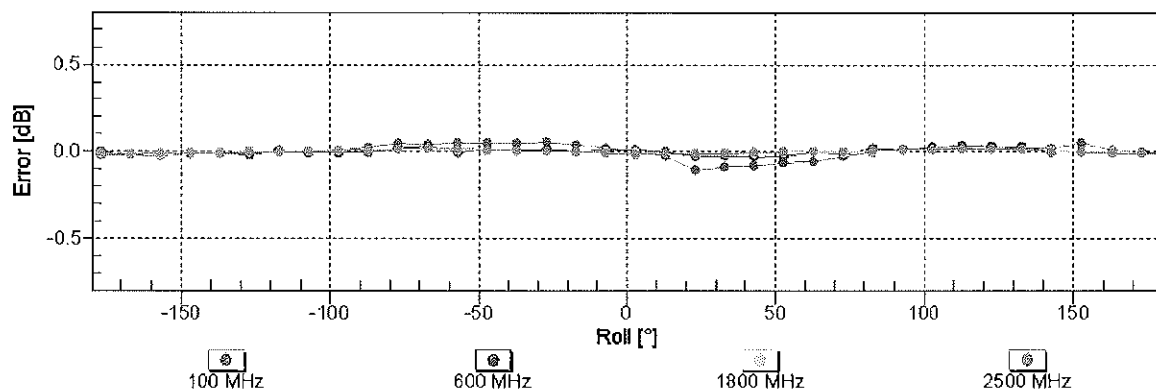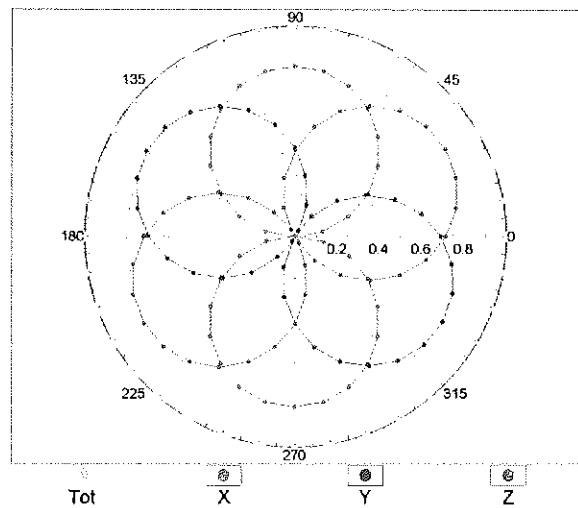


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

# Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f = 900 MHz)

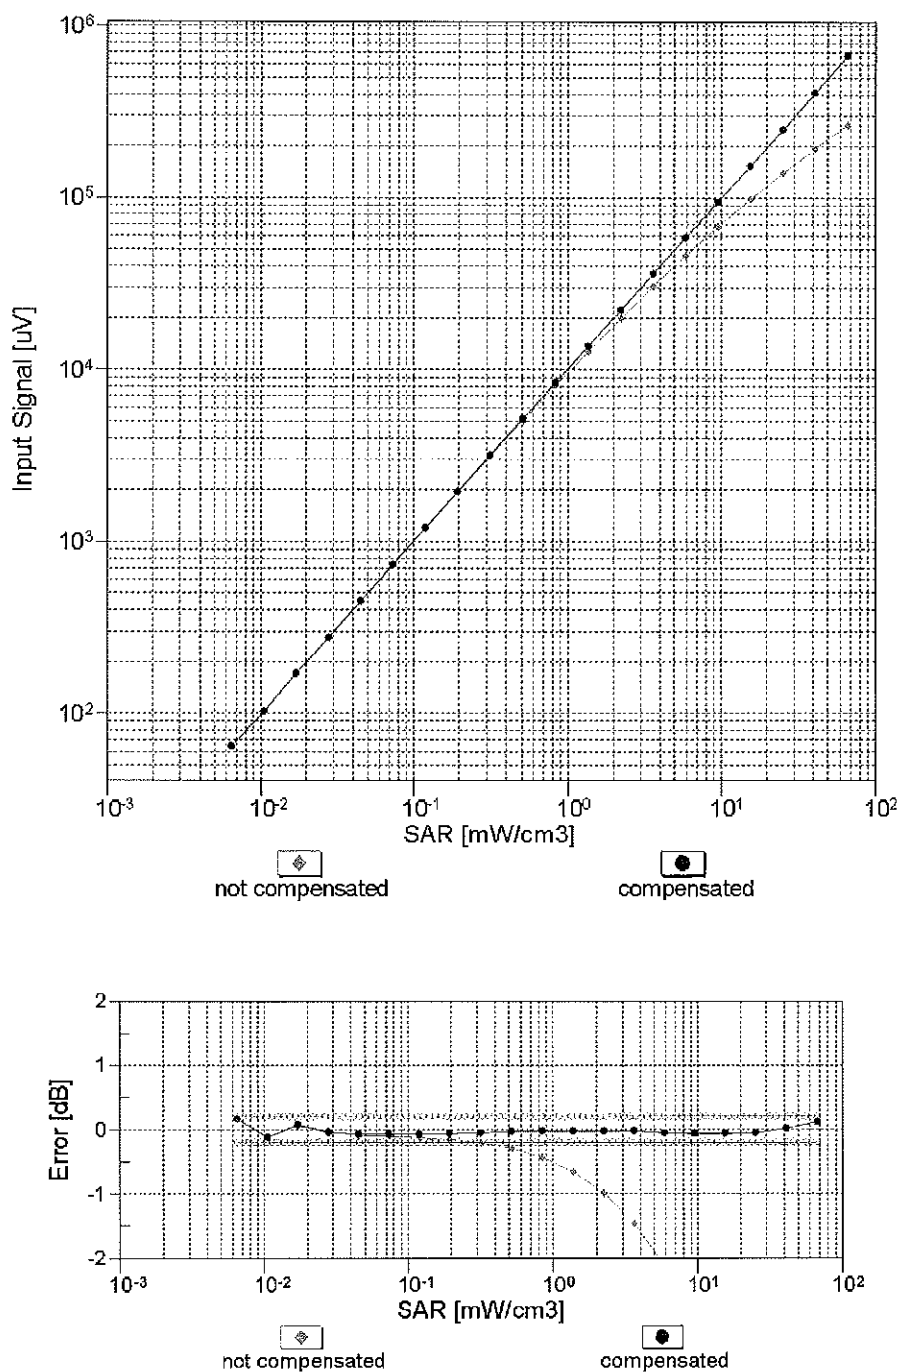



Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)

## Conversion Factor Assessment

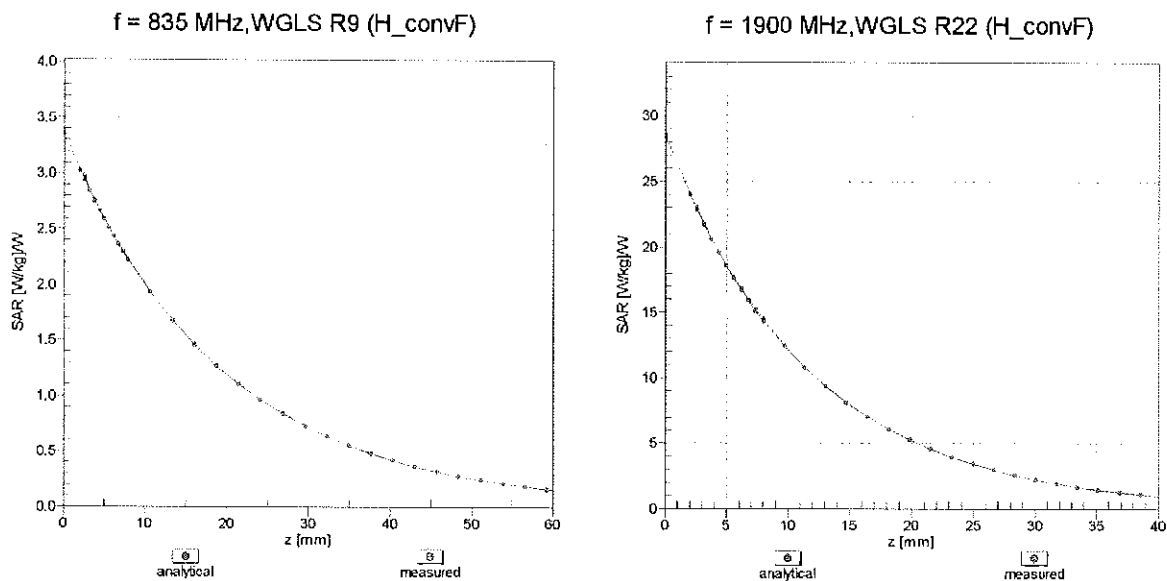

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

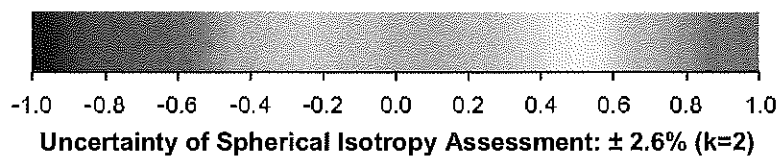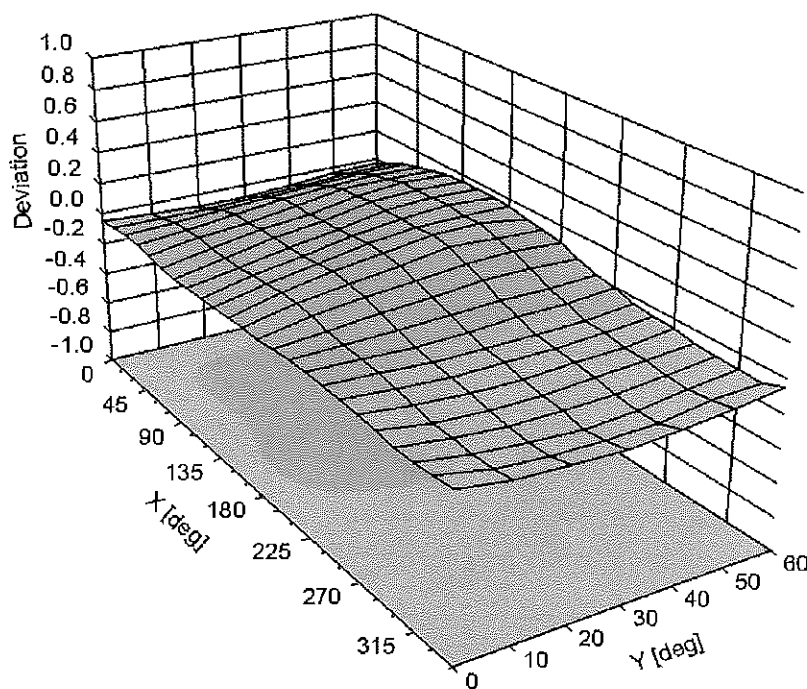

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -127.1     |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 10 mm      |
| Tip Diameter                                  | 4 mm       |
| Probe Tip to Sensor X Calibration Point       | 2 mm       |
| Probe Tip to Sensor Y Calibration Point       | 2 mm       |
| Probe Tip to Sensor Z Calibration Point       | 2 mm       |
| Recommended Measurement Distance from Surface | 3 mm       |



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **EX3-3914\_Oct13**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3914**

Calibration procedure(s) **QA CAL-01 v3, QA CAL-14 v4, QA CAL-23 v5, QA CAL-25 v6**  
 Calibration procedure for dosimetric E-field probes

Calibration date: **October 23, 2013**

*VCC*  
*11/20/2013*

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 28-Dec-12 (No. ES3-3013_Dec12)    | Dec-13                 |
| DAE4                       | SN: 660         | 4-Sep-13 (No. DAE4-660_Sep13)     | Sep-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-15 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

|                                                                                                                 | Name          | Function              | Signature            |
|-----------------------------------------------------------------------------------------------------------------|---------------|-----------------------|----------------------|
| Calibrated by:                                                                                                  | Leif Klysner  | Laboratory Technician | <i>Leif Klysner</i>  |
| Approved by:                                                                                                    | Katja Pokovic | Technical Manager     | <i>Katja Pokovic</i> |
| Issued: October 25, 2013                                                                                        |               |                       |                      |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |               |                       |                      |

*PCT # 81072*



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                       |                                                                                                                                                   |
|-----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                   | tissue simulating liquid                                                                                                                          |
| NORM <sub>x,y,z</sub> | sensitivity in free space                                                                                                                         |
| ConvF                 | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                        |
| DCP                   | diode compression point                                                                                                                           |
| CF                    | crest factor (1/duty_cycle) of the RF signal                                                                                                      |
| A, B, C, D            | modulation dependent linearization parameters                                                                                                     |
| Polarization $\phi$   | $\phi$ rotation around probe axis                                                                                                                 |
| Polarization $\theta$ | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\theta = 0$ is normal to probe axis |
| Connector Angle       | information used in DASY system to align probe sensor X to the robot coordinate system                                                            |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

# Probe EX3DV4

## SN:3914

Manufactured: December 18, 2012  
Calibrated: October 23, 2013

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3914

## Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2)     |
|-----------------------------------------------------------|----------|----------|----------|---------------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.47     | 0.49     | 0.51     | $\pm 10.1 \%$ |
| DCP (mV) <sup>B</sup>                                     | 99.2     | 98.9     | 98.2     |               |

## Modulation Calibration Parameters

| UID       | Communication System Name                |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C    | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----------|------------------------------------------|---|---------|------------------------------|------|---------|----------|---------------------------|
| 0         | CW                                       | X | 0.0     | 0.0                          | 1.0  | 0.00    | 158.3    | $\pm 3.0 \%$              |
|           |                                          | Y | 0.0     | 0.0                          | 1.0  |         | 154.6    |                           |
|           |                                          | Z | 0.0     | 0.0                          | 1.0  |         | 170.8    |                           |
| 10010-CAA | SAR Validation (Square, 100ms, 10ms)     | X | 0.71    | 53.3                         | 6.1  | 10.00   | 48.4     | $\pm 2.5 \%$              |
|           |                                          | Y | 2.43    | 67.0                         | 13.8 |         | 39.9     |                           |
|           |                                          | Z | 4.18    | 68.7                         | 13.8 |         | 45.7     |                           |
| 10011-CAA | UMTS-FDD (WCDMA)                         | X | 3.05    | 64.4                         | 16.5 | 2.91    | 122.4    | $\pm 0.5 \%$              |
|           |                                          | Y | 3.31    | 66.5                         | 18.2 |         | 123.5    |                           |
|           |                                          | Z | 3.34    | 66.3                         | 17.8 |         | 136.6    |                           |
| 10012-CAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps) | X | 2.49    | 64.8                         | 16.1 | 1.87    | 120.6    | $\pm 0.5 \%$              |
|           |                                          | Y | 2.94    | 68.6                         | 18.7 |         | 123.6    |                           |
|           |                                          | Z | 2.63    | 65.9                         | 17.0 |         | 135.4    |                           |
| 10021-DAA | GSM-FDD (TDMA, GMSK)                     | X | 1.52    | 61.5                         | 10.9 | 9.39    | 83.6     | $\pm 1.2 \%$              |
|           |                                          | Y | 2.22    | 67.4                         | 15.0 |         | 116.0    |                           |
|           |                                          | Z | 2.47    | 66.8                         | 14.7 |         | 95.9     |                           |
| 10023-DAA | GPRS-FDD (TDMA, GMSK, TN 0)              | X | 1.73    | 63.3                         | 11.9 | 9.57    | 81.5     | $\pm 1.7 \%$              |
|           |                                          | Y | 2.11    | 66.2                         | 14.2 |         | 111.8    |                           |
|           |                                          | Z | 2.76    | 69.0                         | 16.0 |         | 93.6     |                           |
| 10024-DAA | GPRS-FDD (TDMA, GMSK, TN 0-1)            | X | 1.34    | 62.1                         | 9.4  | 6.56    | 121.0    | $\pm 1.2 \%$              |
|           |                                          | Y | 4.24    | 78.6                         | 17.9 |         | 130.0    |                           |
|           |                                          | Z | 2.91    | 70.7                         | 14.9 |         | 141.4    |                           |
| 10027-DAA | GPRS-FDD (TDMA, GMSK, TN 0-1-2)          | X | 1.25    | 63.5                         | 9.7  | 4.80    | 143.5    | $\pm 1.4 \%$              |
|           |                                          | Y | 1.59    | 66.9                         | 12.2 |         | 149.7    |                           |
|           |                                          | Z | 2.98    | 71.5                         | 14.0 |         | 123.3    |                           |
| 10028-DAA | GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)        | X | 0.51    | 58.3                         | 7.4  | 3.55    | 113.4    | $\pm 1.2 \%$              |
|           |                                          | Y | 25.43   | 100.0                        | 22.6 |         | 121.3    |                           |
|           |                                          | Z | 38.67   | 97.5                         | 20.6 |         | 133.3    |                           |
| 10032-CAA | IEEE 802.15.1 Bluetooth (GFSK, DH5)      | X | 0.28    | 58.6                         | 5.3  | 1.16    | 134.7    | $\pm 0.9 \%$              |
|           |                                          | Y | 65.75   | 99.6                         | 18.6 |         | 141.3    |                           |
|           |                                          | Z | 0.20    | 55.6                         | 4.1  |         | 112.1    |                           |
| 10039-CAA | CDMA2000 (1xRTT, RC1)                    | X | 4.33    | 64.6                         | 17.4 | 4.57    | 113.8    | $\pm 0.7 \%$              |
|           |                                          | Y | 4.55    | 66.0                         | 18.6 |         | 120.8    |                           |
|           |                                          | Z | 4.85    | 66.2                         | 18.4 |         | 135.9    |                           |
| 10062-CAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps) | X | 9.83    | 67.6                         | 20.7 | 8.68    | 109.0    | $\pm 2.5 \%$              |
|           |                                          | Y | 10.06   | 68.4                         | 21.5 |         | 118.2    |                           |
|           |                                          | Z | 10.66   | 69.2                         | 21.7 |         | 134.0    |                           |



|           |                                               |   |       |      |      |      |       |        |
|-----------|-----------------------------------------------|---|-------|------|------|------|-------|--------|
| 10081-CAA | CDMA2000 (1xRTT, RC3)                         | X | 3.59  | 63.9 | 16.9 | 3.97 | 113.6 | ±0.7 % |
|           |                                               | Y | 3.84  | 65.6 | 18.2 |      | 119.6 |        |
|           |                                               | Z | 3.95  | 65.4 | 17.8 |      | 134.5 |        |
| 10098-CAA | UMTS-FDD (HSUPA, Subtest 2)                   | X | 4.41  | 65.2 | 17.3 | 3.98 | 126.0 | ±0.7 % |
|           |                                               | Y | 4.73  | 66.9 | 18.6 |      | 132.5 |        |
|           |                                               | Z | 4.51  | 65.5 | 17.7 |      | 105.6 |        |
| 10100-CAB | LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)      | X | 6.26  | 66.2 | 18.6 | 5.67 | 130.5 | ±1.2 % |
|           |                                               | Y | 6.61  | 67.7 | 19.8 |      | 139.3 |        |
|           |                                               | Z | 6.21  | 66.0 | 18.7 |      | 107.7 |        |
| 10108-CAB | LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)      | X | 6.13  | 65.8 | 18.6 | 5.80 | 126.3 | ±1.2 % |
|           |                                               | Y | 6.40  | 67.1 | 19.6 |      | 135.6 |        |
|           |                                               | Z | 6.10  | 65.5 | 18.5 |      | 107.4 |        |
| 10110-CAB | LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)       | X | 5.78  | 65.3 | 18.3 | 5.75 | 123.1 | ±1.2 % |
|           |                                               | Y | 5.97  | 66.3 | 19.2 |      | 131.5 |        |
|           |                                               | Z | 5.86  | 65.3 | 18.4 |      | 104.9 |        |
| 10114-CAA | IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK) | X | 9.92  | 67.7 | 20.3 | 8.10 | 115.7 | ±2.5 % |
|           |                                               | Y | 10.25 | 68.7 | 21.2 |      | 126.8 |        |
|           |                                               | Z | 10.71 | 69.4 | 21.3 |      | 146.0 |        |
| 10117-CAA | IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)      | X | 9.95  | 67.8 | 20.3 | 8.07 | 116.6 | ±2.5 % |
|           |                                               | Y | 10.26 | 68.7 | 21.1 |      | 128.3 |        |
|           |                                               | Z | 10.70 | 69.4 | 21.3 |      | 146.9 |        |
| 10151-CAB | LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)       | X | 7.19  | 67.3 | 21.5 | 9.28 | 145.0 | ±2.2 % |
|           |                                               | Y | 7.40  | 68.3 | 22.4 |      | 110.8 |        |
|           |                                               | Z | 7.79  | 68.4 | 22.0 |      | 128.0 |        |
| 10154-CAB | LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)       | X | 5.79  | 65.3 | 18.3 | 5.75 | 124.2 | ±1.2 % |
|           |                                               | Y | 6.03  | 66.5 | 19.4 |      | 131.9 |        |
|           |                                               | Z | 6.29  | 66.9 | 19.3 |      | 149.7 |        |
| 10160-CAB | LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)       | X | 6.23  | 65.9 | 18.6 | 5.82 | 128.3 | ±1.2 % |
|           |                                               | Y | 6.51  | 67.2 | 19.7 |      | 136.9 |        |
|           |                                               | Z | 6.24  | 65.7 | 18.6 |      | 107.3 |        |
| 10169-CAB | LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)         | X | 4.83  | 66.0 | 18.9 | 5.73 | 147.5 | ±1.2 % |
|           |                                               | Y | 4.72  | 65.8 | 19.2 |      | 113.8 |        |
|           |                                               | Z | 5.03  | 66.1 | 19.1 |      | 129.7 |        |
| 10172-CAB | LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)         | X | 5.83  | 69.2 | 22.8 | 9.21 | 149.9 | ±1.9 % |
|           |                                               | Y | 5.81  | 69.4 | 23.4 |      | 120.3 |        |
|           |                                               | Z | 6.38  | 70.0 | 23.2 |      | 137.2 |        |
| 10175-CAB | LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)         | X | 4.86  | 66.1 | 18.9 | 5.72 | 149.8 | ±1.2 % |
|           |                                               | Y | 4.72  | 65.8 | 19.2 |      | 113.3 |        |
|           |                                               | Z | 5.09  | 66.4 | 19.1 |      | 126.0 |        |
| 10181-CAB | LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)         | X | 4.83  | 66.0 | 18.9 | 5.72 | 146.3 | ±1.2 % |
|           |                                               | Y | 4.69  | 65.6 | 19.1 |      | 112.2 |        |
|           |                                               | Z | 5.02  | 66.1 | 19.0 |      | 125.1 |        |
| 10193-CAA | IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)  | X | 9.51  | 67.4 | 20.2 | 8.09 | 108.6 | ±2.5 % |
|           |                                               | Y | 9.72  | 68.1 | 20.9 |      | 118.2 |        |
|           |                                               | Z | 10.30 | 68.9 | 21.1 |      | 135.0 |        |

|           |                                                           |   |       |      |      |      |       |        |
|-----------|-----------------------------------------------------------|---|-------|------|------|------|-------|--------|
| 10196-CAA | IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)                   | X | 9.52  | 67.4 | 20.2 | 8.10 | 111.6 | ±2.5 % |
|           |                                                           | Y | 9.79  | 68.3 | 21.1 |      | 121.3 |        |
|           |                                                           | Z | 10.30 | 68.9 | 21.2 |      | 139.2 |        |
| 10219-CAA | IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)                   | X | 9.47  | 67.4 | 20.2 | 8.03 | 111.8 | ±2.2 % |
|           |                                                           | Y | 9.67  | 68.3 | 21.0 |      | 120.0 |        |
|           |                                                           | Z | 10.20 | 68.9 | 21.1 |      | 138.0 |        |
| 10222-CAA | IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)                    | X | 9.96  | 67.9 | 20.4 | 8.06 | 118.4 | ±2.5 % |
|           |                                                           | Y | 10.25 | 68.8 | 21.2 |      | 128.2 |        |
|           |                                                           | Z | 10.65 | 69.3 | 21.3 |      | 144.5 |        |
| 10225-CAA | UMTS-FDD (HSPA+)                                          | X | 6.96  | 66.7 | 18.9 | 5.97 | 140.0 | ±1.4 % |
|           |                                                           | Y | 7.23  | 67.9 | 20.0 |      | 148.9 |        |
|           |                                                           | Z | 7.03  | 66.4 | 18.9 |      | 115.6 |        |
| 10237-CAB | LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)                     | X | 5.51  | 67.5 | 21.8 | 9.21 | 114.2 | ±1.9 % |
|           |                                                           | Y | 5.82  | 69.4 | 23.4 |      | 123.0 |        |
|           |                                                           | Z | 6.49  | 70.6 | 23.6 |      | 140.2 |        |
| 10252-CAB | LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)                   | X | 6.83  | 67.1 | 21.4 | 9.24 | 136.6 | ±1.9 % |
|           |                                                           | Y | 7.30  | 69.4 | 23.2 |      | 147.3 |        |
|           |                                                           | Z | 7.36  | 68.1 | 22.0 |      | 117.5 |        |
| 10267-CAB | LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)                  | X | 7.26  | 67.5 | 21.6 | 9.30 | 142.7 | ±1.9 % |
|           |                                                           | Y | 7.44  | 68.4 | 22.4 |      | 110.5 |        |
|           |                                                           | Z | 7.84  | 68.7 | 22.2 |      | 122.6 |        |
| 10274-CAA | UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)                 | X | 5.86  | 66.2 | 18.2 | 4.87 | 135.4 | ±0.9 % |
|           |                                                           | Y | 6.12  | 67.5 | 19.2 |      | 142.3 |        |
|           |                                                           | Z | 5.91  | 65.9 | 18.2 |      | 107.6 |        |
| 10275-CAA | UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)                  | X | 4.17  | 64.8 | 17.3 | 3.96 | 115.6 | ±0.7 % |
|           |                                                           | Y | 4.42  | 66.4 | 18.5 |      | 124.6 |        |
|           |                                                           | Z | 4.47  | 66.0 | 18.0 |      | 132.6 |        |
| 10291-AAA | CDMA2000, RC3, SO55, Full Rate                            | X | 3.36  | 64.7 | 17.1 | 3.46 | 109.4 | ±0.5 % |
|           |                                                           | Y | 3.55  | 66.2 | 18.3 |      | 118.2 |        |
|           |                                                           | Z | 3.60  | 65.6 | 17.7 |      | 120.9 |        |
| 10292-AAA | CDMA2000, RC3, SO32, Full Rate                            | X | 3.34  | 64.9 | 17.2 | 3.39 | 110.1 | ±0.5 % |
|           |                                                           | Y | 3.57  | 66.7 | 18.5 |      | 121.0 |        |
|           |                                                           | Z | 3.54  | 65.6 | 17.7 |      | 123.9 |        |
| 10297-AAA | LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)                   | X | 6.14  | 65.8 | 18.6 | 5.81 | 125.1 | ±1.2 % |
|           |                                                           | Y | 6.44  | 67.2 | 19.7 |      | 135.7 |        |
|           |                                                           | Z | 6.52  | 67.0 | 19.3 |      | 142.2 |        |
| 10311-AAA | LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)                  | X | 6.76  | 66.6 | 19.1 | 6.06 | 131.8 | ±1.4 % |
|           |                                                           | Y | 7.03  | 67.8 | 20.0 |      | 142.5 |        |
|           |                                                           | Z | 7.15  | 67.7 | 19.7 |      | 148.6 |        |
| 10315-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle) | X | 2.42  | 64.6 | 16.1 | 1.71 | 116.8 | ±0.5 % |
|           |                                                           | Y | 3.00  | 69.3 | 19.0 |      | 126.9 |        |
|           |                                                           | Z | 2.61  | 66.3 | 17.2 |      | 128.2 |        |
| 10317-AAA | IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)   | X | 9.71  | 67.6 | 20.5 | 8.36 | 111.7 | ±2.5 % |
|           |                                                           | Y | 9.99  | 68.6 | 21.4 |      | 122.2 |        |
|           |                                                           | Z | 10.38 | 68.9 | 21.3 |      | 129.5 |        |

|           |                                                     |   |       |      |      |      |       |        |
|-----------|-----------------------------------------------------|---|-------|------|------|------|-------|--------|
| 10400-AAA | IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle) | X | 9.83  | 67.8 | 20.6 | 8.37 | 112.9 | ±2.5 % |
|           |                                                     | Y | 10.09 | 68.7 | 21.4 |      | 123.9 |        |
|           |                                                     | Z | 10.48 | 68.9 | 21.3 |      | 130.5 |        |
| 10402-AAA | IEEE 802.11ac WiFi (80MHz, 64-QAM, 99pc duty cycle) | X | 10.61 | 68.3 | 20.7 | 8.53 | 121.1 | ±2.5 % |
|           |                                                     | Y | 11.25 | 70.0 | 21.9 |      | 135.4 |        |
|           |                                                     | Z | 11.15 | 69.4 | 21.4 |      | 137.4 |        |
| 10403-AAA | CDMA2000 (1xEV-DO, Rev. 0)                          | X | 4.51  | 67.4 | 17.8 | 3.76 | 119.2 | ±0.5 % |
|           |                                                     | Y | 4.91  | 69.5 | 19.3 |      | 128.3 |        |
|           |                                                     | Z | 4.84  | 67.5 | 18.1 |      | 135.4 |        |
| 10404-AAA | CDMA2000 (1xEV-DO, Rev. A)                          | X | 4.51  | 67.7 | 18.0 | 3.77 | 117.4 | ±0.5 % |
|           |                                                     | Y | 4.92  | 69.8 | 19.5 |      | 125.4 |        |
|           |                                                     | Z | 4.71  | 67.3 | 18.0 |      | 131.9 |        |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 8 and 9).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3914

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 41.9                               | 0.89                            | 9.70    | 9.70    | 9.70    | 0.34               | 1.01                    | ± 12.0 %    |
| 835                  | 41.5                               | 0.90                            | 9.34    | 9.34    | 9.34    | 0.67               | 0.67                    | ± 12.0 %    |
| 1750                 | 40.1                               | 1.37                            | 7.99    | 7.99    | 7.99    | 0.79               | 0.56                    | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 7.69    | 7.69    | 7.69    | 0.80               | 0.58                    | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 6.95    | 6.95    | 6.95    | 0.41               | 0.77                    | ± 12.0 %    |
| 2600                 | 39.0                               | 1.96                            | 6.79    | 6.79    | 6.79    | 0.40               | 0.82                    | ± 12.0 %    |
| 5200                 | 36.0                               | 4.66                            | 4.99    | 4.99    | 4.99    | 0.30               | 1.80                    | ± 13.1 %    |
| 5300                 | 35.9                               | 4.76                            | 4.82    | 4.82    | 4.82    | 0.30               | 1.80                    | ± 13.1 %    |
| 5500                 | 35.6                               | 4.96                            | 4.55    | 4.55    | 4.55    | 0.35               | 1.80                    | ± 13.1 %    |
| 5600                 | 35.5                               | 5.07                            | 4.37    | 4.37    | 4.37    | 0.35               | 1.80                    | ± 13.1 %    |
| 5800                 | 35.3                               | 5.27                            | 4.52    | 4.52    | 4.52    | 0.35               | 1.80                    | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3914

### Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 55.5                               | 0.96                            | 9.39    | 9.39    | 9.39    | 0.63               | 0.74                    | ± 12.0 %    |
| 835                  | 55.2                               | 0.97                            | 9.31    | 9.31    | 9.31    | 0.56               | 0.76                    | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 7.89    | 7.89    | 7.89    | 0.32               | 1.03                    | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 7.51    | 7.51    | 7.51    | 0.51               | 0.76                    | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 7.02    | 7.02    | 7.02    | 0.80               | 0.50                    | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 6.81    | 6.81    | 6.81    | 0.80               | 0.50                    | ± 12.0 %    |
| 5200                 | 49.0                               | 5.30                            | 4.52    | 4.52    | 4.52    | 0.35               | 1.90                    | ± 13.1 %    |
| 5300                 | 48.9                               | 5.42                            | 4.32    | 4.32    | 4.32    | 0.35               | 1.90                    | ± 13.1 %    |
| 5500                 | 48.6                               | 5.65                            | 4.07    | 4.07    | 4.07    | 0.35               | 1.90                    | ± 13.1 %    |
| 5600                 | 48.5                               | 5.77                            | 3.97    | 3.97    | 3.97    | 0.35               | 1.90                    | ± 13.1 %    |
| 5800                 | 48.2                               | 6.00                            | 4.14    | 4.14    | 4.14    | 0.40               | 1.90                    | ± 13.1 %    |


<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## Frequency Response of E-Field


(TEM-Cell: ifi110 EXX, Waveguide: R22)

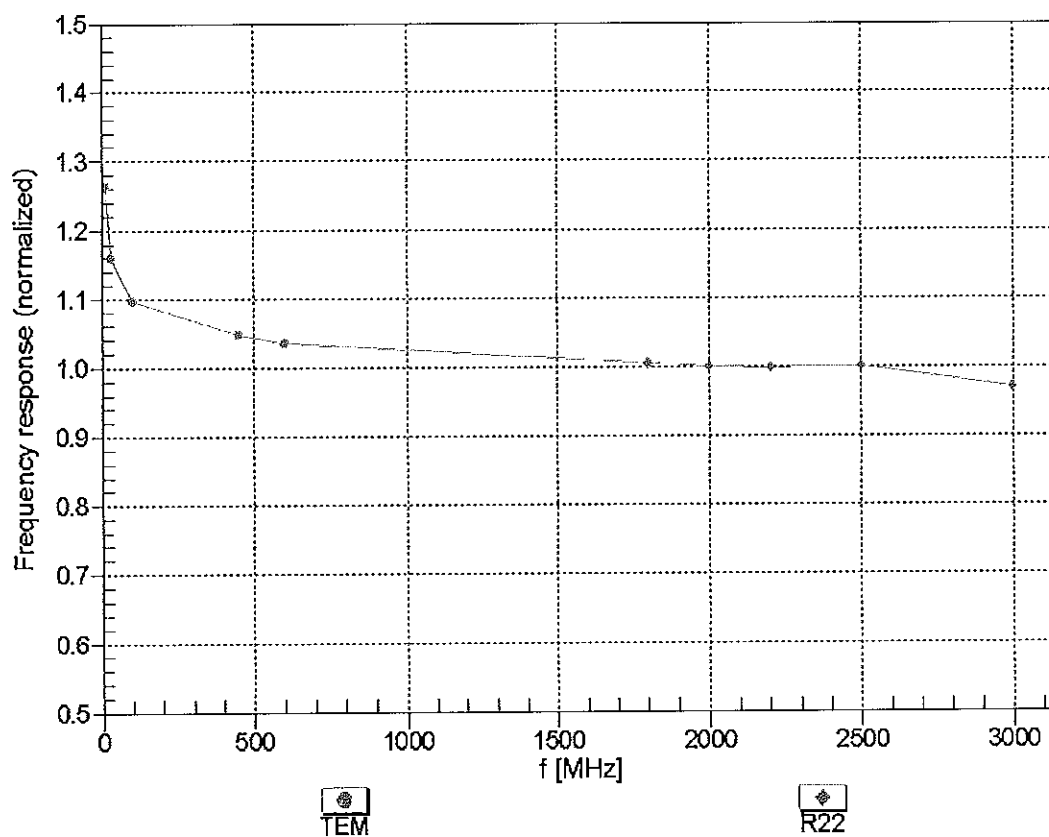



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

$f=600$  MHz, TEM


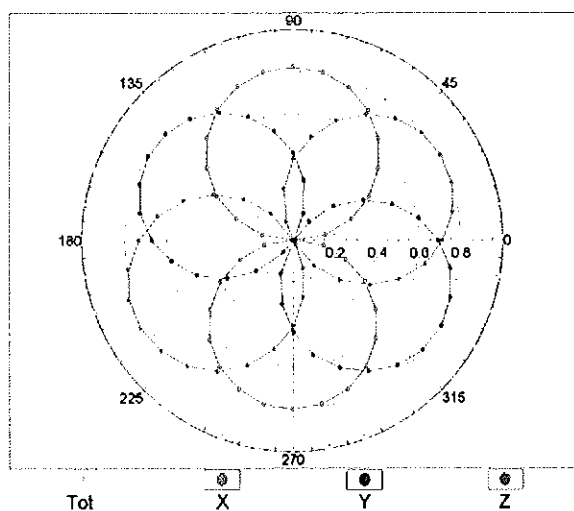


$f=1800$  MHz, R22

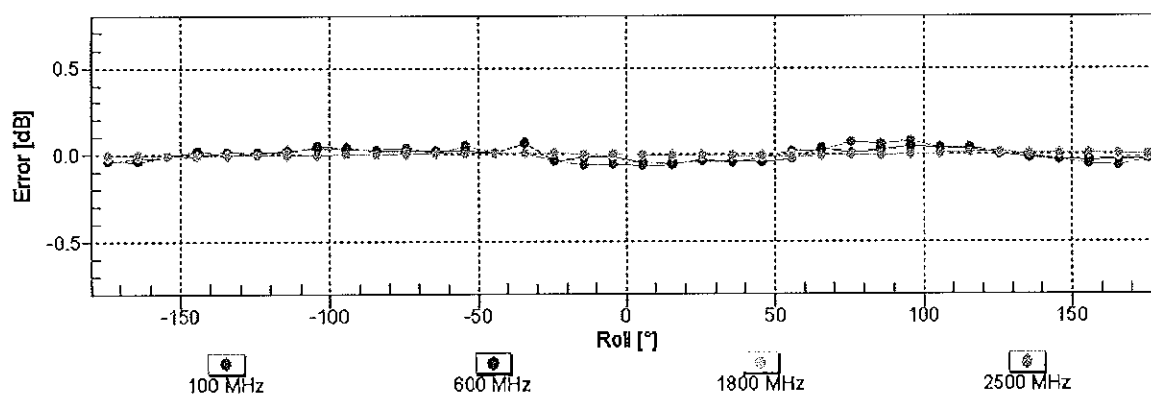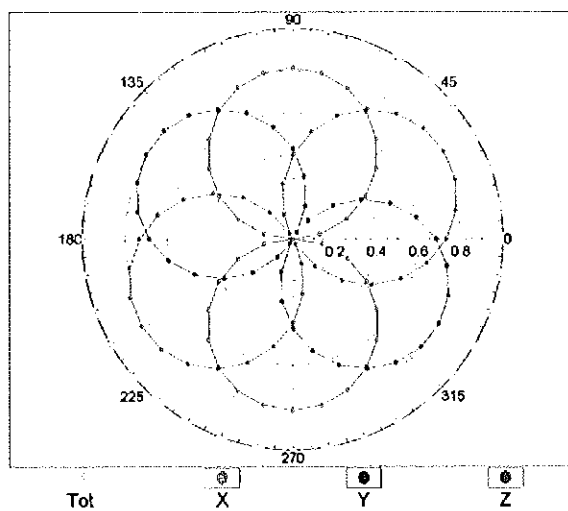

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )


# Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f = 900 \text{ MHz}$ )

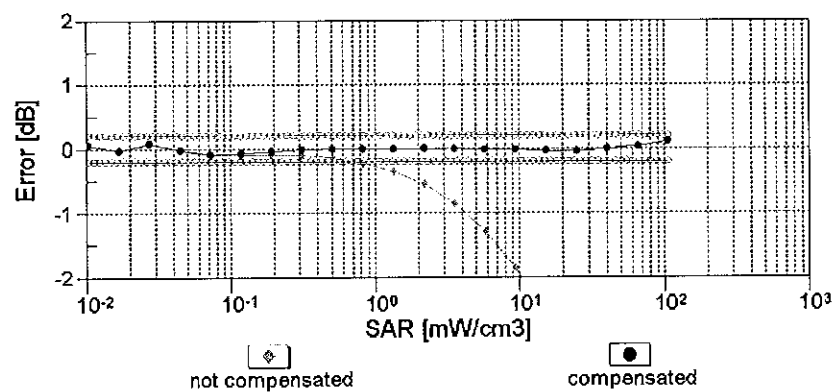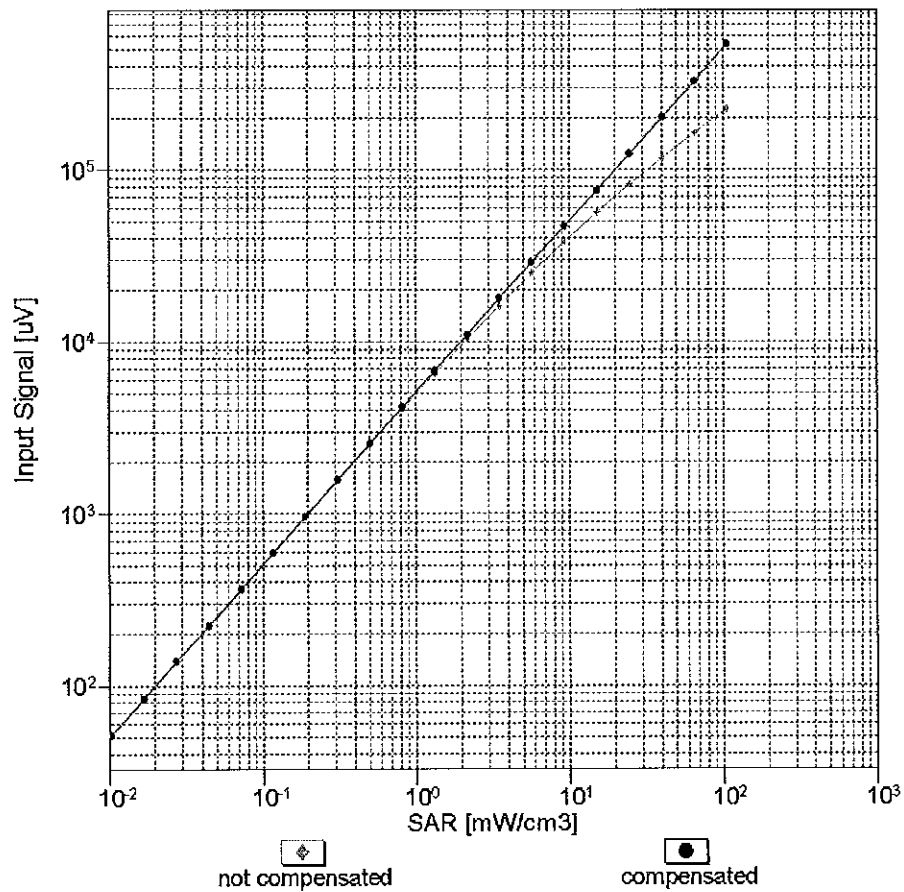

Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )





## Conversion Factor Assessment

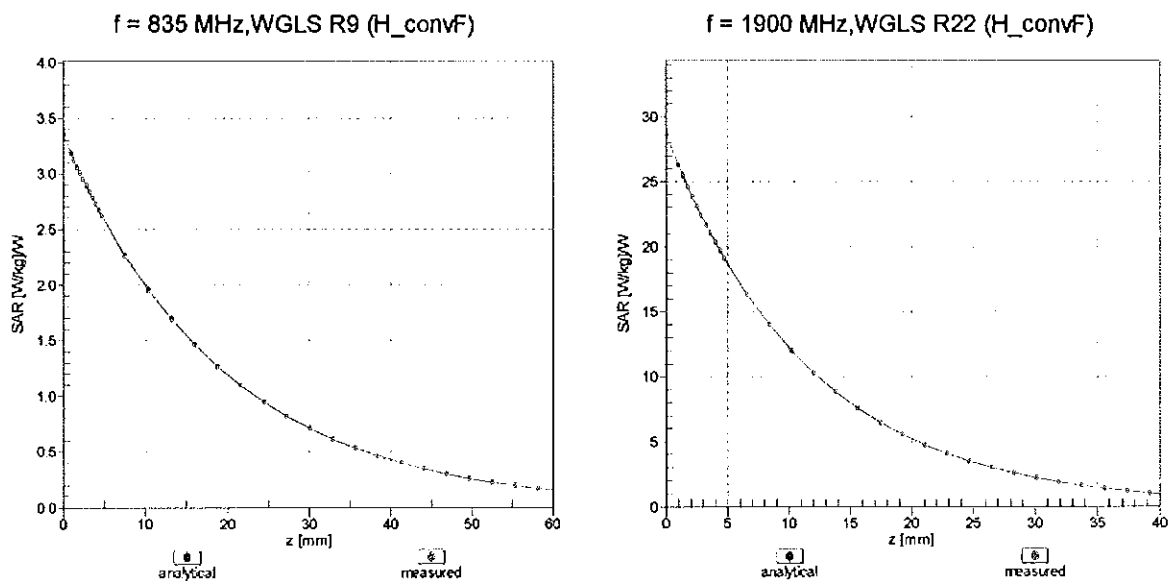

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

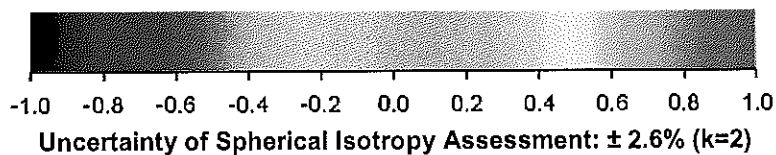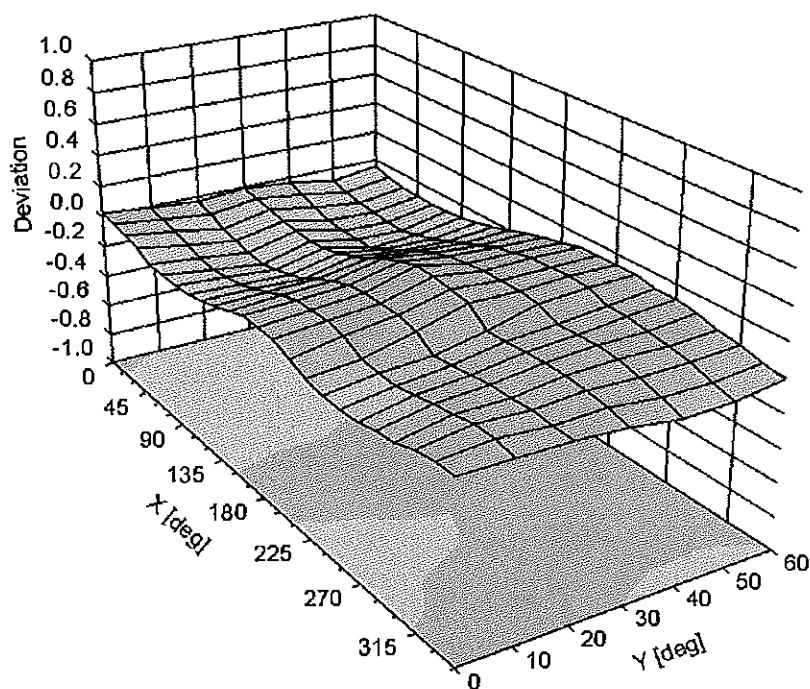

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3914

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -24.3      |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 9 mm       |
| Tip Diameter                                  | 2.5 mm     |
| Probe Tip to Sensor X Calibration Point       | 1 mm       |
| Probe Tip to Sensor Y Calibration Point       | 1 mm       |
| Probe Tip to Sensor Z Calibration Point       | 1 mm       |
| Recommended Measurement Distance from Surface | 2 mm       |



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **EX3-3589\_Jan14**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3589**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **January 29, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 30-Dec-13 (No. ES3-3013_Dec13)    | Dec-14                 |
| DAE4                       | SN: 660         | 13-Dec-13 (No. DAE4-660_Dec13)    | Dec-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-16 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

|                |                 |                       |           |
|----------------|-----------------|-----------------------|-----------|
| Calibrated by: | Name            | Function              | Signature |
|                | Claudio Leubler | Laboratory Technician |           |
| Approved by:   | Name            | Function              | Signature |
|                | Katja Pokovic   | Technical Manager     |           |

Issued: January 30, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C, D               | modulation dependent linearization parameters                                                                                                           |
| Polarization $\varphi$   | $\varphi$ rotation around probe axis                                                                                                                    |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |
| Connector Angle          | information used in DASY system to align probe sensor X to the robot coordinate system                                                                  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

# Probe EX3DV4

## SN:3589

Manufactured: March 30, 2006  
Calibrated: January 29, 2014

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3589

### Basic Calibration Parameters

|                                       | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---------------------------------------|----------|----------|----------|-----------|
| Norm ( $\mu V/(V/m)^2$ ) <sup>A</sup> | 0.46     | 0.40     | 0.40     | ± 10.1 %  |
| DCP (mV) <sup>B</sup>                 | 101.2    | 100.8    | 98.0     |           |

### Modulation Calibration Parameters

| UID       | Communication System Name                |   | A<br>dB | B<br>dB $\sqrt{\mu V}$ | C    | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----------|------------------------------------------|---|---------|------------------------|------|---------|----------|---------------------------|
| 0         | CW                                       | X | 0.0     | 0.0                    | 1.0  | 0.00    | 150.4    | ±3.8 %                    |
|           |                                          | Y | 0.0     | 0.0                    | 1.0  |         | 142.3    |                           |
|           |                                          | Z | 0.0     | 0.0                    | 1.0  |         | 171.7    |                           |
| 10010-CAA | SAR Validation (Square, 100ms, 10ms)     | X | 6.00    | 69.5                   | 14.2 | 10.00   | 42.1     | ±0.9 %                    |
|           |                                          | Y | 7.03    | 71.8                   | 15.0 |         | 40.3     |                           |
|           |                                          | Z | 3.33    | 64.6                   | 12.1 |         | 44.6     |                           |
| 10011-CAA | UMTS-FDD (WCDMA)                         | X | 3.26    | 66.2                   | 17.8 | 2.91    | 117.6    | ±0.9 %                    |
|           |                                          | Y | 3.38    | 66.8                   | 18.2 |         | 113.0    |                           |
|           |                                          | Z | 2.79    | 62.4                   | 14.7 |         | 133.2    |                           |
| 10012-CAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps) | X | 2.77    | 66.8                   | 17.4 | 1.87    | 117.4    | ±0.7 %                    |
|           |                                          | Y | 3.22    | 69.6                   | 18.8 |         | 113.5    |                           |
|           |                                          | Z | 2.22    | 62.0                   | 13.8 |         | 135.2    |                           |
| 10021-DAA | GSM-FDD (TDMA, GMSK)                     | X | 3.61    | 69.7                   | 16.6 | 9.39    | 91.2     | ±1.7 %                    |
|           |                                          | Y | 5.48    | 77.1                   | 19.6 |         | 125.1    |                           |
|           |                                          | Z | 2.18    | 62.5                   | 12.6 |         | 75.3     |                           |
| 10023-DAA | GPRS-FDD (TDMA, GMSK, TN 0)              | X | 3.01    | 66.4                   | 14.9 | 9.57    | 86.1     | ±2.7 %                    |
|           |                                          | Y | 7.02    | 82.0                   | 22.0 |         | 120.5    |                           |
|           |                                          | Z | 2.13    | 62.9                   | 12.7 |         | 71.4     |                           |
| 10024-DAA | GPRS-FDD (TDMA, GMSK, TN 0-1)            | X | 18.01   | 91.8                   | 22.6 | 6.56    | 132.3    | ±1.7 %                    |
|           |                                          | Y | 8.55    | 83.0                   | 19.9 |         | 134.3    |                           |
|           |                                          | Z | 4.04    | 72.4                   | 15.7 |         | 139.6    |                           |
| 10027-DAA | GPRS-FDD (TDMA, GMSK, TN 0-1-2)          | X | 4.70    | 74.7                   | 15.9 | 4.80    | 107.5    | ±1.7 %                    |
|           |                                          | Y | 4.94    | 76.1                   | 16.4 |         | 107.8    |                           |
|           |                                          | Z | 2.97    | 68.7                   | 12.8 |         | 127.1    |                           |
| 10028-DAA | GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)        | X | 67.89   | 99.9                   | 21.4 | 3.55    | 114.7    | ±2.7 %                    |
|           |                                          | Y | 48.02   | 99.7                   | 21.9 |         | 116.6    |                           |
|           |                                          | Z | 1.36    | 61.4                   | 7.8  |         | 134.4    |                           |
| 10032-CAA | IEEE 802.15.1 Bluetooth (GFSK, DH5)      | X | 97.41   | 97.0                   | 17.7 | 1.16    | 129.2    | ±3.0 %                    |
|           |                                          | Y | 71.47   | 99.8                   | 19.3 |         | 130.9    |                           |
|           |                                          | Z | 0.29    | 53.5                   | 0.9  |         | 109.2    |                           |
| 10039-CAA | CDMA2000 (1xRTT, RC1)                    | X | 4.62    | 65.4                   | 18.0 | 4.57    | 113.0    | ±1.7 %                    |
|           |                                          | Y | 4.74    | 66.1                   | 18.4 |         | 111.5    |                           |
|           |                                          | Z | 4.22    | 63.3                   | 15.9 |         | 133.6    |                           |
| 10062-CAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps) | X | 10.10   | 67.8                   | 20.8 | 8.68    | 108.0    | ±2.7 %                    |
|           |                                          | Y | 10.07   | 68.1                   | 21.1 |         | 108.1    |                           |
|           |                                          | Z | 10.03   | 67.6                   | 20.2 |         | 130.3    |                           |

|           |                                               |   |       |      |      |      |       |        |
|-----------|-----------------------------------------------|---|-------|------|------|------|-------|--------|
| 10098-CAA | UMTS-FDD (HSUPA, Subtest 2)                   | X | 4.53  | 65.7 | 17.8 | 3.98 | 122.5 | ±0.9 % |
|           |                                               | Y | 4.72  | 66.6 | 18.4 |      | 123.1 |        |
|           |                                               | Z | 4.38  | 64.5 | 16.7 |      | 147.3 |        |
| 10100-CAB | LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)      | X | 6.32  | 66.5 | 18.8 | 5.67 | 126.9 | ±1.2 % |
|           |                                               | Y | 6.50  | 67.2 | 19.4 |      | 128.9 |        |
|           |                                               | Z | 5.80  | 64.3 | 17.3 |      | 107.2 |        |
| 10108-CAB | LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)      | X | 6.22  | 66.1 | 18.8 | 5.80 | 124.2 | ±1.7 % |
|           |                                               | Y | 6.39  | 66.9 | 19.4 |      | 126.7 |        |
|           |                                               | Z | 6.10  | 65.2 | 17.7 |      | 149.4 |        |
| 10110-CAB | LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)       | X | 5.94  | 65.8 | 18.7 | 5.75 | 121.3 | ±1.7 % |
|           |                                               | Y | 6.05  | 66.3 | 19.1 |      | 123.1 |        |
|           |                                               | Z | 5.80  | 65.0 | 17.7 |      | 144.5 |        |
| 10114-CAA | IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK) | X | 10.01 | 67.7 | 20.3 | 8.10 | 113.9 | ±2.5 % |
|           |                                               | Y | 10.16 | 68.3 | 20.8 |      | 117.0 |        |
|           |                                               | Z | 9.96  | 67.5 | 19.8 |      | 135.3 |        |
| 10117-CAA | IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)      | X | 10.07 | 67.9 | 20.4 | 8.07 | 115.2 | ±2.5 % |
|           |                                               | Y | 10.16 | 68.2 | 20.7 |      | 118.4 |        |
|           |                                               | Z | 10.02 | 67.7 | 19.9 |      | 138.0 |        |
| 10151-CAB | LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)       | X | 7.89  | 68.4 | 21.8 | 9.28 | 108.1 | ±1.9 % |
|           |                                               | Y | 8.15  | 69.7 | 22.8 |      | 109.4 |        |
|           |                                               | Z | 7.38  | 66.5 | 20.4 |      | 123.2 |        |
| 10154-CAB | LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)       | X | 5.94  | 65.7 | 18.6 | 5.75 | 122.1 | ±1.7 % |
|           |                                               | Y | 6.03  | 66.3 | 19.0 |      | 122.5 |        |
|           |                                               | Z | 5.79  | 65.0 | 17.7 |      | 144.0 |        |
| 10160-CAB | LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)       | X | 6.38  | 66.3 | 18.9 | 5.82 | 126.0 | ±1.7 % |
|           |                                               | Y | 6.54  | 67.0 | 19.4 |      | 128.2 |        |
|           |                                               | Z | 6.16  | 65.3 | 17.8 |      | 146.9 |        |
| 10169-CAB | LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)         | X | 5.17  | 66.5 | 19.2 | 5.73 | 149.7 | ±1.2 % |
|           |                                               | Y | 4.95  | 65.8 | 19.0 |      | 108.3 |        |
|           |                                               | Z | 4.64  | 63.9 | 17.1 |      | 125.3 |        |
| 10172-CAB | LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)         | X | 6.79  | 70.4 | 23.0 | 9.21 | 120.6 | ±3.0 % |
|           |                                               | Y | 6.96  | 72.0 | 24.2 |      | 122.8 |        |
|           |                                               | Z | 6.43  | 69.3 | 22.0 |      | 136.7 |        |
| 10175-CAB | LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)         | X | 5.15  | 66.4 | 19.1 | 5.72 | 143.0 | ±1.4 % |
|           |                                               | Y | 5.23  | 67.1 | 19.6 |      | 145.8 |        |
|           |                                               | Z | 4.60  | 63.7 | 17.0 |      | 121.1 |        |
| 10181-CAB | LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)         | X | 5.11  | 66.2 | 19.0 | 5.72 | 141.0 | ±1.4 % |
|           |                                               | Y | 5.27  | 67.3 | 19.7 |      | 144.9 |        |
|           |                                               | Z | 4.54  | 63.4 | 16.8 |      | 119.2 |        |
| 10193-CAA | IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)  | X | 9.57  | 67.1 | 20.1 | 8.09 | 102.2 | ±2.2 % |
|           |                                               | Y | 9.59  | 67.4 | 20.4 |      | 105.3 |        |
|           |                                               | Z | 9.73  | 67.6 | 20.0 |      | 129.6 |        |
| 10196-CAA | IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)       | X | 9.61  | 67.3 | 20.2 | 8.10 | 104.6 | ±2.5 % |
|           |                                               | Y | 9.63  | 67.6 | 20.5 |      | 107.8 |        |
|           |                                               | Z | 9.63  | 67.3 | 19.8 |      | 130.9 |        |

|           |                                                           |   |       |      |      |      |       |        |
|-----------|-----------------------------------------------------------|---|-------|------|------|------|-------|--------|
| 10219-CAA | IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)                   | X | 9.61  | 67.5 | 20.3 | 8.03 | 109.2 | ±2.7 % |
|           |                                                           | Y | 9.54  | 67.5 | 20.4 |      | 107.4 |        |
|           |                                                           | Z | 9.53  | 67.2 | 19.7 |      | 130.7 |        |
| 10222-CAA | IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)                    | X | 10.00 | 67.8 | 20.4 | 8.06 | 114.1 | ±2.7 % |
|           |                                                           | Y | 10.01 | 68.0 | 20.6 |      | 112.3 |        |
|           |                                                           | Z | 9.96  | 67.6 | 19.9 |      | 137.1 |        |
| 10225-CAA | UMTS-FDD (HSPA+)                                          | X | 7.18  | 66.9 | 19.2 | 5.97 | 137.5 | ±1.4 % |
|           |                                                           | Y | 7.25  | 67.4 | 19.5 |      | 134.4 |        |
|           |                                                           | Z | 6.48  | 64.4 | 17.3 |      | 114.6 |        |
| 10237-CAB | LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)                     | X | 6.93  | 71.0 | 23.5 | 9.21 | 123.5 | ±3.0 % |
|           |                                                           | Y | 6.88  | 71.6 | 24.0 |      | 119.3 |        |
|           |                                                           | Z | 6.63  | 70.1 | 22.4 |      | 141.3 |        |
| 10252-CAB | LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)                   | X | 8.19  | 70.5 | 23.1 | 9.24 | 142.9 | ±2.5 % |
|           |                                                           | Y | 8.46  | 72.0 | 24.2 |      | 143.3 |        |
|           |                                                           | Z | 7.10  | 67.0 | 20.8 |      | 119.9 |        |
| 10267-CAB | LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)                  | X | 7.83  | 68.1 | 21.6 | 9.30 | 104.2 | ±2.2 % |
|           |                                                           | Y | 8.07  | 69.4 | 22.7 |      | 103.0 |        |
|           |                                                           | Z | 7.49  | 67.2 | 20.9 |      | 125.2 |        |
| 10274-CAA | UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)                 | X | 5.96  | 66.2 | 18.3 | 4.87 | 128.1 | ±1.7 % |
|           |                                                           | Y | 6.12  | 67.0 | 18.8 |      | 126.0 |        |
|           |                                                           | Z | 5.31  | 63.8 | 16.4 |      | 110.2 |        |
| 10275-CAA | UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)                  | X | 4.30  | 65.5 | 17.8 | 3.96 | 110.5 | ±1.2 % |
|           |                                                           | Y | 4.47  | 66.4 | 18.4 |      | 110.3 |        |
|           |                                                           | Z | 3.92  | 63.1 | 15.6 |      | 135.7 |        |
| 10291-AAA | CDMA2000, RC3, SO55, Full Rate                            | X | 3.59  | 65.7 | 17.7 | 3.46 | 138.1 | ±1.2 % |
|           |                                                           | Y | 3.85  | 67.2 | 18.6 |      | 146.7 |        |
|           |                                                           | Z | 3.08  | 61.7 | 14.7 |      | 123.3 |        |
| 10292-AAA | CDMA2000, RC3, SO32, Full Rate                            | X | 3.59  | 66.0 | 17.8 | 3.39 | 144.2 | ±0.9 % |
|           |                                                           | Y | 3.83  | 67.5 | 18.7 |      | 148.4 |        |
|           |                                                           | Z | 3.18  | 63.1 | 15.7 |      | 128.6 |        |
| 10297-AAA | LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)                   | X | 6.13  | 65.8 | 18.7 | 5.81 | 116.5 | ±1.7 % |
|           |                                                           | Y | 6.30  | 66.6 | 19.2 |      | 119.4 |        |
|           |                                                           | Z | 6.20  | 65.9 | 18.4 |      | 145.6 |        |
| 10311-AAA | LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)                  | X | 6.70  | 66.4 | 19.0 | 6.06 | 122.5 | ±1.4 % |
|           |                                                           | Y | 6.92  | 67.3 | 19.6 |      | 124.5 |        |
|           |                                                           | Z | 6.28  | 65.0 | 17.9 |      | 103.7 |        |
| 10315-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle) | X | 2.66  | 66.7 | 17.4 | 1.71 | 109.5 | ±0.7 % |
|           |                                                           | Y | 3.18  | 70.0 | 19.2 |      | 111.5 |        |
|           |                                                           | Z | 2.08  | 61.6 | 13.4 |      | 134.4 |        |
| 10317-AAA | IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)   | X | 9.78  | 67.4 | 20.4 | 8.36 | 103.5 | ±2.5 % |
|           |                                                           | Y | 9.81  | 67.7 | 20.7 |      | 107.1 |        |
|           |                                                           | Z | 9.86  | 67.6 | 20.3 |      | 129.5 |        |
| 10400-AAA | IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)       | X | 9.86  | 67.5 | 20.4 | 8.37 | 104.9 | ±2.7 % |
|           |                                                           | Y | 9.93  | 67.9 | 20.8 |      | 107.9 |        |
|           |                                                           | Z | 9.97  | 67.7 | 20.2 |      | 134.3 |        |



|           |                                                     |   |       |      |      |      |       |        |
|-----------|-----------------------------------------------------|---|-------|------|------|------|-------|--------|
| 10402-AAA | IEEE 802.11ac WiFi (80MHz, 64-QAM, 99pc duty cycle) | X | 10.47 | 67.9 | 20.5 | 8.53 | 109.9 | ±3.0 % |
|           |                                                     | Y | 10.86 | 68.8 | 21.1 |      | 116.0 |        |
|           |                                                     | Z | 10.68 | 68.2 | 20.4 |      | 142.5 |        |
| 10403-AAA | CDMA2000 (1xEV-DO, Rev. 0)                          | X | 4.74  | 67.0 | 17.9 | 3.76 | 114.9 | ±0.9 % |
|           |                                                     | Y | 5.02  | 68.5 | 18.7 |      | 116.6 |        |
|           |                                                     | Z | 4.23  | 64.4 | 15.8 |      | 145.1 |        |
| 10404-AAA | CDMA2000 (1xEV-DO, Rev. A)                          | X | 4.71  | 67.1 | 17.9 | 3.77 | 112.3 | ±1.4 % |
|           |                                                     | Y | 4.95  | 68.5 | 18.7 |      | 115.0 |        |
|           |                                                     | Z | 4.01  | 63.4 | 15.1 |      | 138.9 |        |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 8 and 9).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3589

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Uct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|------------|
| 750                  | 41.9                               | 0.89                            | 8.86    | 8.86    | 8.86    | 0.80               | 0.62                    | ± 12.0 %   |
| 835                  | 41.5                               | 0.90                            | 8.49    | 8.49    | 8.49    | 0.45               | 0.82                    | ± 12.0 %   |
| 1750                 | 40.1                               | 1.37                            | 7.31    | 7.31    | 7.31    | 0.80               | 0.60                    | ± 12.0 %   |
| 1900                 | 40.0                               | 1.40                            | 7.05    | 7.05    | 7.05    | 0.52               | 0.73                    | ± 12.0 %   |
| 2450                 | 39.2                               | 1.80                            | 6.45    | 6.45    | 6.45    | 0.29               | 1.08                    | ± 12.0 %   |
| 2600                 | 39.0                               | 1.96                            | 6.24    | 6.24    | 6.24    | 0.76               | 0.62                    | ± 12.0 %   |
| 5200                 | 36.0                               | 4.66                            | 4.78    | 4.78    | 4.78    | 0.30               | 1.80                    | ± 13.1 %   |
| 5300                 | 35.9                               | 4.76                            | 4.58    | 4.58    | 4.58    | 0.30               | 1.80                    | ± 13.1 %   |
| 5500                 | 35.6                               | 4.96                            | 4.44    | 4.44    | 4.44    | 0.31               | 1.80                    | ± 13.1 %   |
| 5600                 | 35.5                               | 5.07                            | 4.20    | 4.20    | 4.20    | 0.35               | 1.80                    | ± 13.1 %   |
| 5800                 | 35.3                               | 5.27                            | 4.39    | 4.39    | 4.39    | 0.32               | 1.80                    | ± 13.1 %   |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3589

### Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 55.5                               | 0.96                            | 8.34    | 8.34    | 8.34    | 0.66               | 0.72                    | ± 12.0 %    |
| 835                  | 55.2                               | 0.97                            | 8.29    | 8.29    | 8.29    | 0.31               | 1.11                    | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 6.68    | 6.68    | 6.68    | 0.80               | 0.61                    | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 6.54    | 6.54    | 6.54    | 0.72               | 0.64                    | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 6.26    | 6.26    | 6.26    | 0.80               | 0.57                    | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 6.08    | 6.08    | 6.08    | 0.68               | 0.50                    | ± 12.0 %    |
| 5200                 | 49.0                               | 5.30                            | 4.19    | 4.19    | 4.19    | 0.38               | 1.90                    | ± 13.1 %    |
| 5300                 | 48.9                               | 5.42                            | 3.98    | 3.98    | 3.98    | 0.38               | 1.90                    | ± 13.1 %    |
| 5500                 | 48.6                               | 5.65                            | 3.76    | 3.76    | 3.76    | 0.42               | 1.90                    | ± 13.1 %    |
| 5600                 | 48.5                               | 5.77                            | 3.81    | 3.81    | 3.81    | 0.30               | 1.90                    | ± 13.1 %    |
| 5800                 | 48.2                               | 6.00                            | 3.97    | 3.97    | 3.97    | 0.43               | 1.90                    | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


**Frequency Response of E-Field**  
(TEM-Cell:ifi110 EXX, Waveguide: R22)

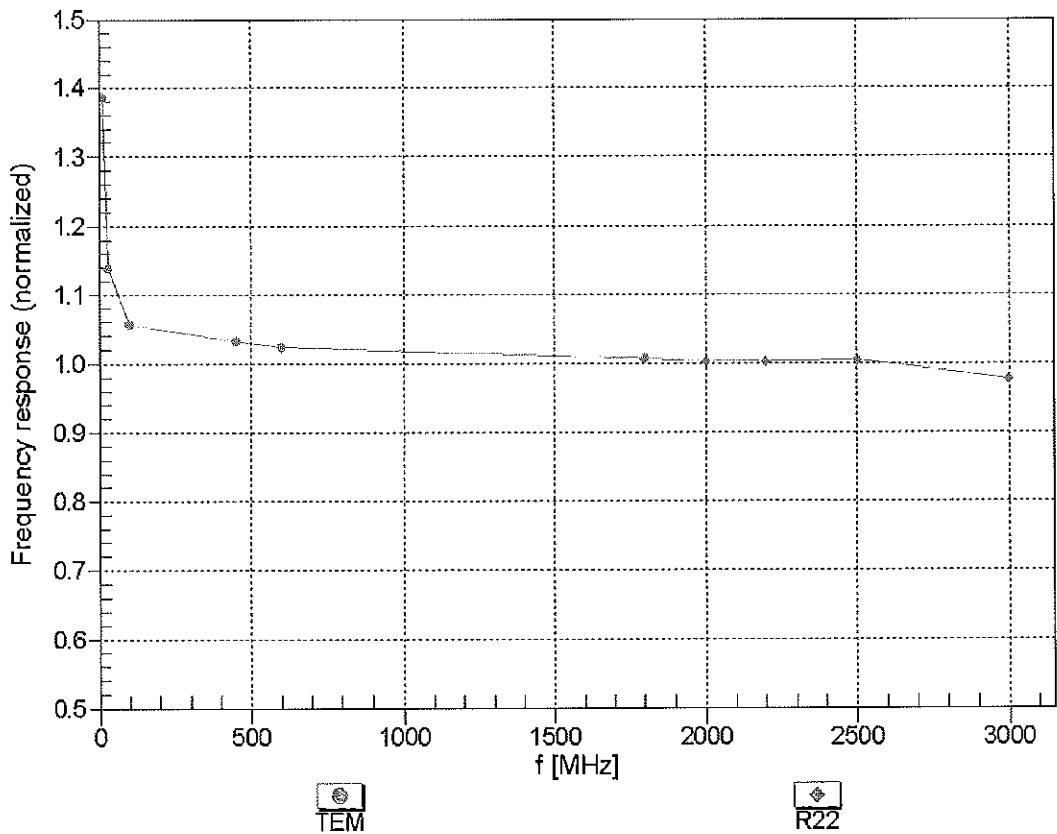



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

f=600 MHz,TEM

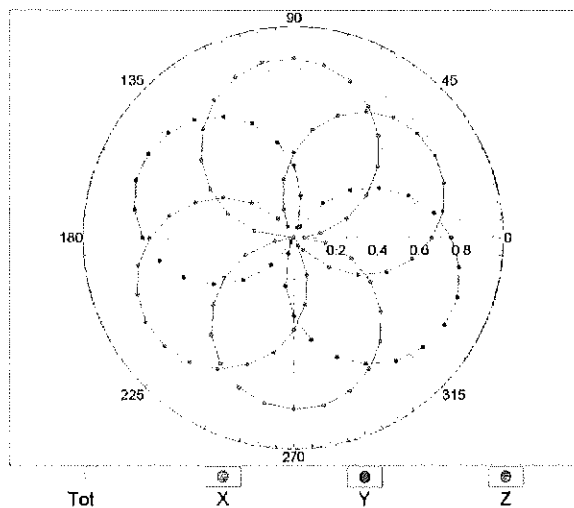


f=1800 MHz,R22

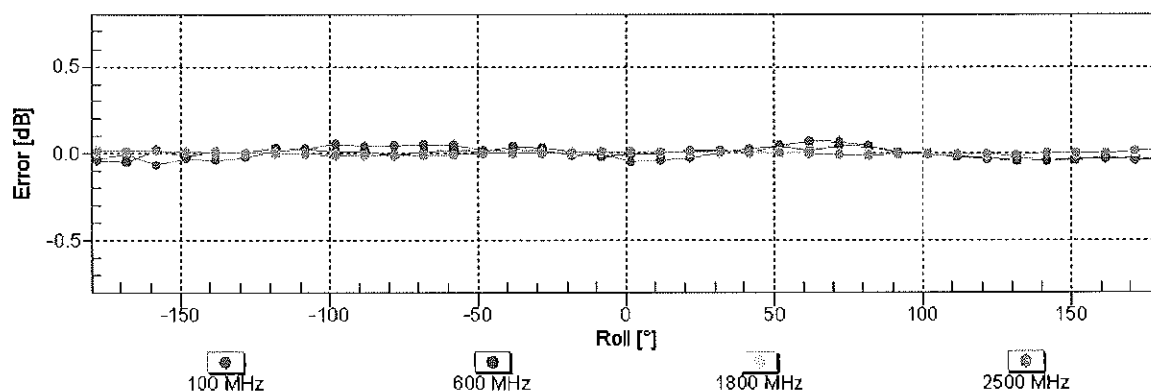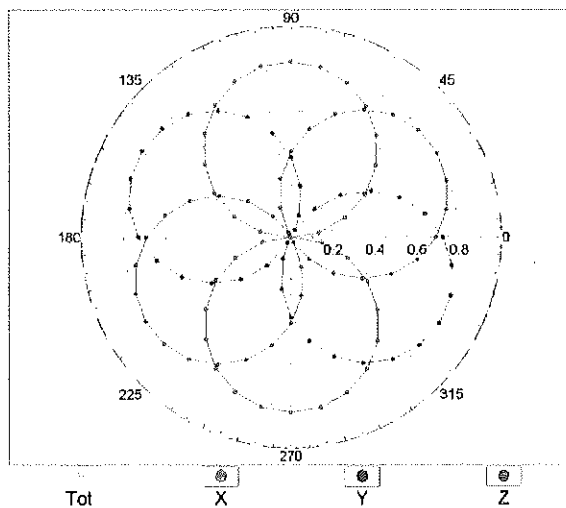

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)


## Dynamic Range f(SAR<sub>head</sub>)

(TEM cell , f = 900 MHz)

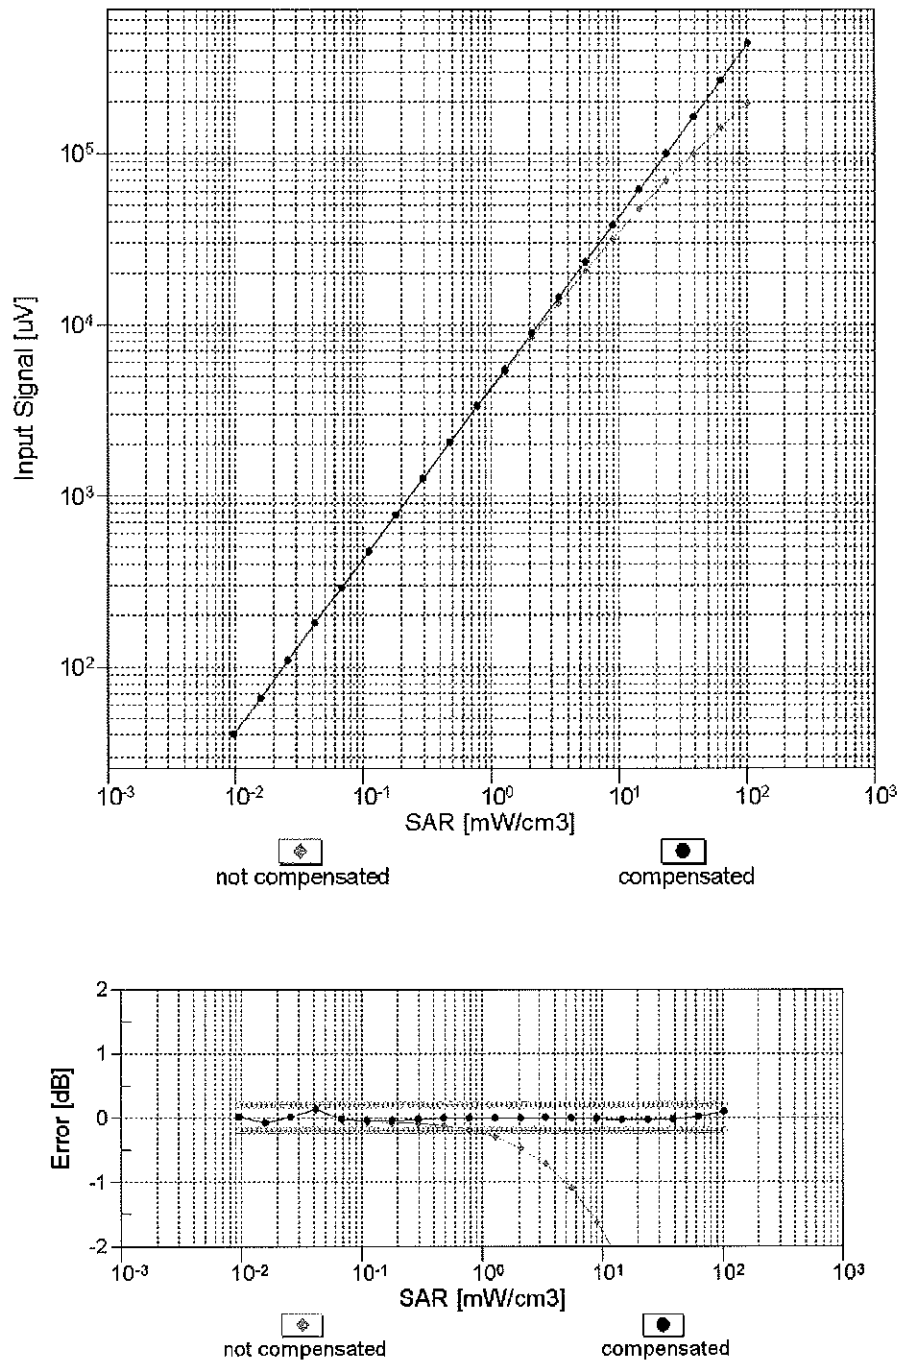


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

# Conversion Factor Assessment

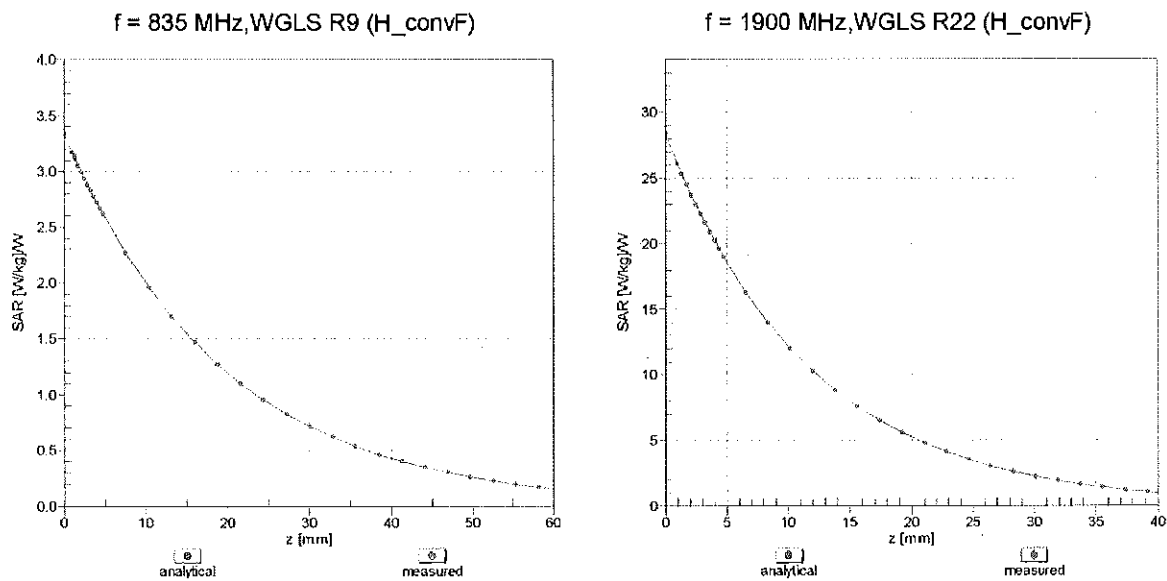

## Deviation from Isotropy in Liquid Error ( $\phi, \vartheta$ ), f = 900 MHz

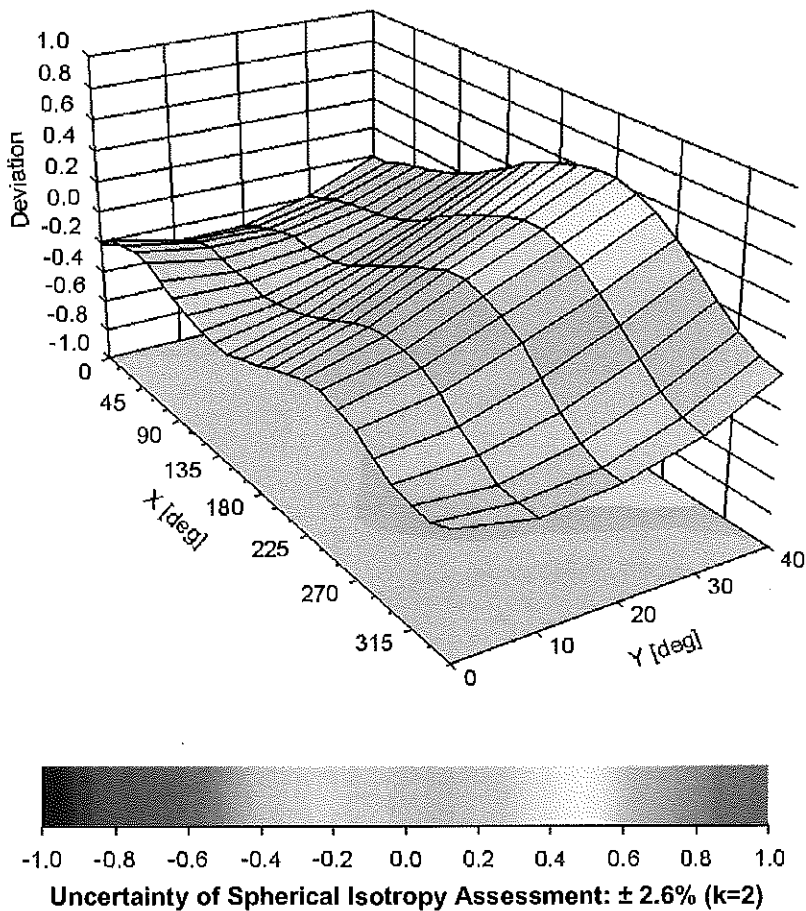

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3589

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -38.2      |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 9 mm       |
| Tip Diameter                                  | 2.5 mm     |
| Probe Tip to Sensor X Calibration Point       | 1 mm       |
| Probe Tip to Sensor Y Calibration Point       | 1 mm       |
| Probe Tip to Sensor Z Calibration Point       | 1 mm       |
| Recommended Measurement Distance from Surface | 2 mm       |



## APPENDIX D: SAR TISSUE SPECIFICATIONS

Measurement Procedure for Tissue verification:

- 1) The network analyzer and probe system was configured and calibrated.
- 2) The probe was immersed in the tissue. The tissue was placed in a nonmetallic container. Trapped air bubbles beneath the flange were minimized by placing the probe at a slight angle.
- 3) The complex admittance with respect to the probe aperture was measured
- 4) The complex relative permittivity  $\epsilon$  can be calculated from the below equation (Pournaropoulos and Misra):

$$Y = \frac{j2\omega\epsilon_r\epsilon_0}{[\ln(b/a)]^2} \int_a^b \int_a^b \int_0^\pi \cos\phi' \frac{\exp[-j\omega r(\mu_0\epsilon_r'\epsilon_0)^{1/2}]}{r} d\phi' d\rho' d\rho$$

where  $Y$  is the admittance of the probe in contact with the sample, the primed and unprimed coordinates refer to source and observation points, respectively,  $r^2 = \rho^2 + \rho'^2 - 2\rho\rho'\cos\phi'$ ,  $\omega$  is the angular frequency, and  $j = \sqrt{-1}$ .

**Table D-I**  
**Composition of the Tissue Equivalent Matter**

| Frequency (MHz)           | 750          | 750             | 835   | 835   | 1750 | 1750 | 1900  | 1900  | 2450       | 2450 | 5200-5800  | 5200-5800 |
|---------------------------|--------------|-----------------|-------|-------|------|------|-------|-------|------------|------|------------|-----------|
| Tissue                    | Head         | Body            | Head  | Body  | Head | Body | Head  | Body  | Head       | Body | Head       | Body      |
| Ingredients (% by weight) |              |                 |       |       |      |      |       |       |            |      |            |           |
| Bactericide               |              |                 | 0.1   | 0.1   |      |      |       |       |            |      |            |           |
| DGBE                      |              |                 |       |       | 47   | 31   | 44.92 | 29.44 |            | 26.7 |            |           |
| HEC                       |              |                 | 1     | 1     |      |      |       |       |            |      |            |           |
| NaCl                      | See Page 2&3 | See Next Page 2 | 1.45  | 0.94  | 0.4  | 0.2  | 0.18  | 0.39  | See Page 4 | 0.1  | See Page 5 |           |
| Sucrose                   |              |                 | 57    | 44.9  |      |      |       |       |            |      |            |           |
| Polysorbate (Tween) 80    |              |                 |       |       |      |      |       |       |            |      |            | 20        |
| Water                     |              |                 | 40.45 | 53.06 | 52.6 | 68.8 | 54.9  | 70.17 |            | 73.2 |            | 80        |

|                                    |                                                                                     |                       |                                                                                       |                                 |
|------------------------------------|-------------------------------------------------------------------------------------|-----------------------|---------------------------------------------------------------------------------------|---------------------------------|
| FCC ID: A3LSMG900A                 |  | SAR EVALUATION REPORT |  | Reviewed by:<br>Quality Manager |
| Test Dates:<br>02/03/14 - 02/17/14 | DUT Type:<br>Portable Handset                                                       |                       |                                                                                       | APPENDIX D:<br>Page 1 of 5      |

## 2 Composition / Information on ingredients

The Item is composed of the following ingredients:

|                                                                  |                                                                                                                                                     |
|------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------|
| H <sub>2</sub> O                                                 | Water, 35 – 58%                                                                                                                                     |
| Sucrose                                                          | Sugar, white, refined, 40 – 60%                                                                                                                     |
| NaCl                                                             | Sodium Chloride, 0 – 6%                                                                                                                             |
| Hydroxyethyl-cellulose                                           | Medium Viscosity (CAS# 9004-62-0), <0.3%                                                                                                            |
| Preventol-D7                                                     | Preservative: aqueous preparation, (CAS# 55965-84-9), containing 5-chloro-2-methyl-3(2H)-isothiazolone and 2-methyl-3(2H)-isothiazolone, 0.1 – 0.7% |
| Relevant for safety; Refer to the respective Safety Data Sheet*. |                                                                                                                                                     |

**Figure D-1**

### Composition of 750 MHz Head and Body Tissue Equivalent Matter

**Note:** 750MHz liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

#### Measurement Certificate / Material Test

|              |                                          |
|--------------|------------------------------------------|
| Item Name    | Body Tissue Simulating Liquid (MSL750V2) |
| Product No.  | SL AAM 075 AA (Charge: 130313-1)         |
| Manufacturer | SPEAG                                    |

#### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

#### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

#### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



#### Test Condition

|                 |                                                              |
|-----------------|--------------------------------------------------------------|
| Ambient         | Environment temperature ( $22 \pm 3$ )°C and humidity < 70%. |
| TSL Temperature | 22°C                                                         |
| Test Date       | 13-Mar-13                                                    |
| Operator        | IEN                                                          |

#### Additional Information

|                   |                         |
|-------------------|-------------------------|
| TSL Density       | 1.212 g/cm <sup>3</sup> |
| TSL Heat-capacity | 3.006 kJ/(kg*K)         |

| f [MHz] | Measured |       |       | Target |       | Diff. to Target [%] |         |
|---------|----------|-------|-------|--------|-------|---------------------|---------|
|         | HP-e"    | HP-e' | sigma | eps    | sigma | Δ-eps               | Δ-sigma |
| 600     | 57.5     | 24.64 | 0.82  | 56.1   | 0.95  | 2.5                 | -13.6   |
| 625     | 57.2     | 24.31 | 0.84  | 56.0   | 0.95  | 2.1                 | -11.4   |
| 650     | 57.0     | 23.99 | 0.87  | 55.9   | 0.96  | 1.8                 | -9.2    |
| 675     | 56.7     | 23.69 | 0.89  | 55.8   | 0.96  | 1.5                 | -7.1    |
| 700     | 56.4     | 23.39 | 0.91  | 55.7   | 0.96  | 1.2                 | -6.1    |
| 725     | 56.2     | 23.19 | 0.93  | 55.6   | 0.96  | 1.0                 | -2.8    |
| 750     | 55.9     | 22.97 | 0.96  | 55.5   | 0.96  | 0.7                 | -0.5    |
| 775     | 55.7     | 22.78 | 0.98  | 55.4   | 0.97  | 0.4                 | 1.7     |
| 800     | 55.4     | 22.60 | 1.01  | 55.3   | 0.97  | 0.1                 | 4.0     |
| 825     | 55.2     | 22.44 | 1.03  | 55.2   | 0.98  | -0.2                | 5.3     |
| 850     | 55.0     | 22.36 | 1.04  | 55.2   | 0.98  | -0.3                | 5.9     |
| 875     | 54.9     | 22.28 | 1.05  | 55.2   | 0.99  | -0.4                | 6.6     |
| 900     | 54.7     | 22.16 | 1.08  | 55.1   | 1.02  | -0.7                | 5.8     |
| 925     | 54.5     | 22.03 | 1.10  | 55.0   | 1.05  | -1.0                | 5.1     |
| 950     | 54.2     | 21.93 | 1.13  | 55.0   | 1.06  | -1.3                | 6.2     |
| 975     | 54.0     | 21.82 | 1.15  | 54.9   | 1.08  | -1.7                | 7.2     |
| 1000    | 53.8     | 21.74 | 1.18  | 54.9   | 1.09  | -2.0                | 8.5     |
|         | 53.6     | 21.66 | 1.21  | 54.8   | 1.10  | -2.3                | 9.7     |

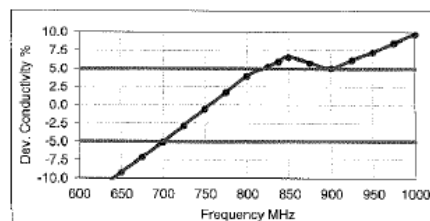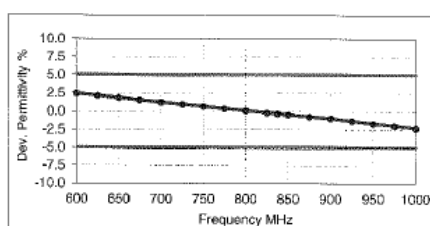

**Figure D-2**

### 750MHz Body Tissue Equivalent Matter

|                                    |                               |                            |  |                                 |
|------------------------------------|-------------------------------|----------------------------|--|---------------------------------|
| FCC ID: A3LSMG900A                 |                               | SAR EVALUATION REPORT      |  | Reviewed by:<br>Quality Manager |
| Test Dates:<br>02/03/14 - 02/17/14 | DUT Type:<br>Portable Handset | APPENDIX D:<br>Page 2 of 5 |  |                                 |

## Measurement Certificate / Material Test

Item Name **Head Tissue Simulating Liquid (HSL750V2)**  
 Product No. SL AAH 075 AA (Charge: 130312-4)  
 Manufacturer SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

### Test Condition

Ambient Environment temperatur ( $22 \pm 3$ )°C and humidity < 70%.  
 TSL Temperature 22°C  
 Test Date 13-Mar-13  
 Operator IEN

### Additional Information

TSL Density 1.284 g/cm<sup>3</sup>  
 TSL Heat-capacity 2.701 kJ/(kg\*K)

| f [MHz] | Measured |        |       | Target |       | Diff. to Target [%] |         |
|---------|----------|--------|-------|--------|-------|---------------------|---------|
|         | HP-e'    | HP-e'' | sigma | eps    | sigma | Δ-eps               | Δ-sigma |
| 600     | 44.6     | 23.25  | 0.78  | 42.7   | 0.88  | 4.3                 | -12.0   |
| 625     | 44.2     | 23.00  | 0.80  | 42.6   | 0.88  | 3.8                 | -9.5    |
| 650     | 43.8     | 22.76  | 0.82  | 42.5   | 0.89  | 3.2                 | -7.1    |
| 675     | 43.4     | 22.50  | 0.84  | 42.3   | 0.89  | 2.6                 | -4.9    |
| 700     | 43.1     | 22.24  | 0.87  | 42.2   | 0.89  | 2.1                 | -2.6    |
| 725     | 42.7     | 22.06  | 0.89  | 42.1   | 0.89  | 1.6                 | -0.2    |
| 750     | 42.4     | 21.88  | 0.91  | 41.9   | 0.89  | 1.1                 | 2.2     |
| 775     | 42.1     | 21.72  | 0.94  | 41.8   | 0.90  | 0.6                 | 4.6     |
| 800     | 41.7     | 21.55  | 0.96  | 41.7   | 0.90  | 0.1                 | 6.9     |
| 825     | 41.4     | 21.40  | 0.98  | 41.6   | 0.91  | -0.4                | 8.3     |
| 838     | 41.3     | 21.32  | 0.99  | 41.5   | 0.91  | -0.8                | 9.0     |
| 850     | 41.1     | 21.24  | 1.00  | 41.5   | 0.92  | -0.9                | 9.6     |
| 875     | 40.8     | 21.11  | 1.03  | 41.5   | 0.94  | -1.6                | 9.0     |
| 900     | 40.6     | 20.99  | 1.05  | 41.5   | 0.97  | -2.3                | 8.3     |
| 925     | 40.3     | 20.87  | 1.07  | 41.5   | 0.98  | -2.9                | 9.4     |
| 950     | 40.0     | 20.76  | 1.10  | 41.4   | 0.99  | -3.5                | 10.3    |
| 975     | 39.7     | 20.66  | 1.12  | 41.4   | 1.00  | -4.0                | 11.5    |
| 1000    | 39.5     | 20.57  | 1.14  | 41.3   | 1.01  | -4.5                | 12.7    |

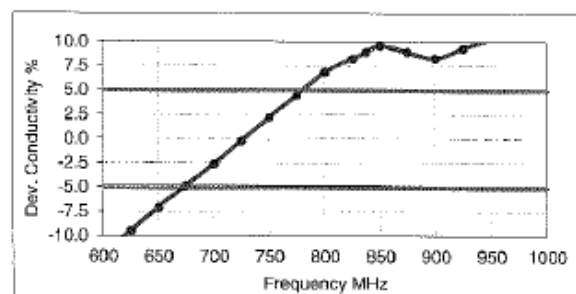
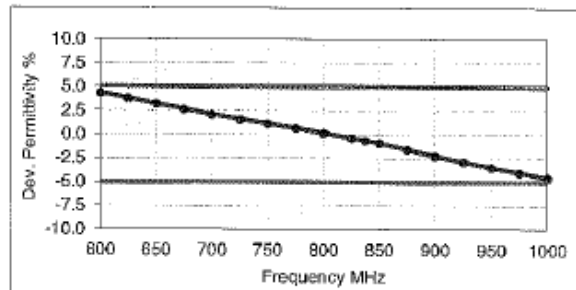


Figure D-3  
750MHz Head Tissue Equivalent Matter

|                                    |                                                                                     |                       |                                                                                       |                                 |
|------------------------------------|-------------------------------------------------------------------------------------|-----------------------|---------------------------------------------------------------------------------------|---------------------------------|
| FCC ID: A3LSMG900A                 |  | SAR EVALUATION REPORT |  | Reviewed by:<br>Quality Manager |
| Test Dates:<br>02/03/14 - 02/17/14 | DUT Type:<br>Portable Handset                                                       |                       |                                                                                       | APPENDIX D:<br>Page 3 of 5      |

## 2 Composition / Information on ingredients

The Item is composed of the following ingredients:

|                                               |                                                                                                                                                                                           |
|-----------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| H <sub>2</sub> O                              | Water, 52 – 75%                                                                                                                                                                           |
| C <sub>8</sub> H <sub>18</sub> O <sub>3</sub> | Diethylene glycol monobutyl ether (DGBE), 25 – 48%<br>(CAS-No. 112-34-5, EC-No. 203-961-6, EC-index-No. 603-096-00-8)<br>Relevant for safety; Refer to the respective Safety Data Sheet*. |
| NaCl                                          | Sodium Chloride, <1.0%                                                                                                                                                                    |

Figure D-4

### Composition of 2.4 GHz Head Tissue Equivalent Matter

**Note:** 2.4 GHz head liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

#### Measurement Certificate / Material Test

|              |                                           |
|--------------|-------------------------------------------|
| Item Name    | Head Tissue Simulating Liquid (HSL2450V2) |
| Product No.  | SL AAH 245 BA (Charge: 130212-2)          |
| Manufacturer | SPEAG                                     |

#### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

#### Setup Validation

Validation results were within  $\pm 2.5\%$  towards the target values of Methanol.

#### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

#### Test Condition

|                 |                                                                         |
|-----------------|-------------------------------------------------------------------------|
| Ambient         | Environment temperature ( $22 \pm 3^\circ\text{C}$ and humidity < 70%). |
| TSL Temperature | 23°C                                                                    |
| Test Date       | 13-Feb-13                                                               |
| Operator        | DI                                                                      |

#### Additional Information

|                   |                         |
|-------------------|-------------------------|
| TSL Density       | 0.988 g/cm <sup>3</sup> |
| TSL Heat-capacity | 3.680 kJ/(kg*K)         |

| f (MHz) | Measured |        |       | Target |       | Diff. to Target [%] |             |
|---------|----------|--------|-------|--------|-------|---------------------|-------------|
|         | HP-e'    | HP-e'' | sigma | eps    | sigma | delta-eps           | delta-sigma |
| 1900    | 40.4     | 11.94  | 1.26  | 40.0   | 1.40  | 1.0                 | -9.9        |
| 1925    | 40.3     | 12.02  | 1.29  | 40.0   | 1.40  | 0.7                 | -8.0        |
| 1950    | 40.2     | 12.11  | 1.31  | 40.0   | 1.40  | 0.5                 | -6.2        |
| 1975    | 40.1     | 12.20  | 1.34  | 40.0   | 1.40  | 0.2                 | -4.2        |
| 2000    | 40.0     | 12.29  | 1.37  | 40.0   | 1.40  | -0.1                | -2.3        |
| 2025    | 39.9     | 12.39  | 1.40  | 40.0   | 1.42  | -0.2                | -1.9        |
| 2050    | 39.8     | 12.49  | 1.42  | 39.9   | 1.44  | -0.4                | -1.4        |
| 2075    | 39.6     | 12.57  | 1.45  | 39.9   | 1.47  | -0.6                | -1.1        |
| 2100    | 39.5     | 12.65  | 1.48  | 39.8   | 1.49  | -0.7                | -0.7        |
| 2125    | 39.4     | 12.74  | 1.51  | 39.8   | 1.51  | -0.9                | -0.4        |
| 2150    | 39.3     | 12.82  | 1.53  | 39.7   | 1.53  | -1.0                | 0.0         |
| 2175    | 39.2     | 12.89  | 1.56  | 39.7   | 1.56  | -1.2                | 0.3         |
| 2200    | 39.1     | 12.97  | 1.59  | 39.6   | 1.58  | -1.3                | 0.6         |
| 2225    | 39.0     | 13.04  | 1.61  | 39.6   | 1.60  | -1.5                | 0.9         |
| 2250    | 38.9     | 13.11  | 1.64  | 39.6   | 1.62  | -1.7                | 1.2         |
| 2275    | 38.8     | 13.20  | 1.67  | 39.5   | 1.64  | -1.8                | 1.6         |
| 2300    | 38.7     | 13.28  | 1.70  | 39.5   | 1.67  | -2.0                | 2.0         |
| 2325    | 38.6     | 13.35  | 1.73  | 39.4   | 1.69  | -2.1                | 2.3         |
| 2350    | 38.5     | 13.42  | 1.75  | 39.4   | 1.71  | -2.3                | 2.6         |
| 2375    | 38.4     | 13.50  | 1.78  | 39.3   | 1.73  | -2.4                | 2.9         |
| 2400    | 38.3     | 13.58  | 1.81  | 39.3   | 1.76  | -2.6                | 3.3         |
| 2425    | 38.2     | 13.65  | 1.84  | 39.2   | 1.78  | -2.7                | 3.6         |
| 2450    | 38.1     | 13.73  | 1.87  | 39.2   | 1.80  | -2.9                | 4.0         |
| 2475    | 38.0     | 13.79  | 1.90  | 39.2   | 1.83  | -3.1                | 3.9         |
| 2500    | 37.9     | 13.85  | 1.93  | 39.1   | 1.85  | -3.3                | 3.9         |
| 2525    | 37.8     | 13.94  | 1.96  | 39.1   | 1.88  | -3.4                | 4.0         |
| 2550    | 37.7     | 14.02  | 1.99  | 39.1   | 1.91  | -3.6                | 4.2         |
| 2575    | 37.6     | 14.09  | 2.02  | 39.0   | 1.94  | -3.8                | 4.3         |
| 2600    | 37.5     | 14.17  | 2.05  | 39.0   | 1.96  | -4.0                | 4.6         |
| 2625    | 37.4     | 14.23  | 2.08  | 39.0   | 1.99  | -4.2                | 4.4         |
| 2650    | 37.3     | 14.29  | 2.11  | 38.9   | 2.02  | -4.3                | 4.4         |
| 2675    | 37.1     | 14.36  | 2.14  | 38.9   | 2.05  | -4.5                | 4.5         |
| 2700    | 37.0     | 14.43  | 2.17  | 38.9   | 2.07  | -4.8                | 4.6         |

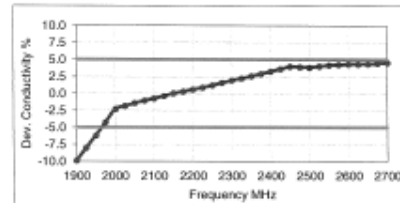
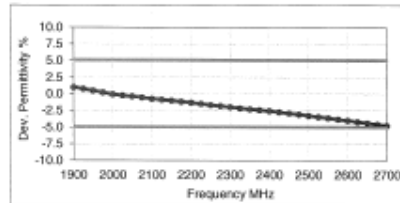


Figure D-5

### 2.4 GHz Head Tissue Equivalent Matter

|                                    |                                                                                     |                       |                                                                                       |                                 |
|------------------------------------|-------------------------------------------------------------------------------------|-----------------------|---------------------------------------------------------------------------------------|---------------------------------|
| FCC ID: A3LSMG900A                 |  | SAR EVALUATION REPORT |  | Reviewed by:<br>Quality Manager |
| Test Dates:<br>02/03/14 - 02/17/14 | DUT Type:<br>Portable Handset                                                       |                       |                                                                                       | APPENDIX D:<br>Page 4 of 5      |

## 2 Composition / Information on ingredients

The Item is composed of the following ingredients:

|             |          |
|-------------|----------|
| Water       | 50 – 65% |
| Mineral oil | 10 – 30% |
| Emulsifiers | 8 – 25%  |
| Sodium salt | 0 – 1.5% |

**Figure D-6**  
**Composition of 5 GHz Head Tissue Equivalent Matter**

**Note:** 5GHz head liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

### Measurement Certificate / Material Test

|              |                                                 |
|--------------|-------------------------------------------------|
| Item Name    | Head Tissue Simulating Liquid (HBBL3500-5800V5) |
| Product No.  | SL AAH 502 AB (Charge: 120402-2)                |
| Manufacturer | SPEAG                                           |

### Measurement Method

TSL dielectric parameters measured using calibrated OCP probe (type DAK).

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

### Test Condition



Ambient Condition 22°C ; 30% humidity  
TSL Temperature 22°C  
Test Date 4-Apr-12

### Additional Information

TSL Density 0.985 g/cm<sup>3</sup>  
TSL Heat-capacity 3.383 kJ/(kg\*K)

### Results

|         | Measured        |                  |       | Target |       | Diff.to Target [%] |                 |
|---------|-----------------|------------------|-------|--------|-------|--------------------|-----------------|
| f [MHz] | HP- $\epsilon'$ | HP- $\epsilon''$ | sigma | eps    | sigma | $\Delta$ -eps      | $\Delta$ -sigma |
| 3400    | 38.7            | 14.86            | 2.83  | 38.0   | 2.81  | 1.8                | 0.7             |
| 3500    | 38.6            | 14.91            | 2.90  | 37.9   | 2.91  | 1.7                | -0.3            |
| 3600    | 38.5            | 14.92            | 2.99  | 37.8   | 3.02  | 1.7                | -0.9            |
| 3700    | 38.3            | 14.92            | 3.07  | 37.7   | 3.12  | 1.7                | -1.5            |
| 3800    | 38.2            | 14.94            | 3.16  | 37.6   | 3.22  | 1.7                | -1.9            |
| 3900    | 38.1            | 14.95            | 3.24  | 37.5   | 3.32  | 1.7                | -2.4            |
| 4000    | 38.0            | 15.00            | 3.34  | 37.4   | 3.43  | 1.8                | -2.5            |
| 4100    | 37.9            | 15.04            | 3.43  | 37.2   | 3.53  | 1.8                | -2.6            |
| 4200    | 37.8            | 15.08            | 3.52  | 37.1   | 3.63  | 1.8                | -2.9            |
| 4300    | 37.7            | 15.14            | 3.62  | 37.0   | 3.73  | 1.8                | -3.0            |
| 4400    | 37.5            | 15.18            | 3.71  | 36.9   | 3.84  | 1.7                | -3.1            |
| 4500    | 37.4            | 15.20            | 3.81  | 36.8   | 3.94  | 1.6                | -3.3            |
| 4600    | 37.3            | 15.29            | 3.91  | 36.7   | 4.04  | 1.6                | -3.2            |
| 4700    | 37.1            | 15.34            | 4.01  | 36.6   | 4.14  | 1.5                | -3.2            |
| 4800    | 37.0            | 15.39            | 4.11  | 36.4   | 4.25  | 1.4                | -3.2            |
| 4850    | 36.9            | 15.43            | 4.16  | 36.4   | 4.30  | 1.3                | -3.1            |
| 4900    | 36.8            | 15.45            | 4.21  | 36.3   | 4.35  | 1.3                | -3.1            |
| 4950    | 36.7            | 15.47            | 4.26  | 36.3   | 4.40  | 1.2                | -3.1            |
| 5000    | 36.7            | 15.50            | 4.31  | 36.2   | 4.45  | 1.2                | -3.1            |
| 5050    | 36.6            | 15.55            | 4.37  | 36.2   | 4.50  | 1.1                | -3.0            |
| 5100    | 36.5            | 15.60            | 4.43  | 36.1   | 4.55  | 1.1                | -2.8            |
| 5150    | 36.4            | 15.62            | 4.48  | 36.0   | 4.60  | 1.0                | -2.8            |
| 5200    | 36.4            | 15.65            | 4.53  | 36.0   | 4.66  | 1.0                | -2.8            |
| 5250    | 36.3            | 15.67            | 4.58  | 35.9   | 4.71  | 1.0                | -2.8            |
| 5300    | 36.2            | 15.70            | 4.63  | 35.9   | 4.76  | 1.0                | -2.7            |
| 5350    | 36.1            | 15.70            | 4.67  | 35.8   | 4.81  | 0.9                | -2.9            |
| 5400    | 36.1            | 15.74            | 4.73  | 35.8   | 4.86  | 0.8                | -2.7            |
| 5450    | 36.0            | 15.75            | 4.77  | 35.7   | 4.91  | 0.9                | -2.8            |
| 5500    | 35.9            | 15.75            | 4.82  | 35.6   | 4.96  | 0.8                | -2.9            |
| 5550    | 35.9            | 15.80            | 4.88  | 35.6   | 5.01  | 0.8                | -2.7            |
| 5600    | 35.8            | 15.82            | 4.93  | 35.5   | 5.07  | 0.7                | -2.7            |
| 5650    | 35.7            | 15.86            | 4.98  | 35.5   | 5.12  | 0.7                | -2.6            |
| 5700    | 35.7            | 15.88            | 5.03  | 35.4   | 5.17  | 0.7                | -2.6            |
| 5750    | 35.6            | 15.90            | 5.08  | 35.4   | 5.22  | 0.6                | -2.6            |
| 5800    | 35.5            | 15.94            | 5.14  | 35.3   | 5.27  | 0.6                | -2.4            |
| 5850    | 35.4            | 15.98            | 5.20  | 35.3   | 5.34  | 0.4                | -2.5            |
| 5900    | 35.4            | 16.02            | 5.26  | 35.3   | 5.40  | 0.2                | -2.6            |

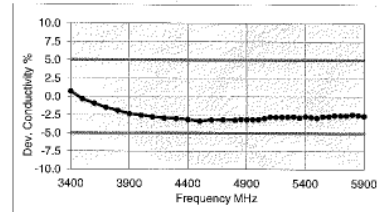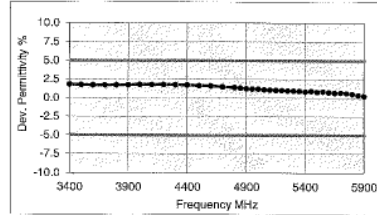

**Figure D-7**  
**5GHz Head Tissue Equivalent Matter**

|                                    |                                                                                     |                       |                                                                                       |                                 |
|------------------------------------|-------------------------------------------------------------------------------------|-----------------------|---------------------------------------------------------------------------------------|---------------------------------|
| FCC ID: A3LSMG900A                 |  | SAR EVALUATION REPORT |  | Reviewed by:<br>Quality Manager |
| Test Dates:<br>02/03/14 - 02/17/14 | DUT Type:<br>Portable Handset                                                       |                       |                                                                                       | APPENDIX D:<br>Page 5 of 5      |

## APPENDIX E: SAR SYSTEM VALIDATION

Per FCC KDB 865664 D02v01, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue- equivalent media for system validation, according to the procedures outlined in FCC KDB 865664 D01 v01 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

**Table E-I**  
**SAR System Validation Summary**

| SAR SYSTEM # | FREQ. [MHz] | DATE      | PROBE SN | PROBE TYPE | PROBE CAL. POINT |      | COND. | PERM. | CW VALIDATION |                 |                | MOD. VALIDATION |             |      |
|--------------|-------------|-----------|----------|------------|------------------|------|-------|-------|---------------|-----------------|----------------|-----------------|-------------|------|
|              |             |           |          |            |                  |      | (σ)   | (ε)   | SENSI- TIVITY | PROBE LINEARITY | PROBE ISOTROPY | MOD. TYPE       | DUTY FACTOR | PAR  |
| I            | 750         | 6/27/2013 | 3319     | ES3DV3     | 750              | Head | 0.918 | 41.73 | PASS          | PASS            | PASS           | N/A             | N/A         | N/A  |
| H            | 835         | 2/7/2014  | 3589     | EX3DV4     | 835              | Head | 0.892 | 40.40 | PASS          | PASS            | PASS           | GMSK            | PASS        | N/A  |
| B            | 1750        | 11/6/2013 | 3288     | ES3DV3     | 1750             | Head | 1.406 | 40.47 | PASS          | PASS            | PASS           | N/A             | N/A         | N/A  |
| B            | 1900        | 11/4/2013 | 3288     | ES3DV3     | 1900             | Head | 1.381 | 38.59 | PASS          | PASS            | PASS           | GMSK            | PASS        | N/A  |
| K            | 2450        | 2/8/2014  | 3287     | ES3DV3     | 2450             | Head | 1.832 | 38.03 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5200        | 12/3/2013 | 3914     | EX3DV4     | 5200             | Head | 4.482 | 34.70 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5300        | 12/3/2013 | 3914     | EX3DV4     | 5300             | Head | 4.604 | 34.60 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5500        | 12/3/2013 | 3914     | EX3DV4     | 5500             | Head | 4.821 | 34.28 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5600        | 12/3/2013 | 3914     | EX3DV4     | 5600             | Head | 4.907 | 34.13 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5800        | 12/3/2013 | 3914     | EX3DV4     | 5800             | Head | 5.133 | 33.89 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| C            | 750         | 8/14/2013 | 3263     | ES3DV3     | 750              | Body | 0.975 | 54.36 | PASS          | PASS            | PASS           | N/A             | N/A         | N/A  |
| C            | 835         | 8/14/2013 | 3263     | ES3DV3     | 835              | Body | 0.993 | 53.17 | PASS          | PASS            | PASS           | GMSK            | PASS        | N/A  |
| B            | 1750        | 11/6/2013 | 3288     | ES3DV3     | 1750             | Body | 1.534 | 51.18 | PASS          | PASS            | PASS           | N/A             | N/A         | N/A  |
| I            | 1900        | 7/1/2013  | 3319     | ES3DV3     | 1900             | Body | 1.502 | 52.10 | PASS          | PASS            | PASS           | GMSK            | PASS        | N/A  |
| H            | 2450        | 6/21/2013 | 3318     | ES3DV3     | 2450             | Body | 2.006 | 51.66 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5200        | 12/7/2013 | 3914     | EX3DV4     | 5200             | Body | 5.330 | 48.16 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5300        | 12/7/2013 | 3914     | EX3DV4     | 5300             | Body | 5.481 | 47.91 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5500        | 12/7/2013 | 3914     | EX3DV4     | 5500             | Body | 5.807 | 47.39 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5600        | 12/7/2013 | 3914     | EX3DV4     | 5600             | Body | 5.933 | 47.15 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |
| E            | 5800        | 12/7/2013 | 3914     | EX3DV4     | 5800             | Body | 6.240 | 46.70 | PASS          | PASS            | PASS           | OFDM            | N/A         | PASS |

NOTES: While the probes have been calibrated for both a CW and modulated signals, all measurements were performed using probes calibrated for CW signals only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01 for scenarios when CW probe calibrations are used with other signal types. SAR systems were validated for modulated signals with a periodic duty cycle, such as GMSK, or with a high peak to average ratio (>5 dB), such as OFDM according to KDB 865664.

|                                    |                                                                                     |                       |                                                                                       |                                 |
|------------------------------------|-------------------------------------------------------------------------------------|-----------------------|---------------------------------------------------------------------------------------|---------------------------------|
| FCC ID: A3LSMG900A                 |  | SAR EVALUATION REPORT |  | Reviewed by:<br>Quality Manager |
| Test Dates:<br>02/03/14 - 02/17/14 | DUT Type:<br>Portable Handset                                                       |                       |                                                                                       | APPENDIX E:<br>Page 1 of 1      |