


835MHz Brain Dipole Validation

Generic Twin Phantom; Flat Section; Probe: ET3DV6 - SN1560 -- Probe Cal Date 20/02/01; ConvF(6.78,6.78,6.78)
Med. Parameters 835 MHz Brain: $\sigma = 0.90$ mho/m $\epsilon_r = 41.5$ $\rho = 1.00$ g/cm³; Antenna Position -- Out; Crest Factor 1.0
SAR (1g): 2.43 mW/g, SAR (10g): 1.60 mW/g


835MHz Brain Dipole Validation (D835V2 S/N: 406)
Frequency: 835 MHz; Antenna Input Power: 250 [mW]
PCTEST Brain Tissue Simulating Liquid [01-23-2002]

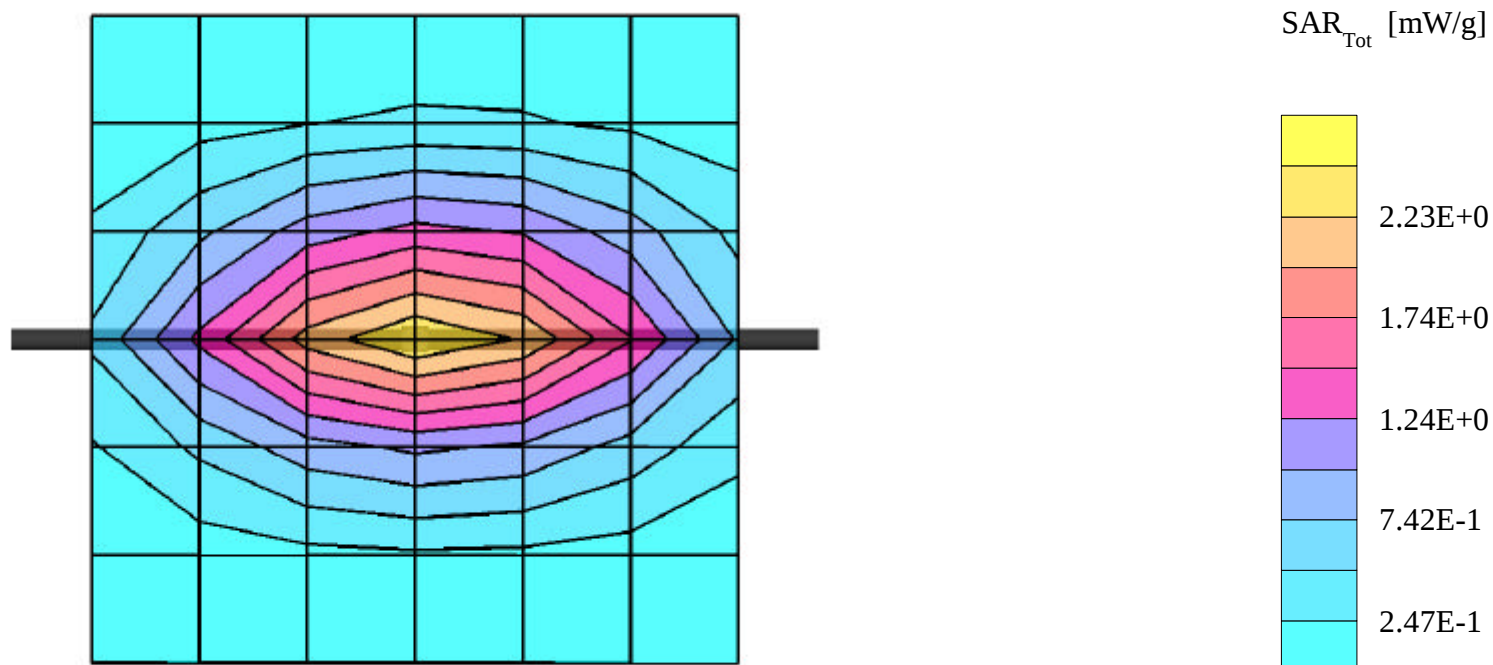

835MHz Muscle Dipole Validation

Generic Twin Phantom; Flat Section; Probe: ET3DV6 - SN1560 -- Probe Cal Date 20/02/01; ConvF(6.52,6.52,6.52)
Med. Parameters 835 MHz Muscle: $\sigma = 0.97$ mho/m $\epsilon_r = 55.2$ $\rho = 1.00$ g/cm³; Antenna Position -- Out; Crest Factor 1.0
SAR (1g): 2.35 mW/g, SAR (10g): 1.55 mW/g

835MHz Muscle Dipole Validation (D835V2 S/N: 406)
Frequency: 835 MHz; Antenna Input Power: 250 [mW]
PCTEST Muscle Tissue Simulating Liquid [01-24-2002]

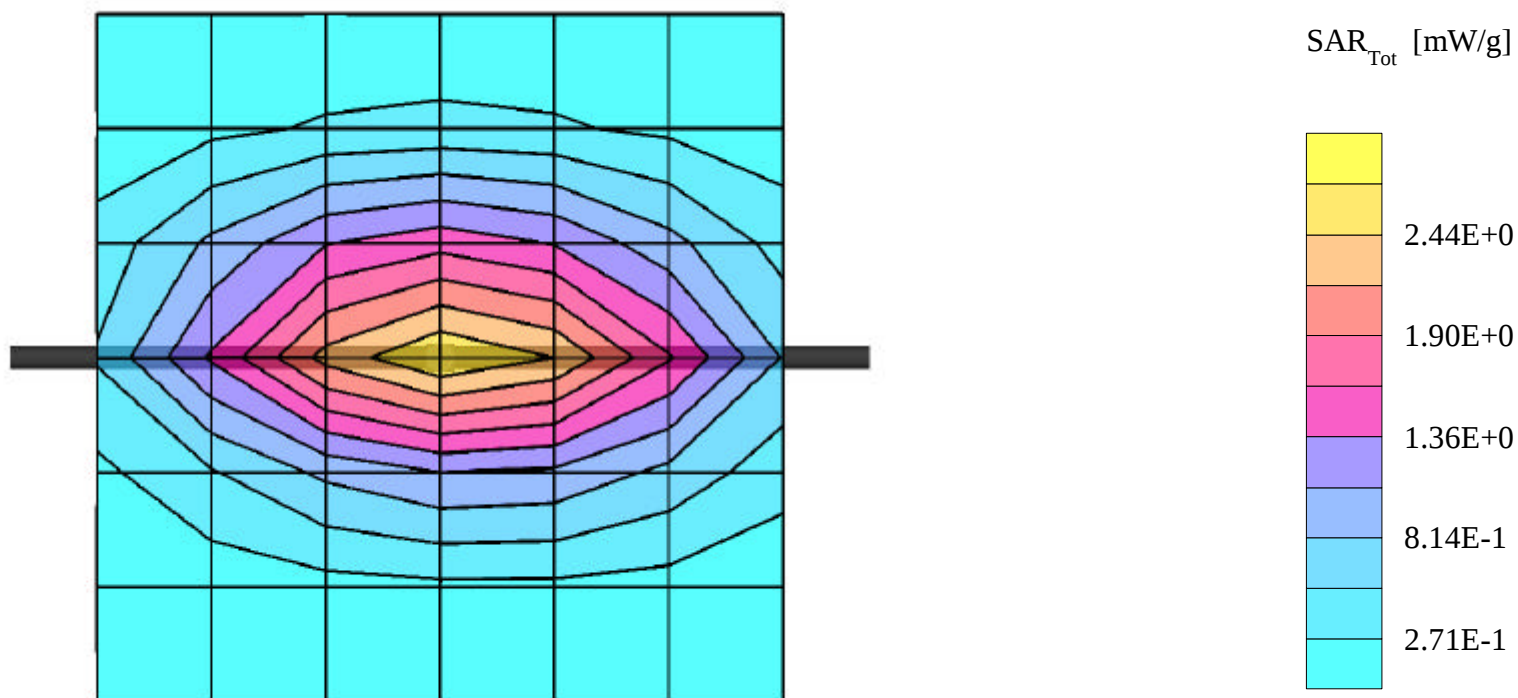

835MHz Brain Dipole Validation

Generic Twin Phantom; Flat Section; Probe: ET3DV6 - SN1560 -- Probe Cal Date 20/02/01; ConvF(6.78,6.78,6.78)
Med. Parameters 835 MHz Brain: $\sigma = 0.90$ mho/m $\epsilon_r = 41.5$ $\rho = 1.00$ g/cm³; Antenna Position -- Out; Crest Factor 1.0
SAR (1g): 2.31 mW/g, SAR (10g): 1.54 mW/g

835MHz Brain Dipole Validation (D835V2 S/N: 406)
Frequency: 835 MHz; Antenna Input Power: 250 [mW]
PCTEST Brain Tissue Simulating Liquid [01-28-2002]

