

APPENDIX D : Calibration Certificates

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

Dosimetric E-Field Probe

Type:	ET3DV6
Serial Number:	1729
Place of Calibration:	Zurich
Date of Calibration:	November 20, 2002
Calibration Interval:	12 months


Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:



Approved by:



**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Telephone +41 1 245 97 00, Fax +41 1 245 97 79

Probe ET3DV6

SN:1729

Manufactured: October 1, 2002
Last calibration: November 20, 2002

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1729

November 20, 2002

DASY - Parameters of Probe: ET3DV6 SN:1729

Sensitivity in Free Space

NormX	$1.59 \mu\text{V}/(\text{V/m})^2$
NormY	$1.53 \mu\text{V}/(\text{V/m})^2$
NormZ	$1.75 \mu\text{V}/(\text{V/m})^2$

Diode Compression

DCP X	95	mV
DCP Y	95	mV
DCP Z	95	mV

Sensitivity in Tissue Simulating Liquid

Head	900 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.97 \pm 5\% \text{ mho/m}$
Head	835 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.90 \pm 5\% \text{ mho/m}$
ConvF X	$6.4 \pm 9.5\% (k=2)$	Boundary effect:	
ConvF Y	$6.4 \pm 9.5\% (k=2)$	Alpha	0.47
ConvF Z	$6.4 \pm 9.5\% (k=2)$	Depth	2.12
Head	1800 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\% \text{ mho/m}$
Head	1900 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\% \text{ mho/m}$
ConvF X	$5.3 \pm 9.5\% (k=2)$	Boundary effect:	
ConvF Y	$5.3 \pm 9.5\% (k=2)$	Alpha	0.52
ConvF Z	$5.3 \pm 9.5\% (k=2)$	Depth	2.44

Boundary Effect

Head	900 MHz	Typical SAR gradient: 5 % per mm	
Probe Tip to Boundary		1 mm	2 mm
SAR _{90%} [%]	Without Correction Algorithm	9.2	5.0
SAR _{90%} [%]	With Correction Algorithm	0.2	0.4
Head	1800 MHz	Typical SAR gradient: 10 % per mm	
Probe Tip to Boundary		1 mm	2 mm
SAR _{90%} [%]	Without Correction Algorithm	12.6	8.4
SAR _{90%} [%]	With Correction Algorithm	0.2	0.2


Sensor Offset

Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.3 ± 0.2	mm

ET3DV6 SN:1729


November 20, 2002

Receiving Pattern (ϕ), $\theta = 0^\circ$

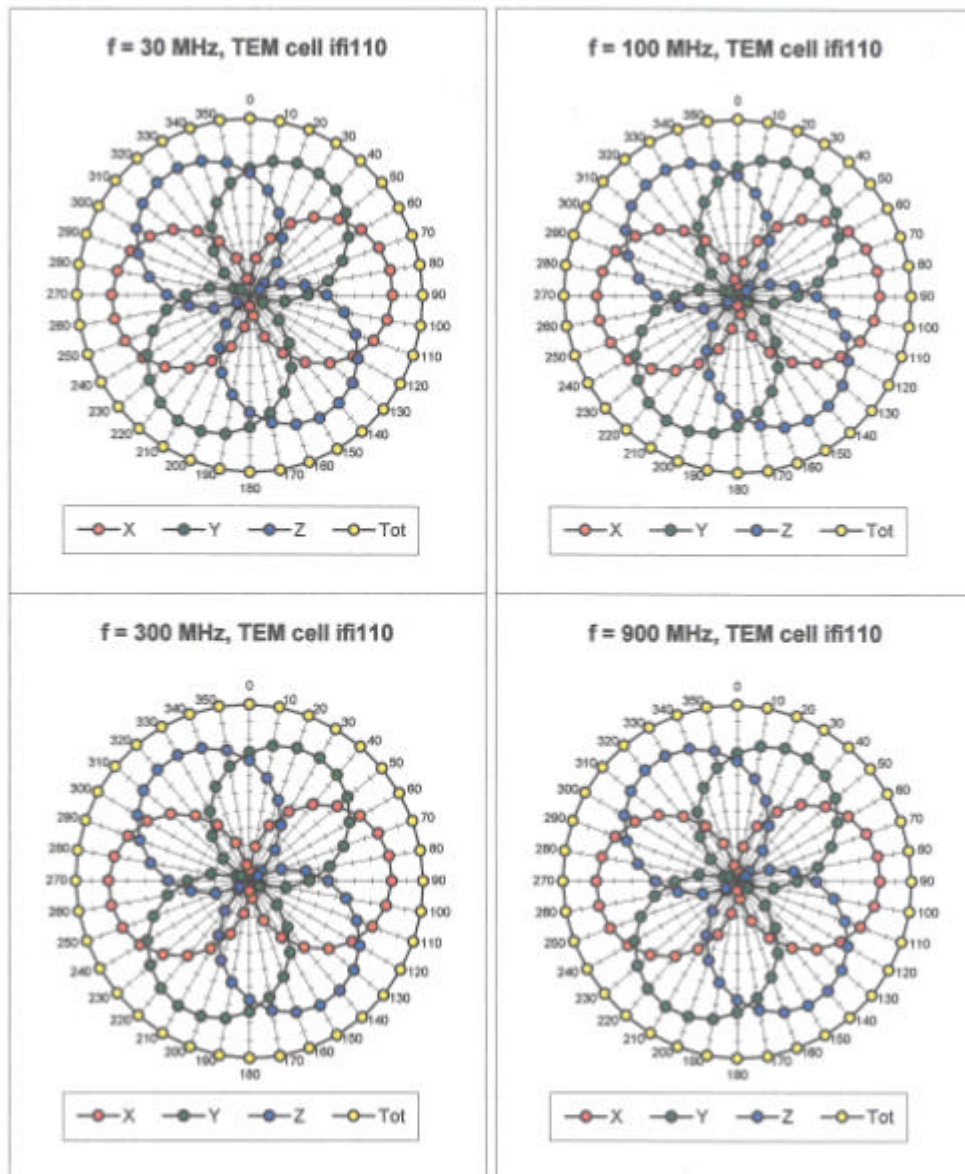


ET3DV6 SN:1729

November 20, 2002

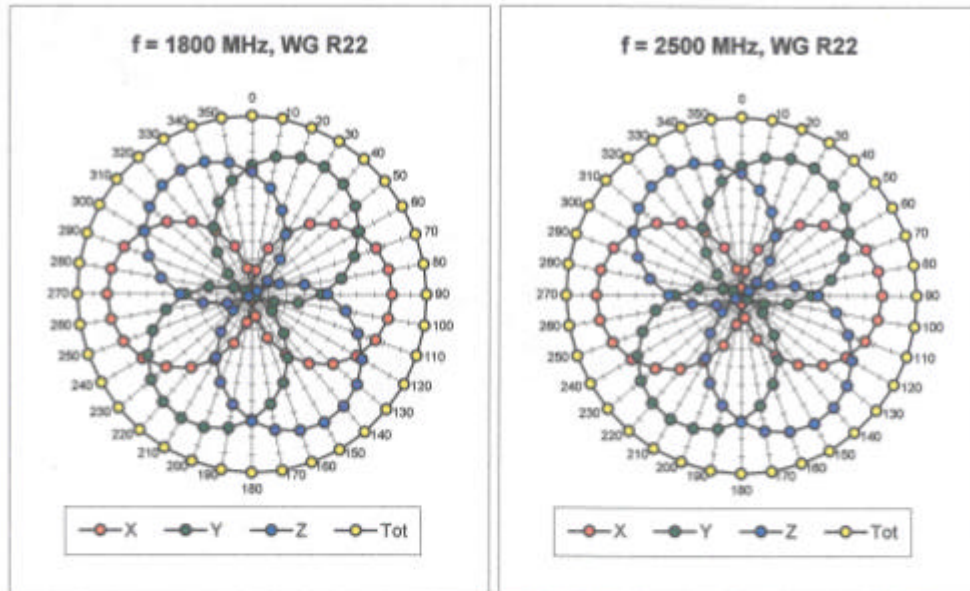


Isotropy Error (ϕ), $\theta = 0^\circ$

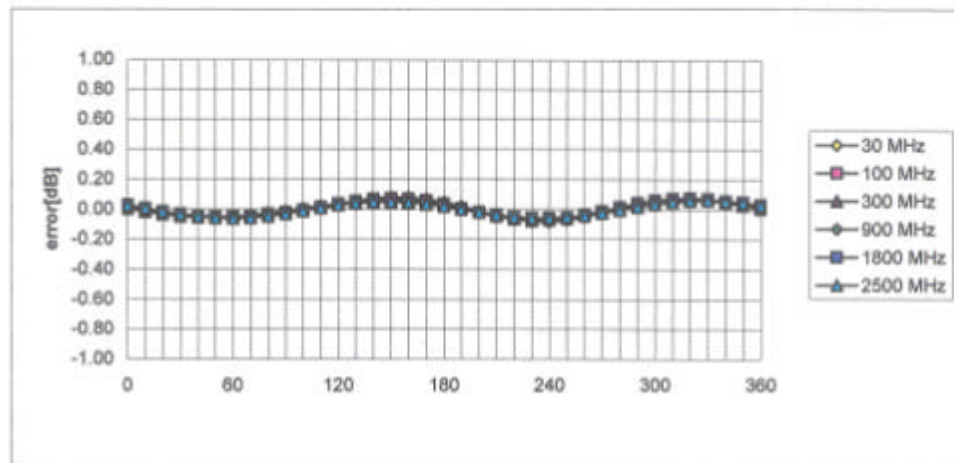

ET3DV6 SN:1729

November 20, 2002



Frequency Response of E-Field (TEM-Cell:ifi110, Waveguide R22)

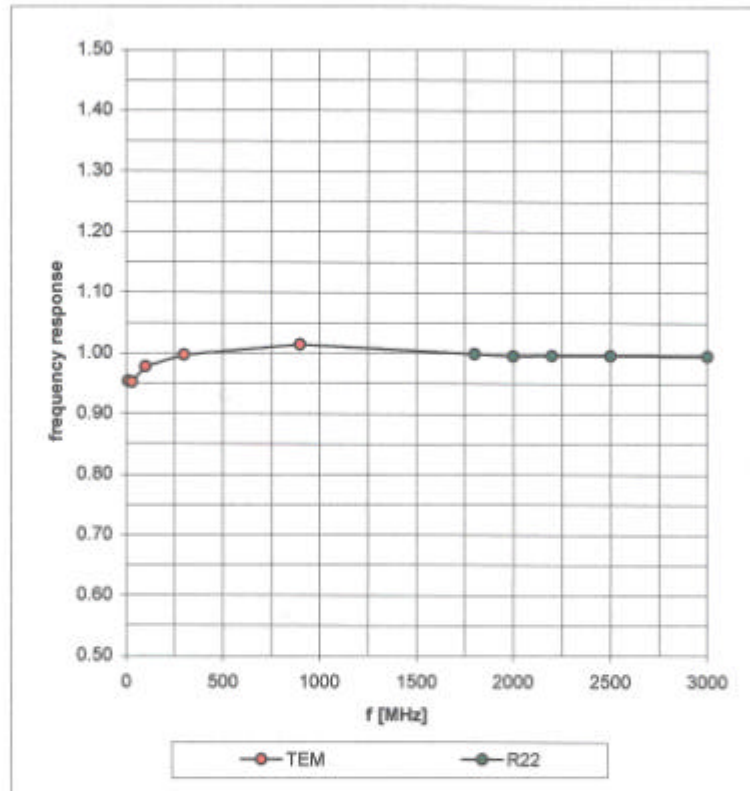

ET3DV6 SN:1729

November 20, 2002


Dynamic Range f(SAR_{brain}) (Waveguide R22)

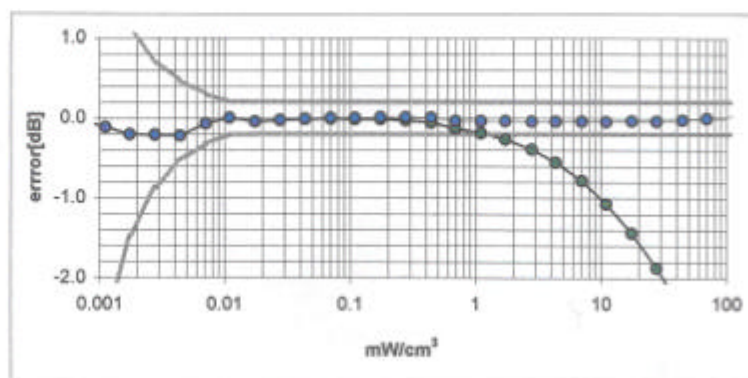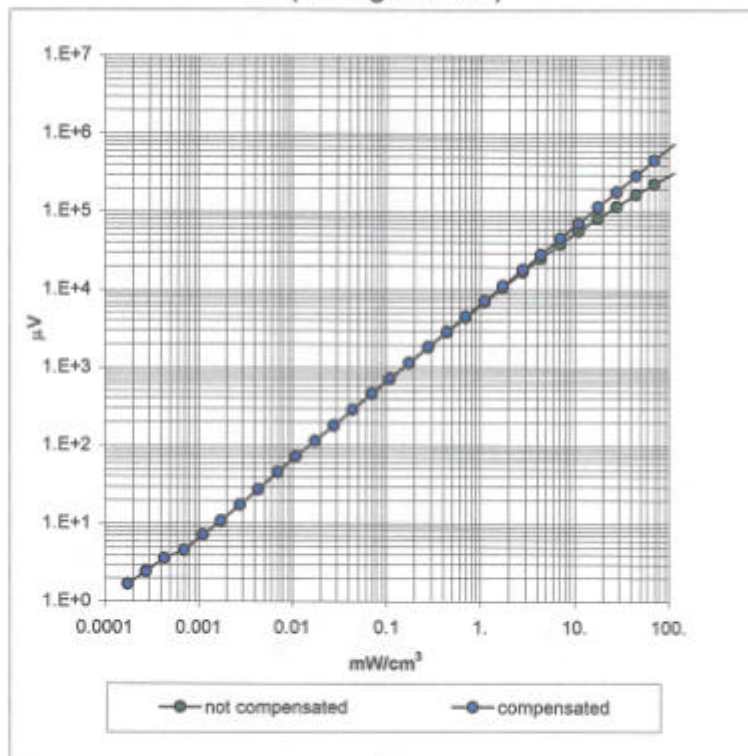

ET3DV6 SN:1729

November 20, 2002

Conversion Factor Assessment

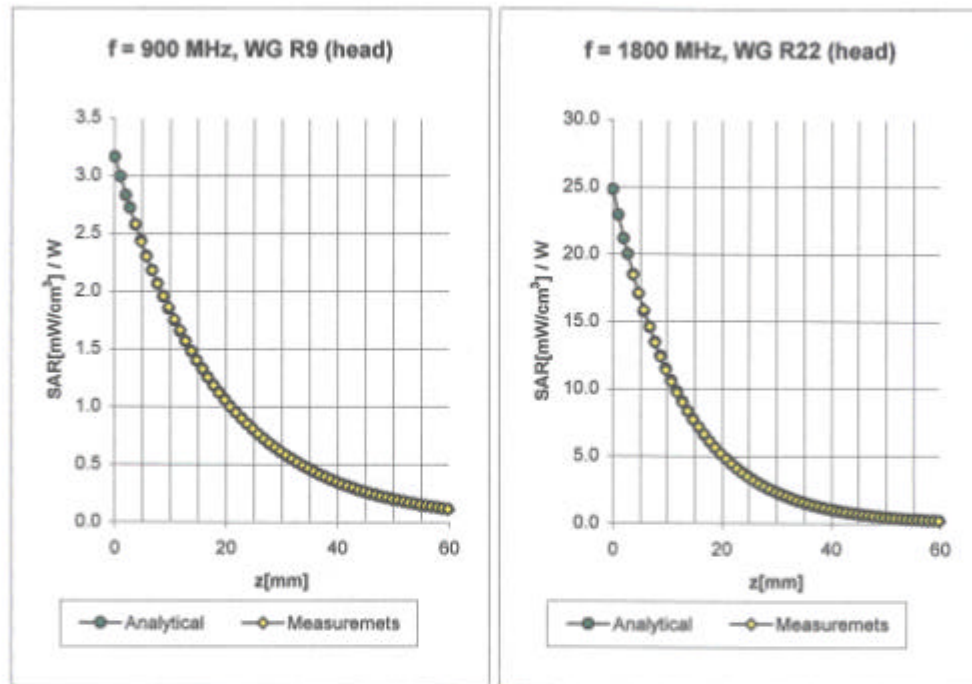


Head	900 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.97 \pm 5\%$ mho/m
Head	835 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.90 \pm 5\%$ mho/m
	ConvF X	$6.4 \pm 9.5\%$ (k=2)	Boundary effect:
	ConvF Y	$6.4 \pm 9.5\%$ (k=2)	Alpha 0.47
	ConvF Z	$6.4 \pm 9.5\%$ (k=2)	Depth 2.12
Head	1800 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\%$ mho/m
Head	1900 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\%$ mho/m
	ConvF X	$5.3 \pm 9.5\%$ (k=2)	Boundary effect:
	ConvF Y	$5.3 \pm 9.5\%$ (k=2)	Alpha 0.52
	ConvF Z	$5.3 \pm 9.5\%$ (k=2)	Depth 2.44

ET3DV6 SN:1729

November 20, 2002

Deviation from Isotropy in HSL

Error (θ, ϕ), $f = 900$ MHz

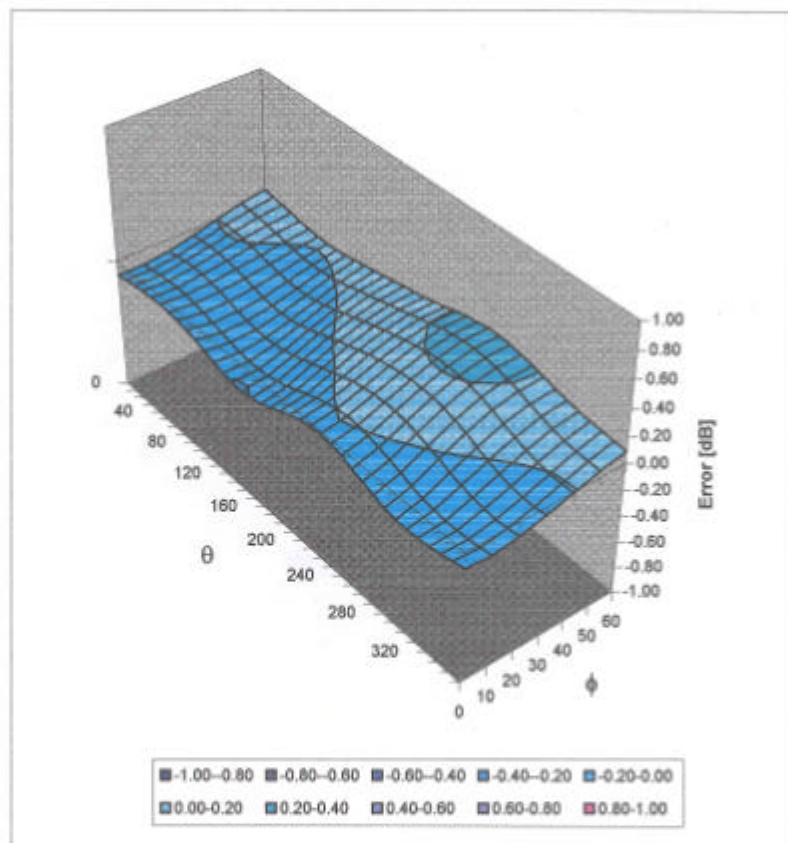

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@spesg.com, <http://www.spesg.com>

Additional Conversion Factors

for Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1729

Place of Assessment:

Zurich

Date of Assessment:

May 22, 2003

Probe Calibration Date:

November 20, 2002

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 1 245 9700, Fax +41 1 245 9779
 info@speag.com, <http://www.speag.com>

Dosimetric E-Field Probe ET3DV6 SN:1729Conversion factor ($\pm$ standard deviation)835 MHz ConvF **6.3 $\pm$ 8%**

$\epsilon_r = 55.2 \pm 5\%$ $\sigma = 0.97 \pm 5\% \text{ mho/m}$ (body tissue)

1900 MHz ConvF **4.7 $\pm$ 8%**

$\epsilon_r = 53.3 \pm 5\%$ $\sigma = 1.52 \pm 5\% \text{ mho/m}$ (body tissue)

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate**835 MHz System Validation Dipole**

Type:

D835V2

Serial Number:

471

Place of Calibration:

Zurich

Date of Calibration:

December 4, 2002

Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:



Approved by:

