

Test Laboratory: Compliance Certification Services

File Name: D1800V2 SN 294_8.86 mW.da4

DUT: Dipole 1800 MHz Type & Serial Number: D1800V2 SN 294

Program: System Validation (ET3DV6 SN 1577); I/P Power 250 mW, Air temp. 23 deg C, liquid temp. 21 deg C

Communication System: CW_1800 MHz; Frequency: 1800 MHz; Duty Cycle: 1:1

Medium: Head 1800 MHz ($\sigma = 1.3819$ mho/m, $\epsilon = 38.95$, $\rho = 1000$ kg/m³)

Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(5.6, 5.6, 5.6); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1 - TP:1185
- Software: DASY4, V4.0 Build 51

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm


Reference Value = 90 V/m

Peak SAR = 15.1 mW/g

SAR(1 g) = 8.86 mW/g; SAR(10 g) = 4.64 mW/g

Power Drift = 0.007 dB

Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

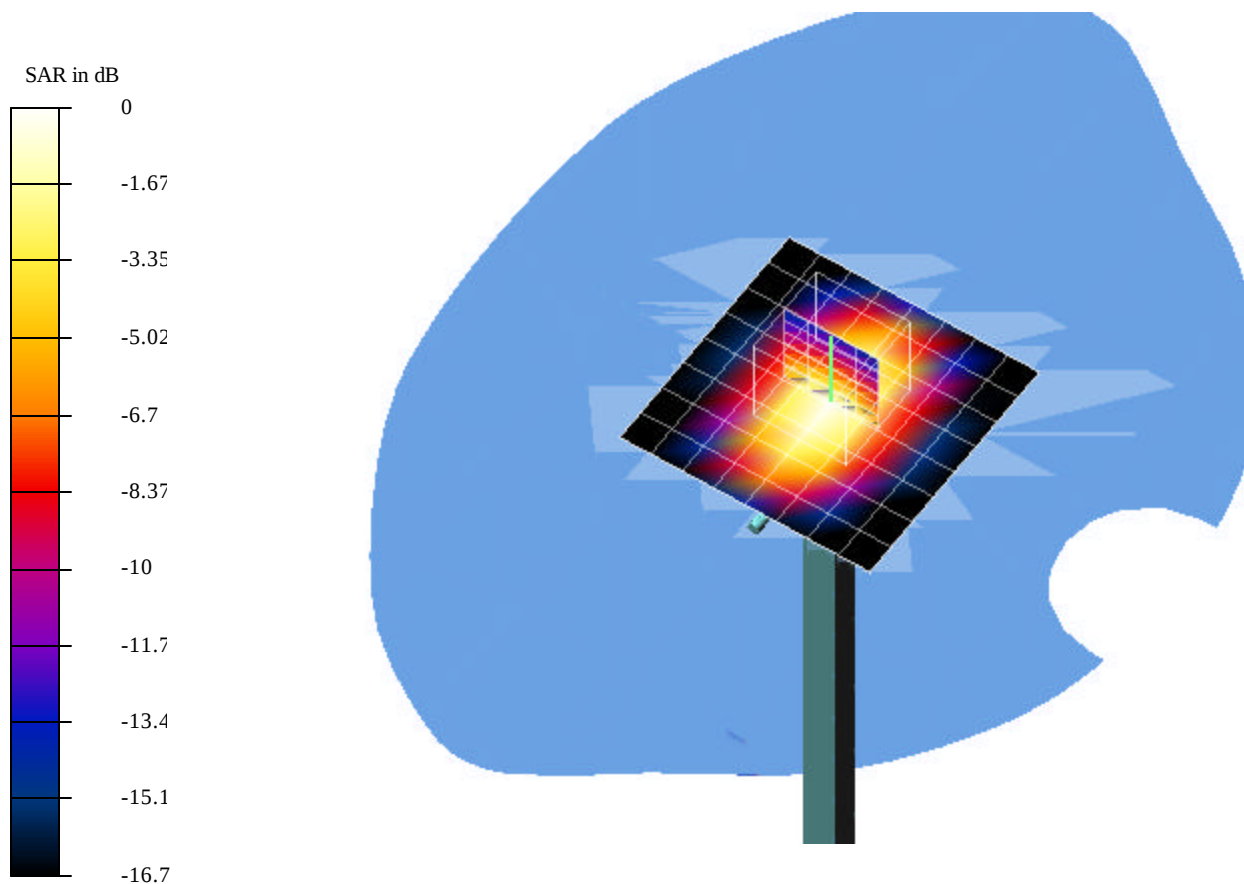

Test Laboratory: Compliance Certification Services

File Name: D1800V2 SN 294_8.95 mW.da4

DUT: Dipole 1800 MHz Type & Serial Number: D1800V2 SN 294

Program: System Validation (ET3DV6 SN 1577); I/P Power 250 mW, Air temp. 23.5 deg C, liquid temp. 21.5 d

Communication System: CW_1800 MHz; Frequency: 1800 MHz; Duty Cycle: 1:1

Medium: Head 1800 MHz ($\sigma = 1.3719$ mho/m, $\epsilon = 39.318$, $\rho = 1000$ kg/m³)

Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(5.6, 5.6, 5.6); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1 - TP:1185
- Software: DASY4, V4.0 Build 51

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm



Reference Value = 90 V/m

Peak SAR = 15.2 mW/g

SAR(1 g) = 8.95 mW/g; SAR(10 g) = 4.69 mW/g

Power Drift = 0.05 dB

Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

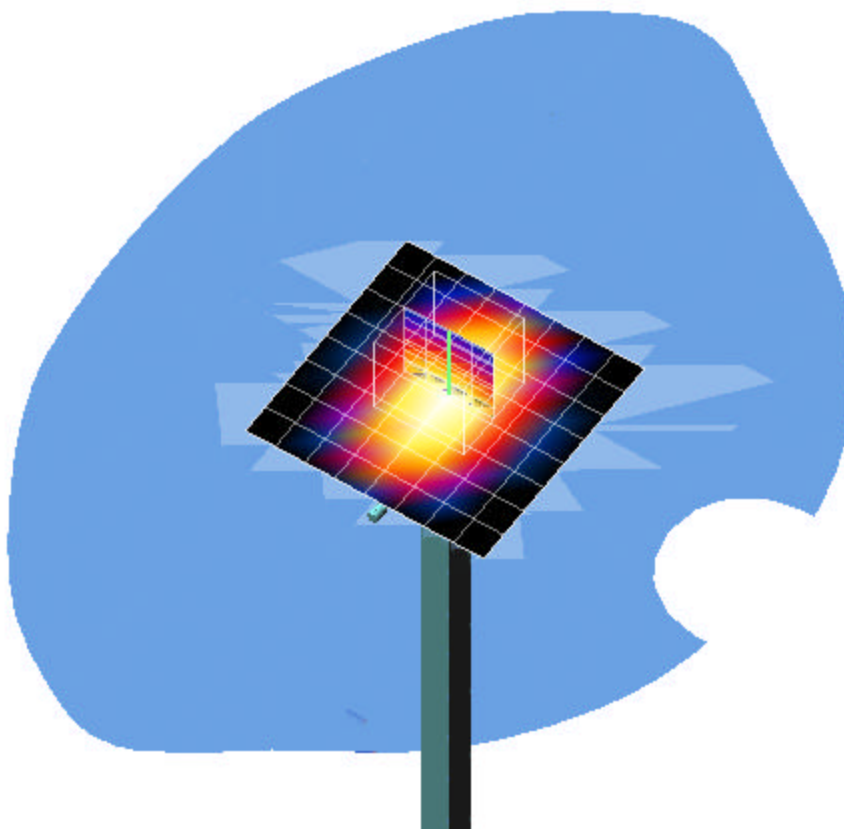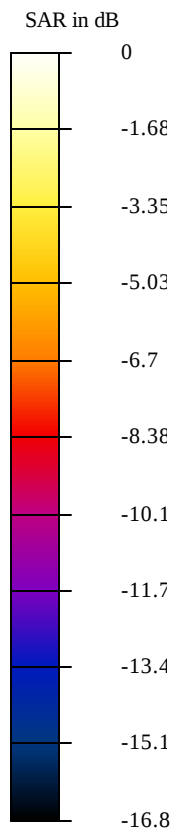

Test Laboratory: Compliance Certification Services

File Name: D1800V2 SN 294_8.92 mW.da4

DUT: Dipole 1800 MHz Type & Serial Number: D1800V2 SN 294

Program: System Validation (ET3DV6 SN 1577); I/P Power 250 mW, Air temp. 23 deg C, liquid temp. 21 deg C

Communication System: CW_1800 MHz; Frequency: 1800 MHz; Duty Cycle: 1:1

Medium: Head 1800 MHz ($\sigma = 1.3936$ mho/m, $\epsilon = 38.74$, $\rho = 1000$ kg/m³)

Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(5.6, 5.6, 5.6); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1 - TP:1185
- Software: DASY4, V4.0 Build 51

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm

Reference Value = 90.2 V/m

Peak SAR = 15.1 mW/g

SAR(1 g) = 8.92 mW/g; SAR(10 g) = 4.67 mW/g

Power Drift = -0.01 dB

Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

