



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: GFSK 2480MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:15:01

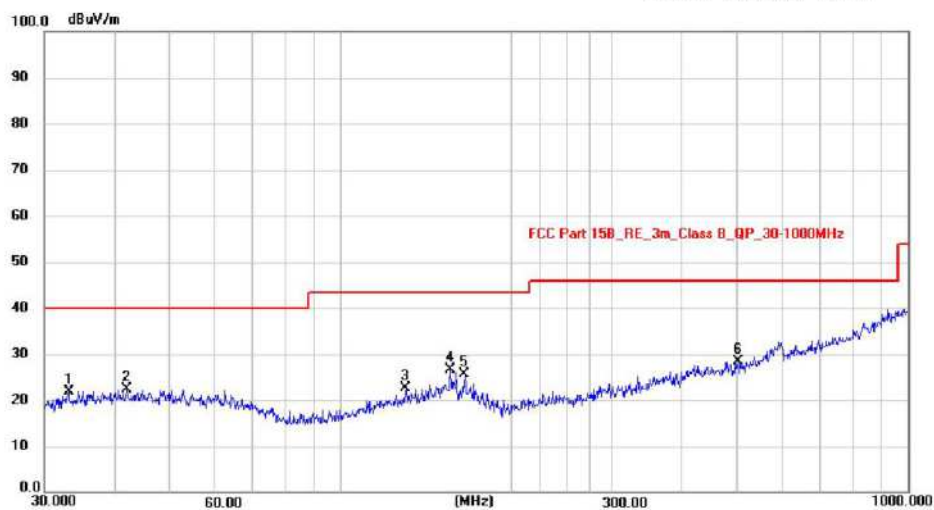

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	33.0950	8.47	13.52	21.99	40.00	-18.01	peak	100	321	P	
2	41.8596	7.78	14.49	22.27	40.00	-17.73	peak	100	45	P	
3	130.3789	9.38	13.25	22.63	43.50	-20.87	peak	100	254	P	
4 *	155.9101	12.34	14.26	26.60	43.50	-16.90	peak	100	126	P	
5	165.4866	11.72	13.81	25.53	43.50	-17.97	peak	100	39	P	
6	501.1790	8.20	20.19	28.39	46.00	-17.61	peak	100	48	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
M/N: Sara 1 Test Engineer: Felix Pang
Test Mode: GFSK 2480MHz
Test Voltage: DC 3.7V
Note:

Radiated Emission Measurement

Test Date: 2024/10/23 13:18:37



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	37.4165	9.09	14.19	23.28	40.00	-16.72	peak	200	45	P	
2	51.1209	9.35	14.03	23.38	40.00	-16.62	peak	200	65	P	
3 *	159.2251	19.30	14.33	33.63	43.50	-9.87	peak	200	123	P	
4	171.3926	17.53	13.24	30.77	43.50	-12.73	peak	200	256	P	
5	364.2595	13.16	16.72	29.88	46.00	-16.12	peak	200	44	P	
6	465.5994	9.77	19.32	29.09	46.00	-16.91	peak	200	265	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2402MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:21:04



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	38.4809	7.79	14.35	22.14	40.00	-17.86	peak	200	321	P	
2	52.7600	9.99	13.86	23.85	40.00	-16.15	peak	200	48	P	
3	57.9993	10.30	13.32	23.62	40.00	-16.38	peak	200	256	P	
4 *	158.1123	18.11	14.31	32.42	43.50	-11.08	peak	200	124	P	
5	171.9946	17.05	13.18	30.23	43.50	-13.27	peak	200	32	P	
6	364.2595	11.47	16.72	28.19	46.00	-17.81	peak	200	156	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2402MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:23:00

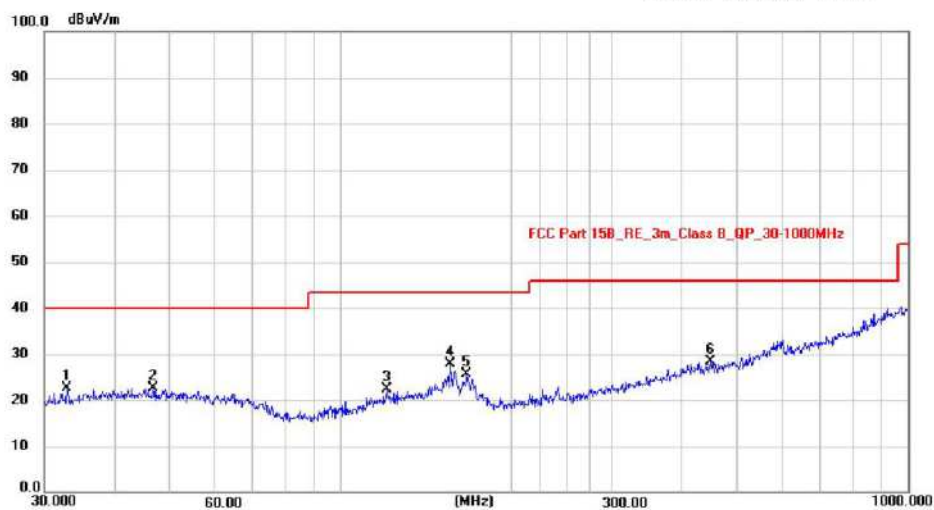

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	32.8637	9.11	13.48	22.59	40.00	-17.41	peak	100	125	P	
2	46.6664	8.34	14.29	22.63	40.00	-17.37	peak	100	256	P	
3	120.2766	9.75	12.57	22.32	43.50	-21.18	peak	100	48	P	
4 *	155.9101	13.67	14.26	27.93	43.50	-15.57	peak	100	65	P	
5	166.6514	12.04	13.70	25.74	43.50	-17.76	peak	100	321	P	
6	447.9822	9.51	18.89	28.40	46.00	-17.60	peak	100	257	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2441MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:26:22

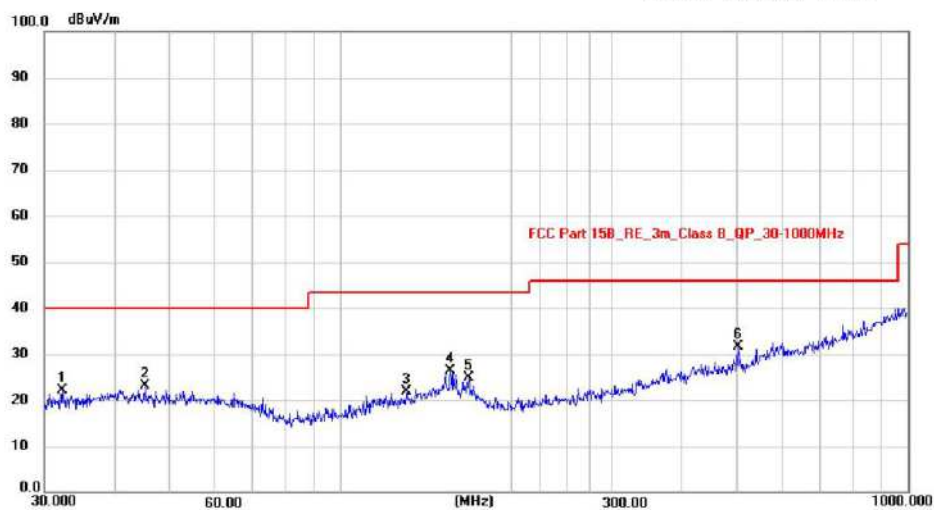

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	32.1795	8.79	13.37	22.16	40.00	-17.84	peak	100	254	P	
2	45.0583	8.68	14.36	23.04	40.00	-16.96	peak	100	127	P	
3	130.8369	8.72	13.28	22.00	43.50	-21.50	peak	100	28	P	
4	155.9101	12.09	14.26	26.35	43.50	-17.15	peak	100	49	P	
5	167.8243	11.25	13.59	24.84	43.50	-18.66	peak	100	265	P	
6 *	501.1790	11.48	20.19	31.67	46.00	-14.33	peak	100	45	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2441MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:29:50



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	38.2120	7.59	14.31	21.90	40.00	-18.10	peak	200	125	P	
2	45.3755	8.50	14.34	22.84	40.00	-17.16	peak	200	214	P	
3	54.8348	8.71	13.65	22.36	40.00	-17.64	peak	200	158	P	
4 *	159.7844	19.77	14.35	34.12	43.50	-9.38	peak	200	320	P	
5	171.3926	17.92	13.24	31.16	43.50	-12.34	peak	200	25	P	
6	364.2595	12.14	16.72	28.86	46.00	-17.14	peak	200	65	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2480MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:32:11



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	38.8878	7.51	14.40	21.91	40.00	-18.09	peak	200	258	P	
2	46.0164	8.14	14.31	22.45	40.00	-17.55	peak	200	45	P	
3	51.8430	8.43	13.96	22.39	40.00	-17.61	peak	200	210	P	
4 *	159.7844	18.69	14.35	33.04	43.50	-10.46	peak	200	326	P	
5	171.3926	16.90	13.24	30.14	43.50	-13.36	peak	200	58	P	
6	364.2595	11.42	16.72	28.14	46.00	-17.86	peak	200	98	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2480MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:36:36

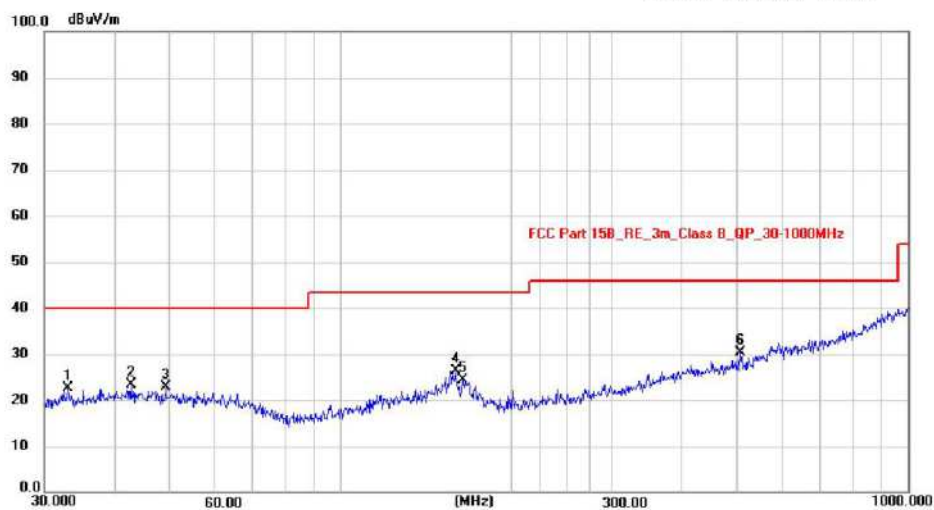

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	32.9791	9.24	13.50	22.74	40.00	-17.26	peak	100	125	P	
2	42.6000	9.03	14.46	23.49	40.00	-16.51	peak	100	201	P	
3	49.0145	8.70	14.19	22.89	40.00	-17.11	peak	100	54	P	
4	159.2251	12.04	14.33	26.37	43.50	-17.13	peak	100	78	P	
5	163.7550	10.43	13.98	24.41	43.50	-19.09	peak	100	203	P	
6 *	506.4791	10.08	20.33	30.41	46.00	-15.59	peak	100	65	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
M/N: Sara 1 Test Engineer: Felix Pang
Test Mode: 8DPSK 2402MHz
Test Voltage: DC 3.7V
Note:

Radiated Emission Measurement

Test Date: 2024/10/23 13:39:58

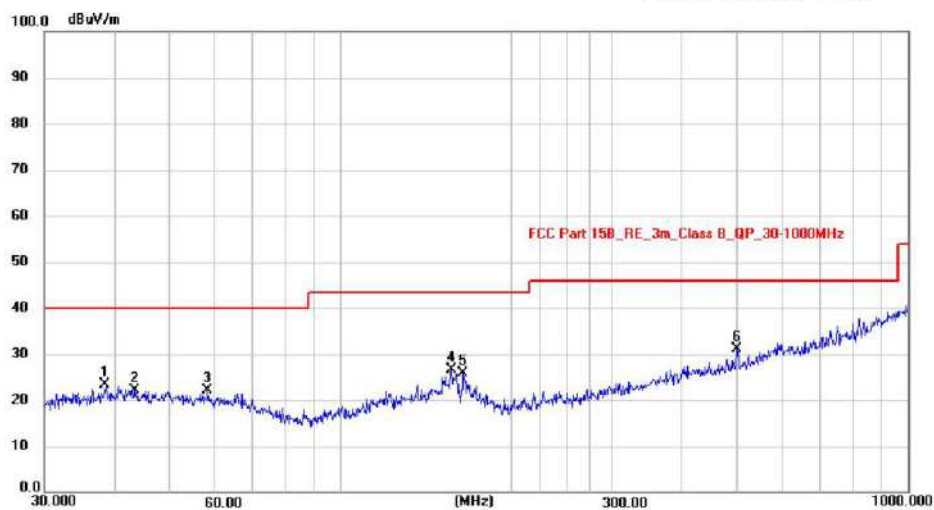

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	38.4809	8.92	14.35	23.27	40.00	-16.73	peak	100	25	P	
2	43.3534	7.72	14.43	22.15	40.00	-17.85	peak	100	120	P	
3	58.2030	8.73	13.30	22.03	40.00	-17.97	peak	100	258	P	
4	156.4578	12.37	14.27	26.64	43.50	-16.86	peak	100	69	P	
5	164.3301	11.99	13.93	25.92	43.50	-17.58	peak	100	159	P	
6 *	499.4247	11.03	20.14	31.17	46.00	-14.83	peak	100	357	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: 8DPSK 2402MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:42:41



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	36.7662	8.40	14.10	22.50	40.00	-17.50	peak	200	154	P	
2	39.9942	7.97	14.57	22.54	40.00	-17.46	peak	200	210	P	
3	48.6719	8.36	14.20	22.56	40.00	-17.44	peak	200	258	P	
4 *	159.7844	18.45	14.35	32.80	43.50	-10.70	peak	200	352	P	
5	171.3926	17.19	13.24	30.43	43.50	-13.07	peak	200	12	P	
6	364.2595	12.12	16.72	28.84	46.00	-17.16	peak	200	150	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: 8DPSK 2441MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:46:00



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	32.5198	8.61	13.42	22.03	40.00	-17.97	peak	200	102	P	
2	44.1202	8.37	14.39	22.76	40.00	-17.24	peak	200	145	P	
3 *	160.3456	20.02	14.32	34.34	43.50	-9.16	peak	200	57	P	
4	171.9946	18.50	13.18	31.68	43.50	-11.82	peak	200	89	P	
5	364.2595	11.62	16.72	28.34	46.00	-17.66	peak	200	201	P	
6	595.1329	9.59	22.75	32.34	46.00	-13.66	peak	200	231	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: 8DPSK 2441MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:51:29

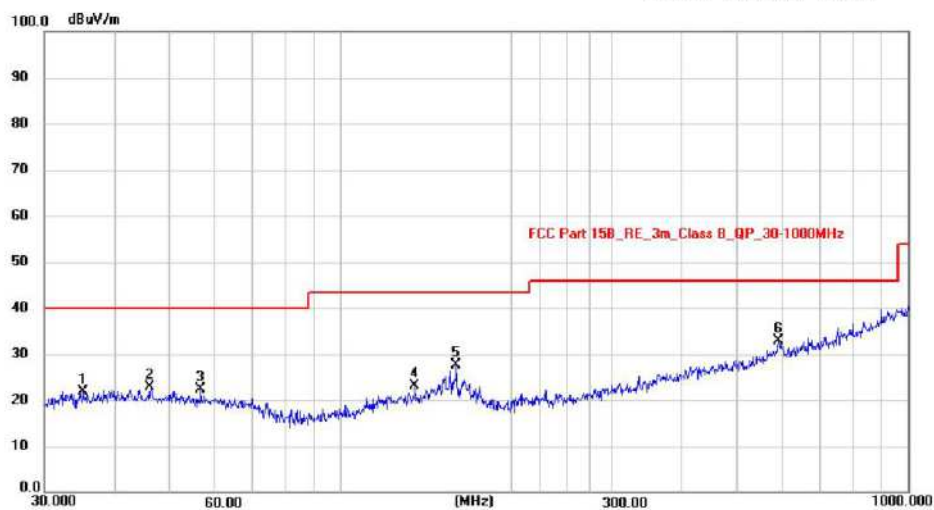

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	35.1278	8.12	13.86	21.98	40.00	-18.02	peak	100	254	P	
2	46.1779	8.55	14.31	22.86	40.00	-17.14	peak	100	120	P	
3	56.5929	8.81	13.46	22.27	40.00	-17.73	peak	100	236	P	
4	135.0319	9.46	13.57	23.03	43.50	-20.47	peak	100	225	P	
5	159.7844	13.22	14.35	27.57	43.50	-15.93	peak	100	102	P	
6 *	590.9737	10.12	22.64	32.76	46.00	-13.24	peak	100	298	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: 8DPSK 2480MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:55:50



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	39.5757	8.03	14.51	22.54	40.00	-17.46	peak	100	114	P	
2	43.2017	8.28	14.43	22.71	40.00	-17.29	peak	100	258	P	
3	48.1626	7.94	14.22	22.16	40.00	-17.84	peak	100	98	P	
4	155.9101	12.19	14.26	26.45	43.50	-17.05	peak	100	65	P	
5	166.0680	11.61	13.76	25.37	43.50	-18.13	peak	100	201	P	
6 *	595.1329	9.45	22.75	32.20	46.00	-13.80	peak	100	118	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: 8DPSK 2480MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/23 13:59:18



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	41.7129	7.88	14.49	22.37	40.00	-17.63	peak	200	226	P	
2	53.6932	9.12	13.76	22.88	40.00	-17.12	peak	200	301	P	
3 *	159.2251	18.53	14.33	32.86	43.50	-10.64	peak	200	157	P	
4	171.9946	17.44	13.18	30.62	43.50	-12.88	peak	200	48	P	
5	413.2706	12.98	18.06	31.04	46.00	-14.96	peak	200	95	P	
6	599.3212	10.42	22.86	33.28	46.00	-12.72	peak	200	326	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

1GHz - 18GHz




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: GFSK 2402MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 12:31:06

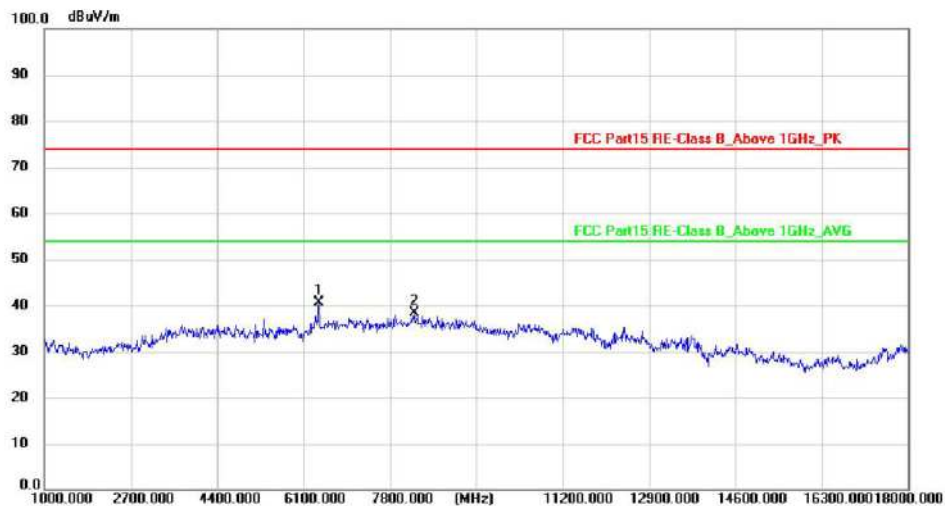

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	6406.000	50.40	-9.73	40.67	74.00	-33.33	peak	150	103	P	
2	8276.000	45.31	-6.90	38.41	74.00	-35.59	peak	150	265	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: GFSK 2402MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/24 12:35:34

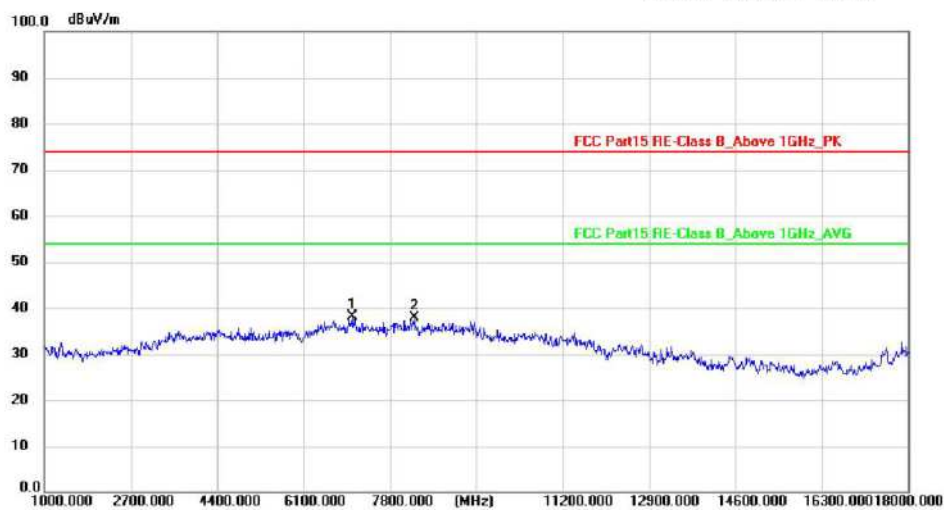

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	7052.000	46.13	-8.00	38.13	74.00	-35.87	peak	150	54	P	
2	8278.125	44.70	-6.90	37.80	74.00	-36.20	peak	150	129	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: GFSK 2441MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/24 12:38:58



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	6531.375	46.53	-9.36	37.17	74.00	-36.83	peak	150	265	P	
2 *	8267.500	44.45	-6.90	37.55	74.00	-36.45	peak	150	124	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
M/N: Sara 1 Test Engineer: Felix Pang
Test Mode: GFSK 2441MHz
Test Voltage: DC 3.7V
Note:

Radiated Emission Measurement

Test Date: 2024/10/24 12:45:22

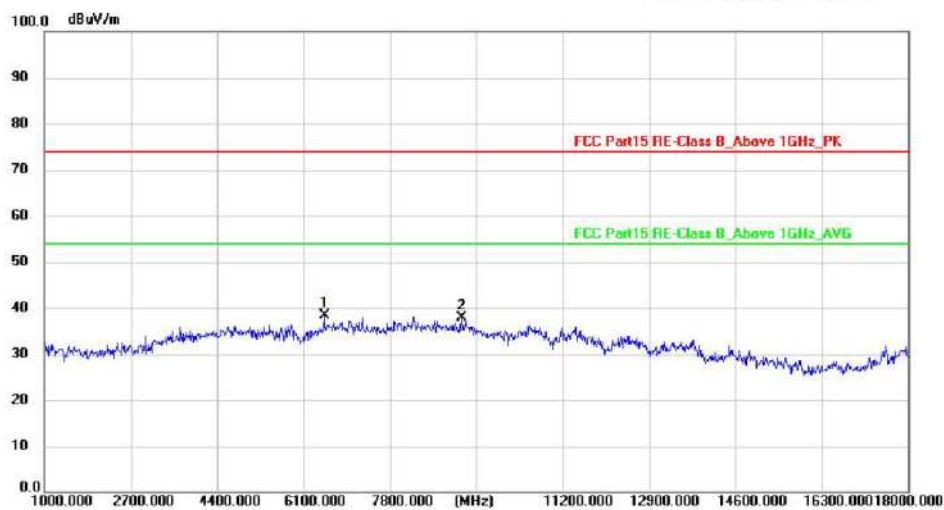

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	6508.000	47.77	-9.44	38.33	74.00	-35.67	peak	150	215	P	
2	9217.375	43.91	-6.07	37.84	74.00	-36.16	peak	150	126	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: GFSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 12:47:27

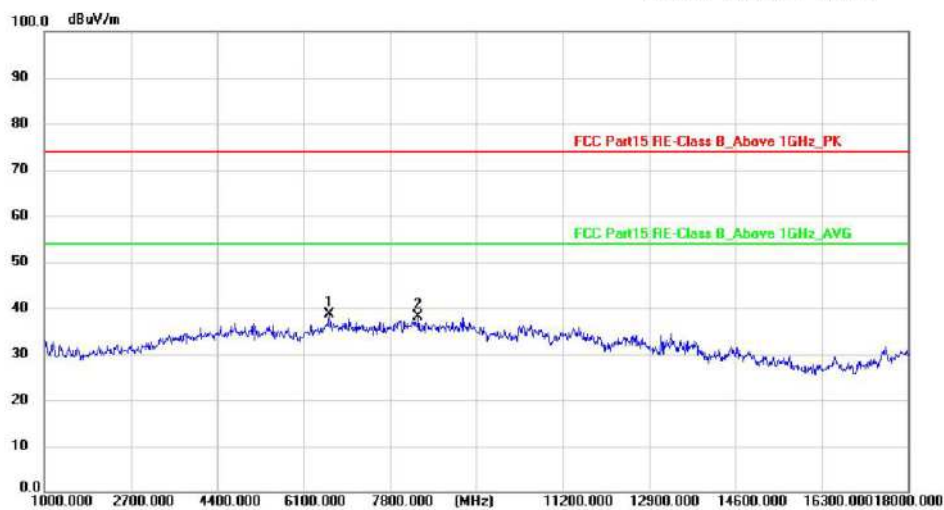

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	6612.125	47.72	-9.14	38.58	74.00	-35.42	peak	150	236	P	
2	8365.250	44.92	-6.81	38.11	74.00	-35.89	peak	150	254	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: GFSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 12:49:56



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	6484.625	46.81	-9.50	37.31	74.00	-36.69	peak	150	78	P	
2 *	8099.625	44.58	-7.07	37.51	74.00	-36.49	peak	150	126	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: Pi/4DQPSK 2402MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 12:52:29



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	6703.500	47.11	-8.88	38.23	74.00	-35.77	peak	150	204	P	
2 *	8252.625	45.27	-6.92	38.35	74.00	-35.65	peak	150	135	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: Pi/4DQPSK 2402MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 12:56:56



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	6406.000	49.05	-9.73	39.32	74.00	-34.68	peak	150	215	P	
2	8273.875	44.79	-6.90	37.89	74.00	-36.11	peak	150	126	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2441MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/24 12:59:49



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	6510.125	47.48	-9.44	38.04	74.00	-35.96	peak	150	165	P	
2 *	8093.250	45.24	-7.08	38.16	74.00	-35.84	peak	150	129	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
 1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
 Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
 EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
 M/N: Sara 1 Test Engineer: Felix Pang
 Test Mode: Pi/4DQPSK 2441MHz
 Test Voltage: DC 3.7V
 Note:

Radiated Emission Measurement

Test Date: 2024/10/24 13:03:18



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	4780.375	50.22	-13.34	36.88	74.00	-37.12	peak	150	98	P	
2 *	8569.250	43.99	-6.62	37.37	74.00	-36.63	peak	150	125	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
 1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
 Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
 EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
 M/N: Sara 1 Test Engineer: Felix Pang
 Test Mode: Pi/4DQPSK 2480MHz
 Test Voltage: DC 3.7V
 Note:

Radiated Emission Measurement

Test Date: 2024/10/24 13:06:02

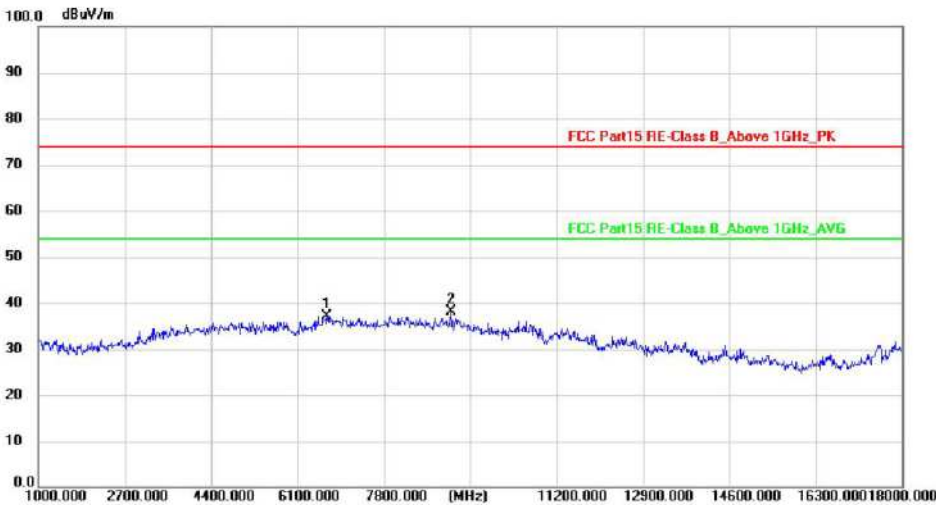

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	6688.625	45.95	-8.91	37.04	74.00	-36.96	peak	150	127	P	
2 *	9128.125	44.34	-6.12	38.22	74.00	-35.78	peak	150	247	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: Pi/4DQPSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 13:09:28



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	4251.250	58.25	-15.45	42.80	74.00	-31.20	peak	150	321	P	
2	6612.125	46.76	-9.14	37.62	74.00	-36.38	peak	150	157	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: 8DPSK 2402MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 13:12:38

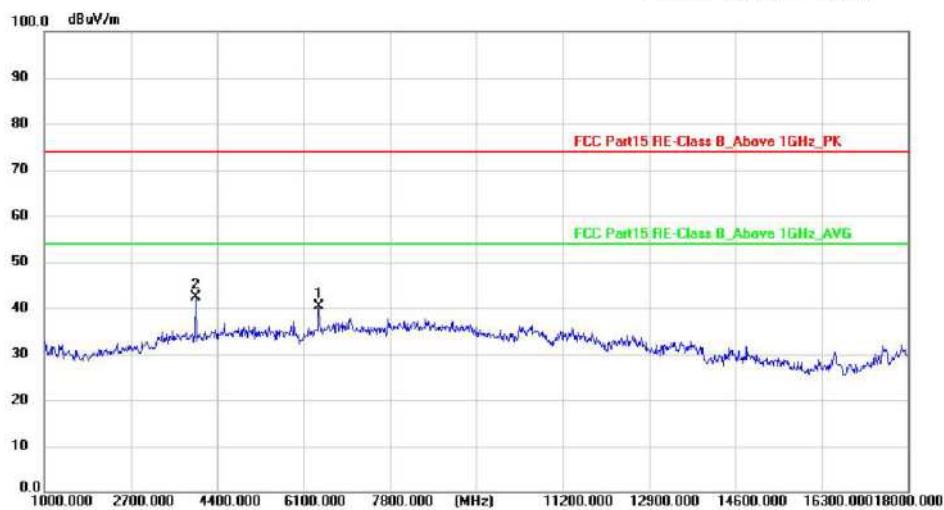

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	6406.000	50.12	-9.73	40.39	74.00	-33.61	peak	150	102	P	
2 *	3985.625	58.58	-16.14	42.44	74.00	-31.56	peak	150	325	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: 8DPSK 2402MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 13:18:08

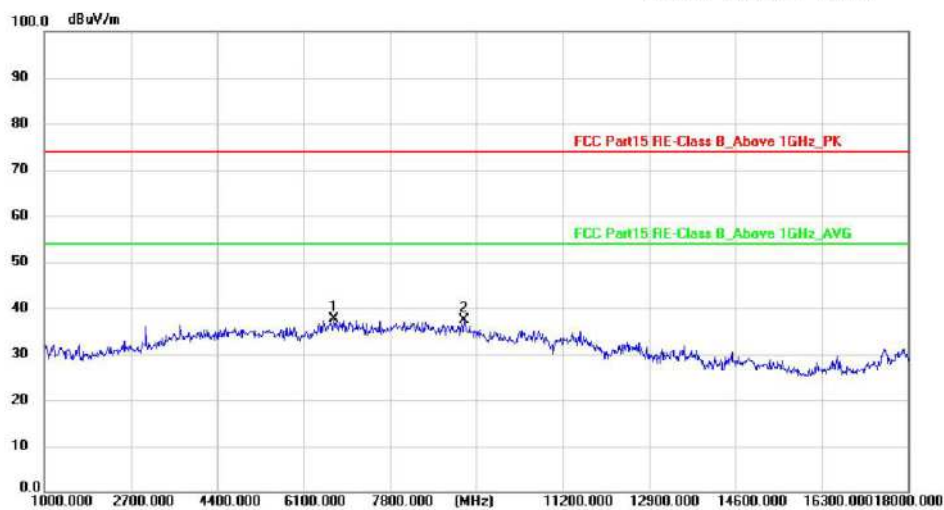

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	6703.500	46.44	-8.88	37.56	74.00	-36.44	peak	150	126	P	
2	9264.125	43.42	-6.05	37.37	74.00	-36.63	peak	150	254	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
 1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
 Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
 EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
 M/N: Sara 1 Test Engineer: Felix Pang
 Test Mode: 8DPSK 2441MHz
 Test Voltage: DC 3.7V
 Note:

Radiated Emission Measurement

Test Date: 2024/10/24 13:22:15



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	7018.000	46.96	-8.03	38.93	74.00	-35.07	peak	150	159	P	
2	8579.875	44.64	-6.61	38.03	74.00	-35.97	peak	150	235	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: 8DPSK 2441MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 13:26:39



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	3989.875	55.12	-16.12	39.00	74.00	-35.00	peak	150	217	P	
2	7030.750	46.77	-8.02	38.75	74.00	-35.25	peak	150	158	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: 8DPSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 13:29:14

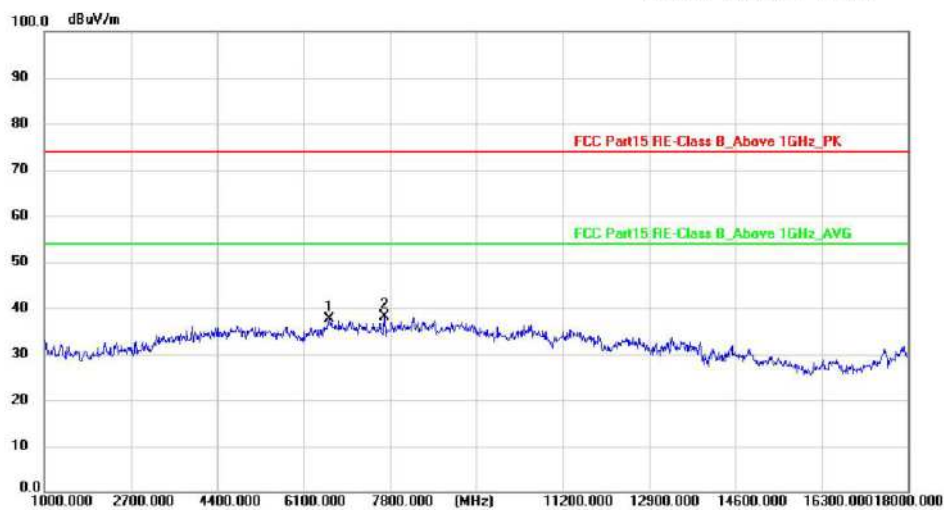

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	6614.250	46.86	-9.13	37.73	74.00	-36.27	peak	150	321	P	
2 *	7700.125	45.54	-7.43	38.11	74.00	-35.89	peak	150	157	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: 8DPSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 13:34:49



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	4482.875	51.09	-14.39	36.70	74.00	-37.30	peak	150	124	P	
2 *	7453.625	45.26	-7.64	37.62	74.00	-36.38	peak	150	208	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix A.8: Test Results of Radiated Emissions in Restricted Bands




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
M/N: Sara 1 Test Engineer: Felix Pang
Test Mode: GFSK 2402MHz
Test Voltage: DC 3.7V
Note:

Radiated Emission Measurement

Test Date: 2024/10/24 14:35:16

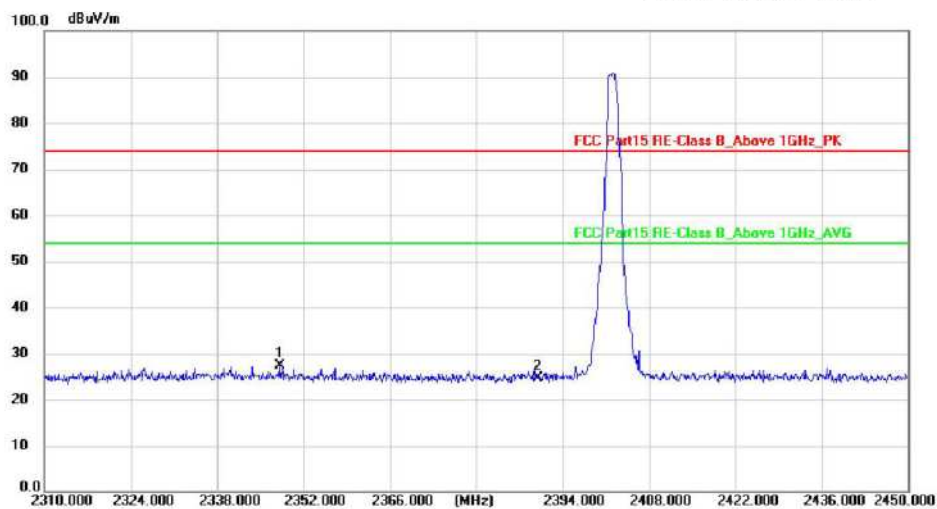

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2348.133	53.64	-26.24	27.40	74.00	-46.60	peak	150	126	P	
2	2390.000	50.67	-26.12	24.55	74.00	-49.45	peak	150	254	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
M/N: Sara 1 Test Engineer: Felix Pang
Test Mode: GFSK 2402MHz
Test Voltage: DC 3.7V
Note:

Radiated Emission Measurement

Test Date: 2024/10/24 14:38:21

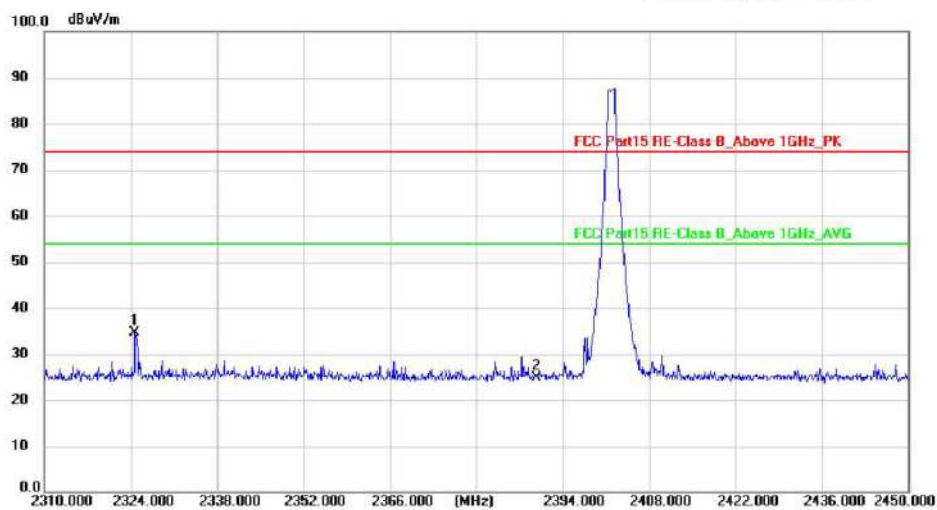

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2324.805	60.99	-26.32	34.67	74.00	-39.33	peak	150	103	P	
2	2390.000	51.11	-26.12	24.99	74.00	-49.01	peak	150	254	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: GFSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 14:42:01

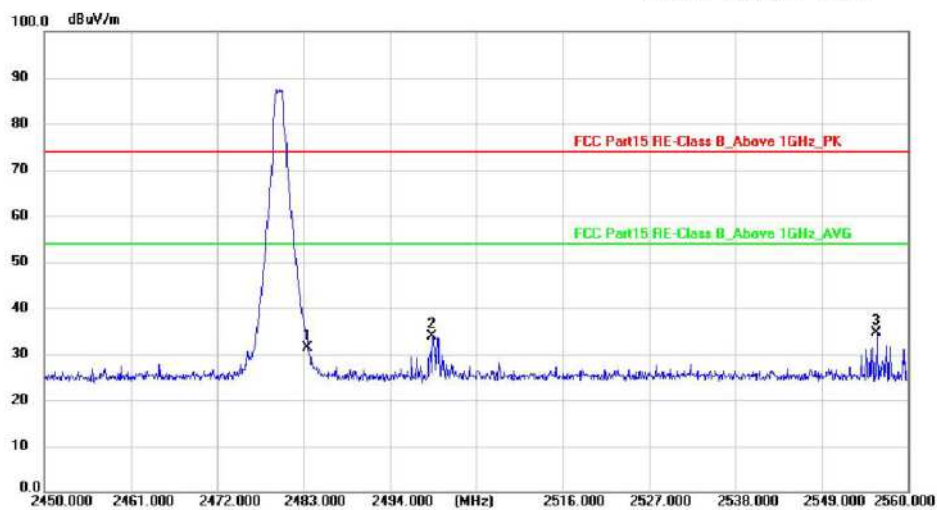

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	2483.500	57.33	-25.84	31.49	74.00	-42.51	peak	150	102	P	
2	2499.541	59.75	-25.78	33.97	74.00	-40.03	peak	150	357	P	
3 *	2556.136	60.20	-25.62	34.58	74.00	-39.42	peak	150	257	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: GFSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 14:46:59

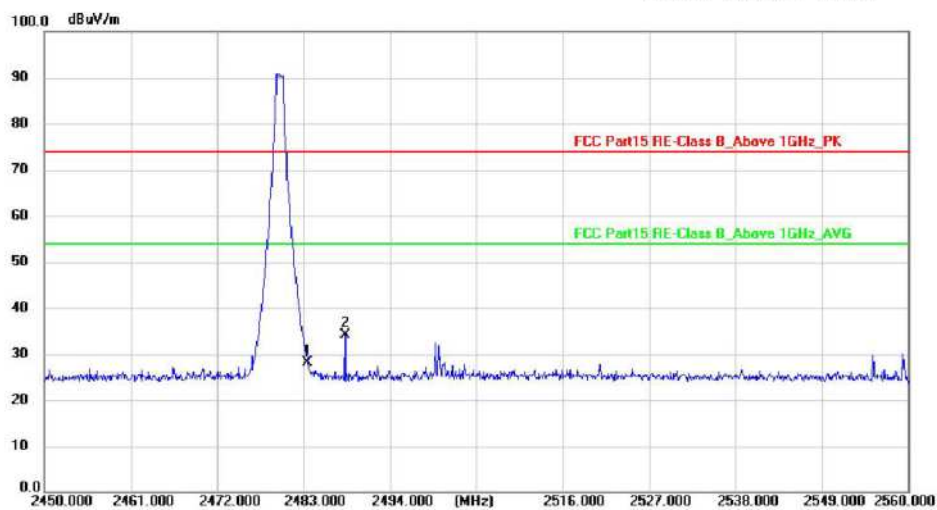

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	2483.500	53.90	-25.84	28.06	74.00	-45.94	peak	150	209	P	
2 *	2488.363	59.96	-25.82	34.14	74.00	-39.86	peak	150	320	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2402MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/24 14:50:13

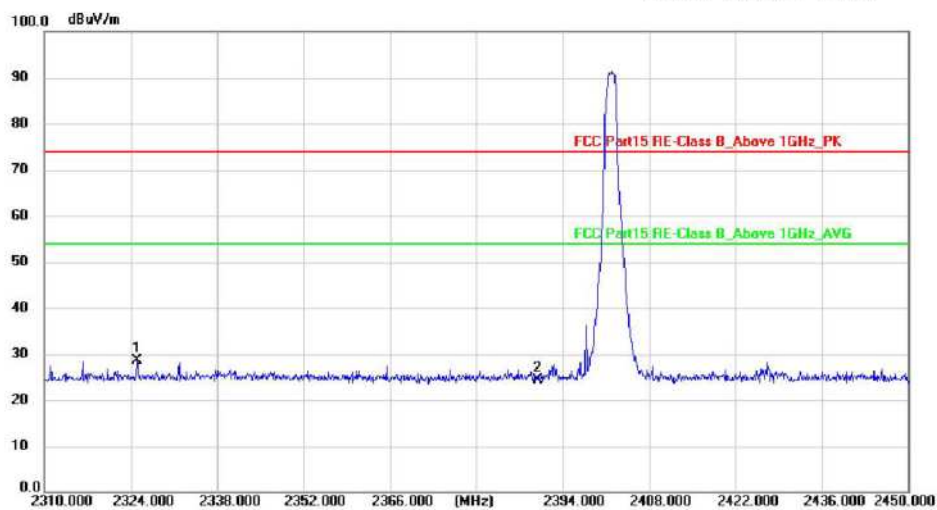

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2325.050	55.06	-26.32	28.74	74.00	-45.26	peak	150	204	P	
2	2390.000	50.52	-26.12	24.40	74.00	-49.60	peak	150	125	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2402MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Vertical**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/24 14:58:33

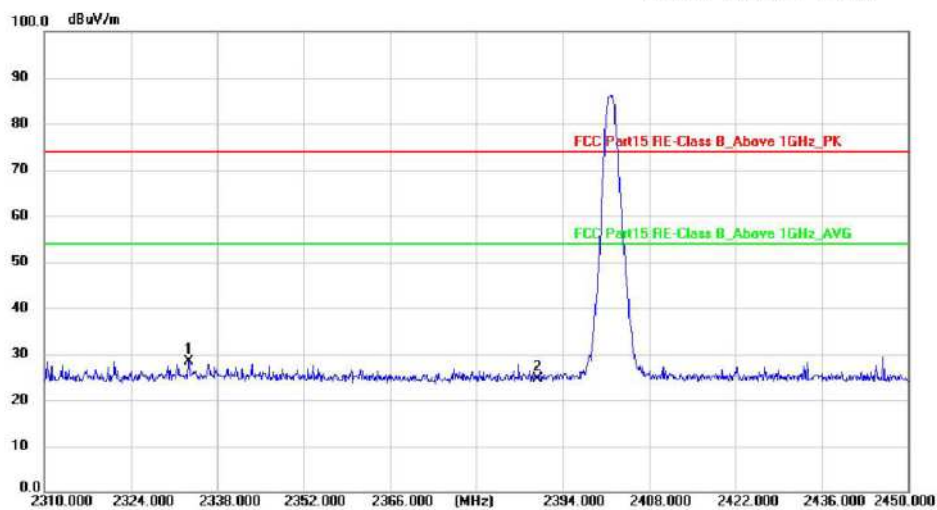

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2333.450	54.57	-26.28	28.29	74.00	-45.71	peak	150	98	P	
2	2390.000	50.85	-26.12	24.73	74.00	-49.27	peak	150	208	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: Pi/4DQPSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 15:08:50

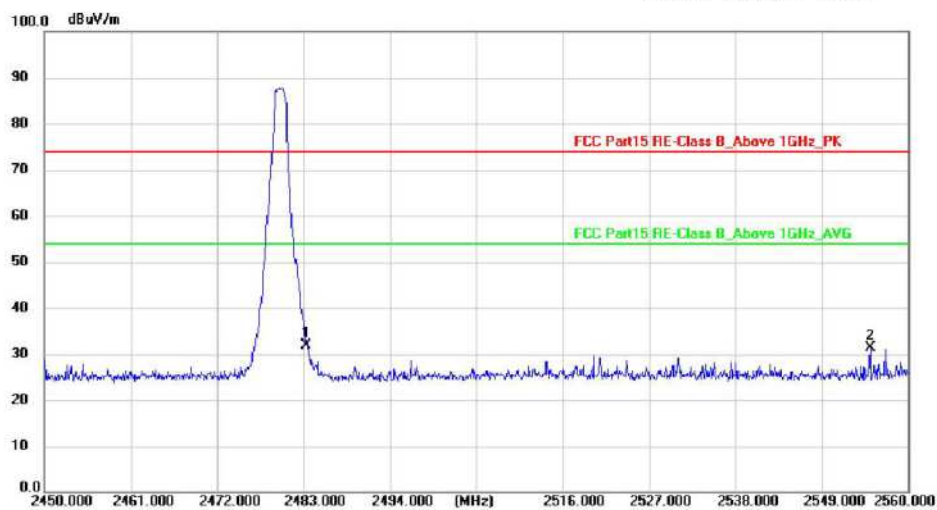

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2483.500	57.61	-25.84	31.77	74.00	-42.23	peak	150	157	P	
2	2555.188	57.05	-25.62	31.43	74.00	-42.57	peak	150	214	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: ITE Hearing Aids
M/N: Sara 1
Test Mode: Pi/4DQPSK 2480MHz
Test Voltage: DC 3.7V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix Pang

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2024/10/24 15:14:54

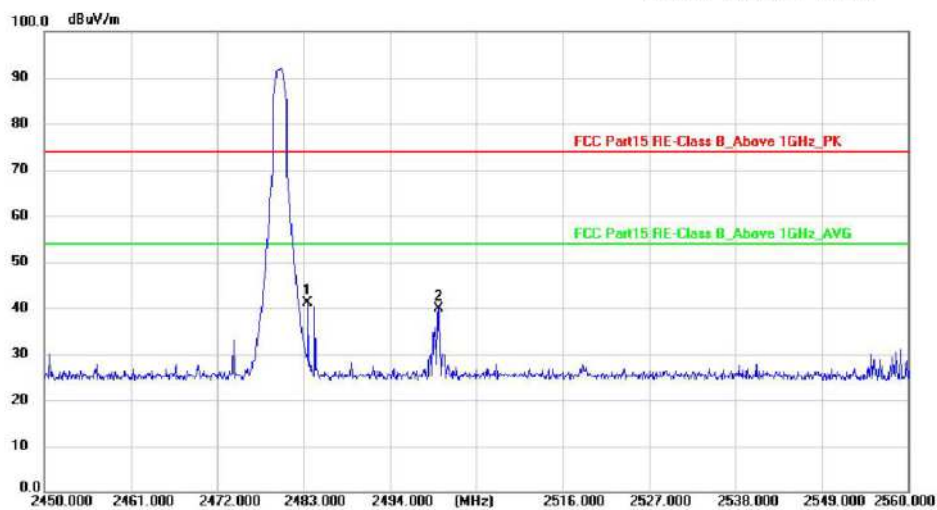

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2483.500	67.02	-25.84	41.18	74.00	-32.82	peak	150	201	P	
2	2500.174	65.78	-25.78	40.00	74.00	-34.00	peak	150	156	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
 1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
 Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
 EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
 M/N: Sara 1 Test Engineer: Felix Pang
 Test Mode: 8DPSK 2402MHz
 Test Voltage: DC 3.7V
 Note:

Radiated Emission Measurement

Test Date: 2024/10/24 15:19:58

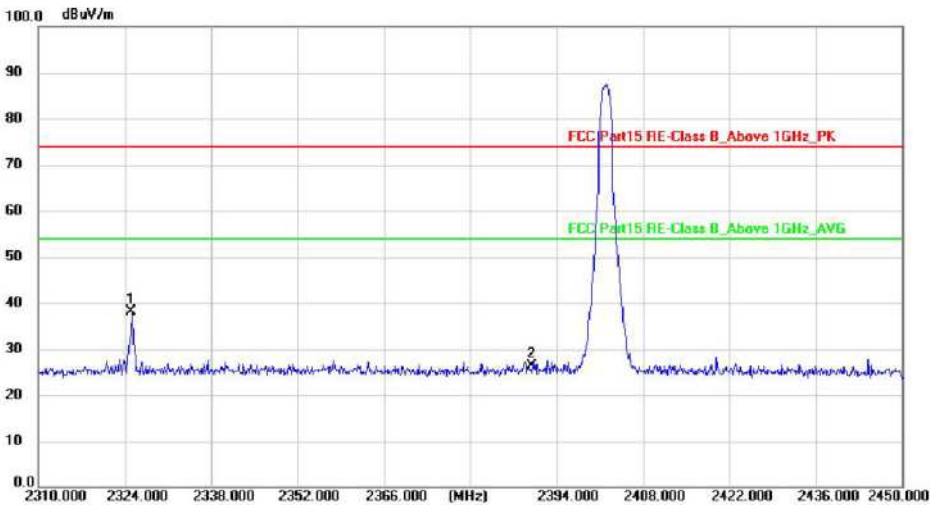

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2325.207	64.53	-26.32	38.21	74.00	-35.79	peak	150	145	P	
2	2390.000	52.43	-26.12	26.31	74.00	-47.69	peak	150	267	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: 8DPSK 2402MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 15:24:07

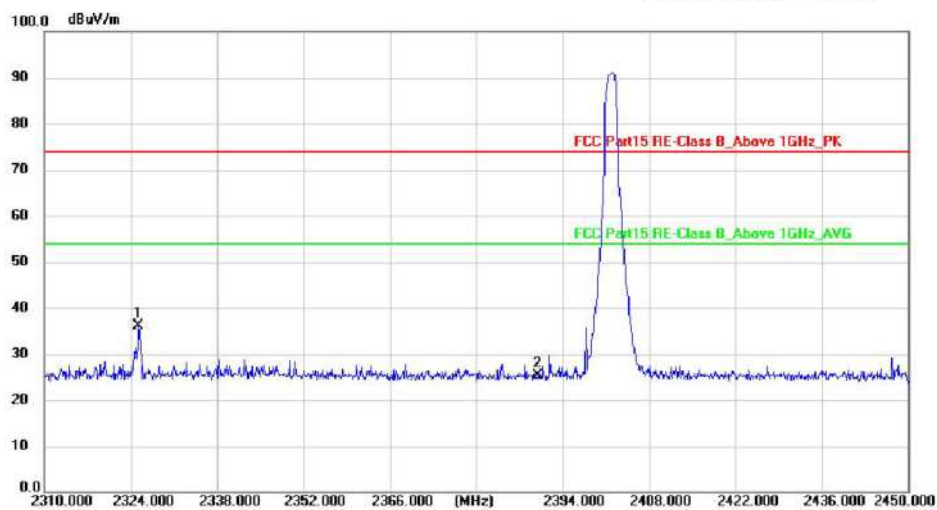

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	2325.383	62.41	-26.32	36.09	74.00	-37.91	peak	150	206	P	
2	2390.000	51.52	-26.12	25.40	74.00	-48.60	peak	150	218	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: ITE Hearing Aids Distance: 3m Humidity: 54 %RH
M/N: Sara 1 Test Engineer: Felix Pang
Test Mode: 8DPSK 2480MHz
Test Voltage: DC 3.7V
Note:

Radiated Emission Measurement

Test Date: 2024/10/24 15:28:32

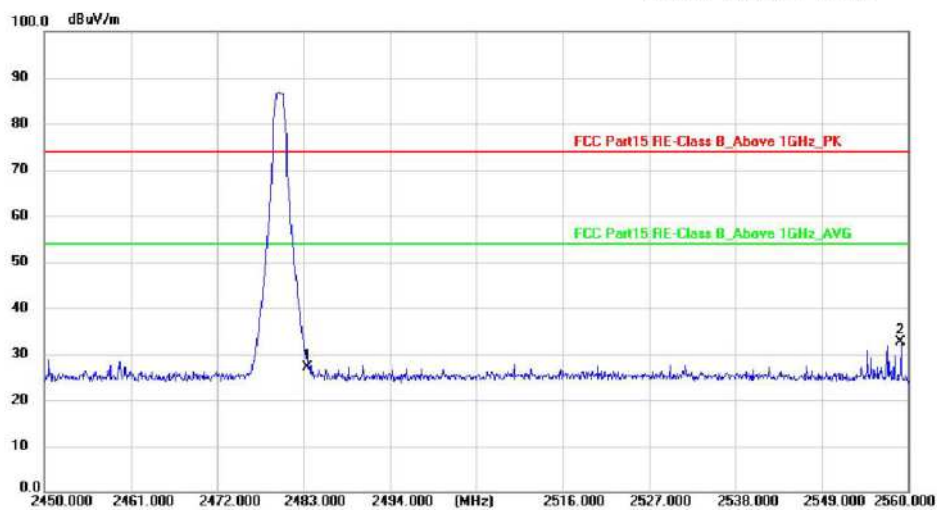

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	2483.500	52.87	-25.84	27.03	74.00	-46.97	peak	150	78	P	
2 *	2559.216	58.12	-25.60	32.52	74.00	-41.48	peak	150	125	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: ITE Hearing Aids	Distance: 3m	Humidity: 54 %RH
M/N: Sara 1	Test Engineer: Felix Pang	
Test Mode: 8DPSK 2480MHz		
Test Voltage: DC 3.7V		
Note:		

Radiated Emission Measurement

Test Date: 2024/10/24 15:32:19

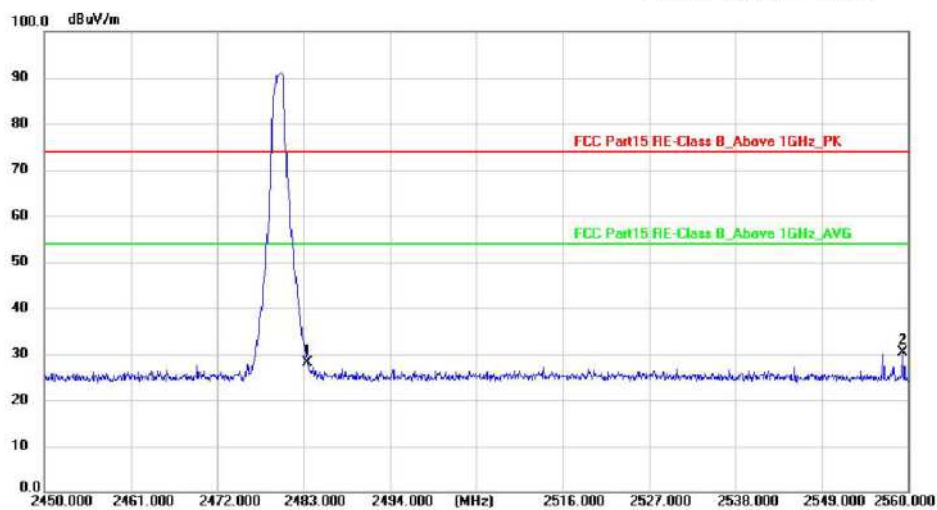

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	2483.500	53.86	-25.84	28.02	74.00	-45.98	peak	150	21	P	
2 *	2559.409	56.04	-25.60	30.44	74.00	-43.56	peak	150	157	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit