

Date: 2025/8/31

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.53, 10.34, 10.38); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.54 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.2 W/kg; SAR (10g) = 1.4 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

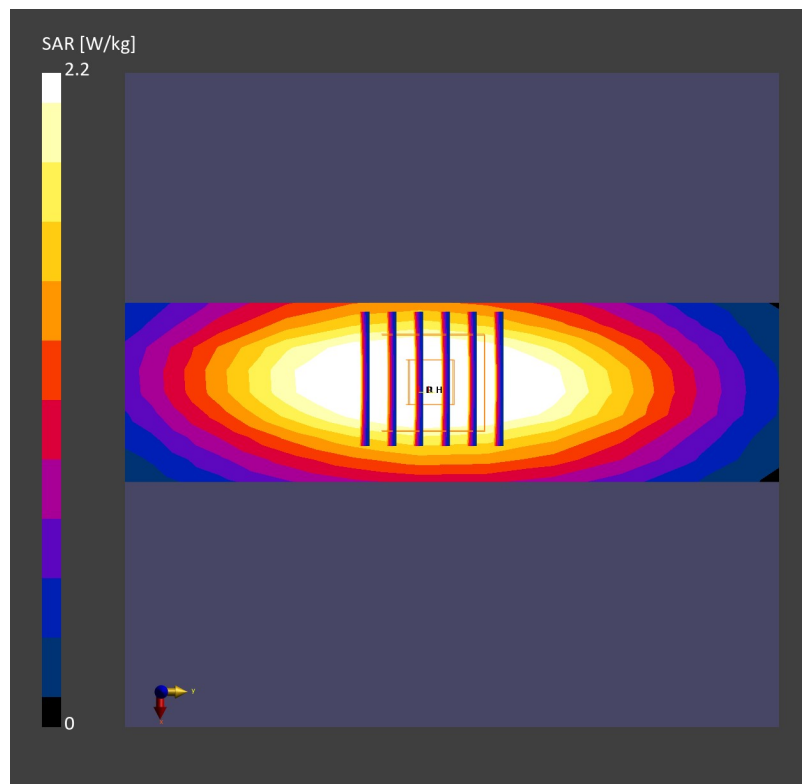

Date: 2025/8/31

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.919$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.23, 10.04, 10.08); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (36.0 mm x 210.0 mm): Measurement Grid: 3.0 mm x 15.0 mm

SAR (1g) = 2.58 W/kg; SAR (10g) = 1.70 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.41 W/kg; SAR (10g) = 1.55 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

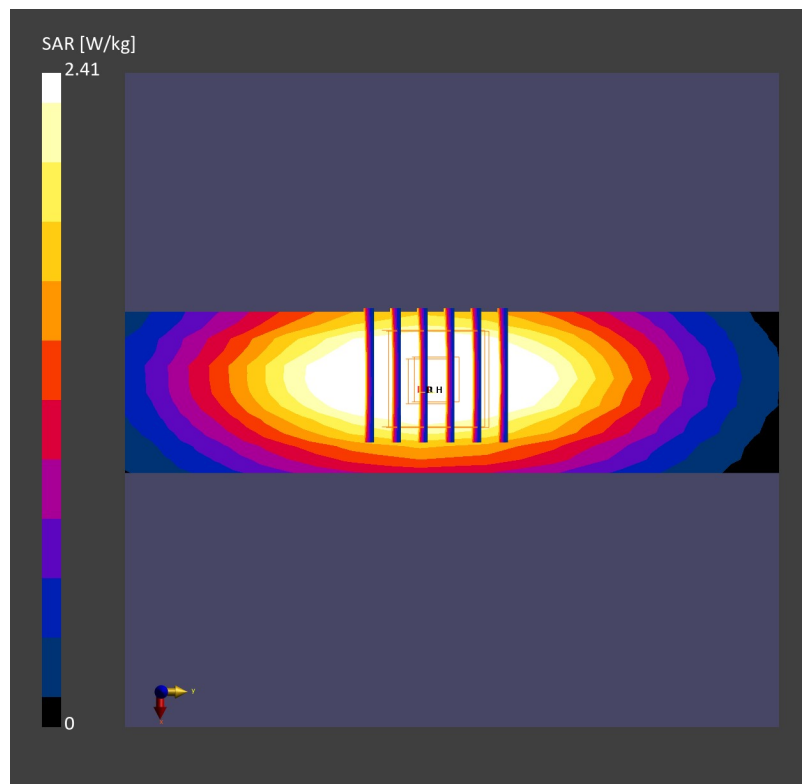

Date: 2025/8/31

System Check_2450MHz**DUT:D2450V2-SN:924**

Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 13.0 W/kg; SAR (10g) = 6.14 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 13.2 W/kg; SAR (10g) = 6.13 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

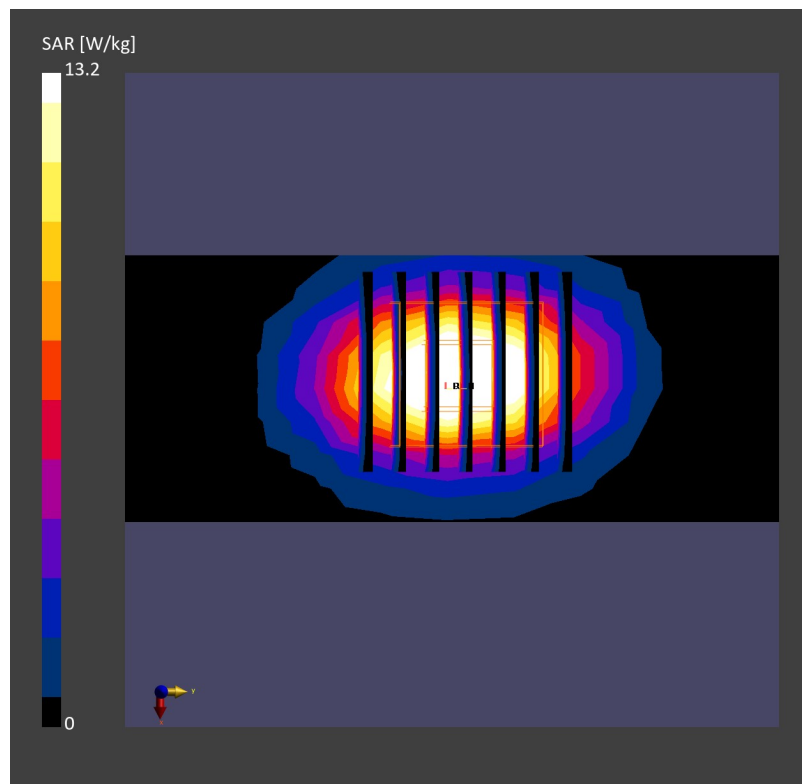

Date: 2025/8/31

System Check_3500MHz**DUT:D3500V2-SN:1037**

Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.77$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.99, 6.86, 6.89); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 6.31 W/kg; SAR (10g) = 2.46 W/kg;


Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 6.48 W/kg; SAR (10g) = 2.52 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

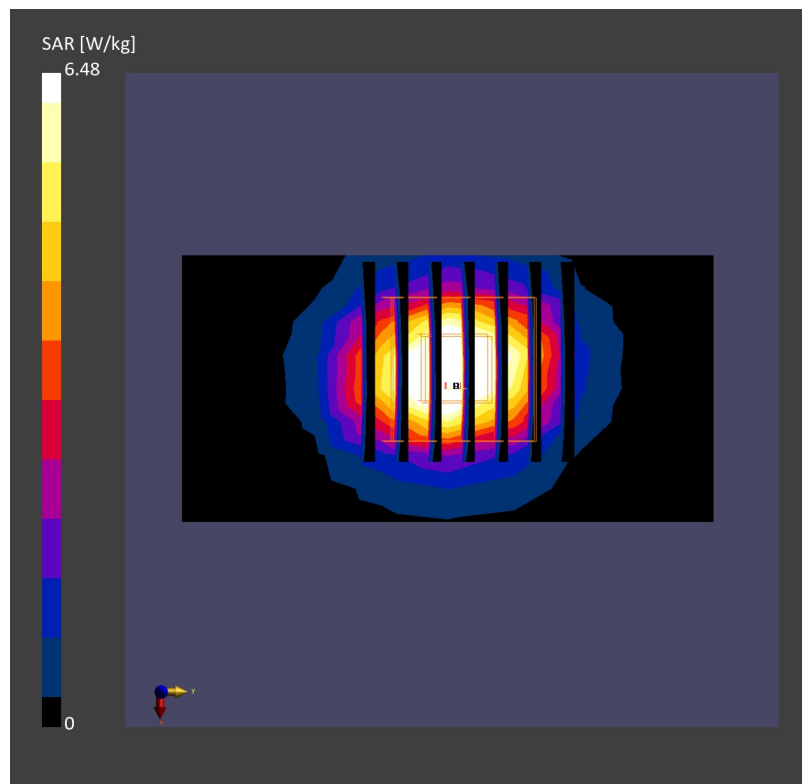

Date: 2025/8/31

System Check_3700MHz**DUT:D3700V2-SN:1008**

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.85, 6.72, 6.76); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.22 W/kg; SAR (10g) = 2.72 W/kg;


Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 7.21 W/kg; SAR (10g) = 2.63 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

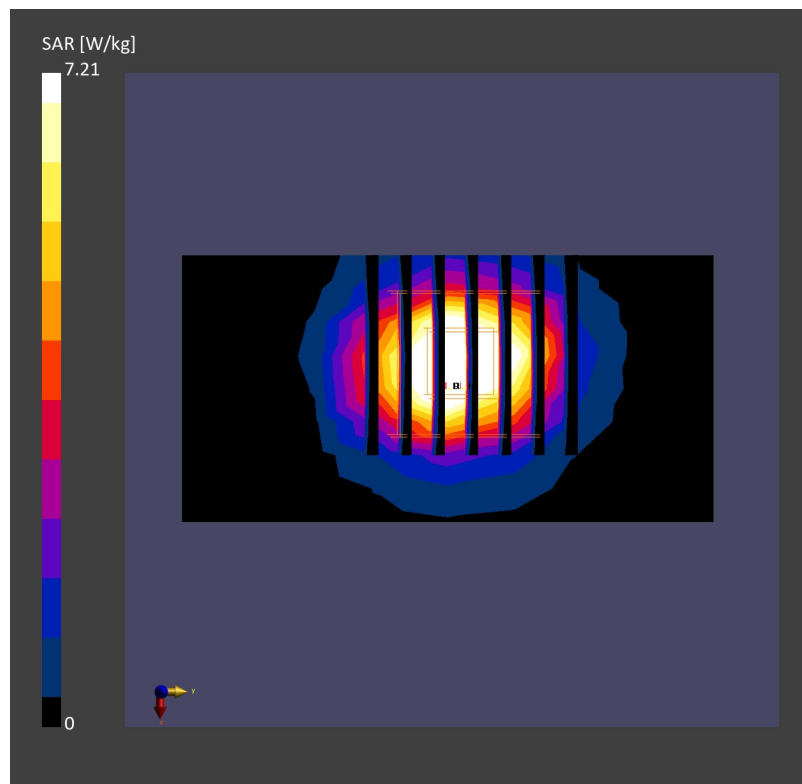

Date: 2025/8/31

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.52, 5.42, 5.44); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.60 W/kg; SAR (10g) = 2.17 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 8.07 W/kg; SAR (10g) = 2.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 57.8 %

