

Date: 2026-02-15

System Check_2450MHz**DUT:D2450V2-SN:929**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.0 W/kg; SAR (10g) = 6.21 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.07 dB

SAR (1g) = 12.8 W/kg; SAR (10g) = 5.95 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

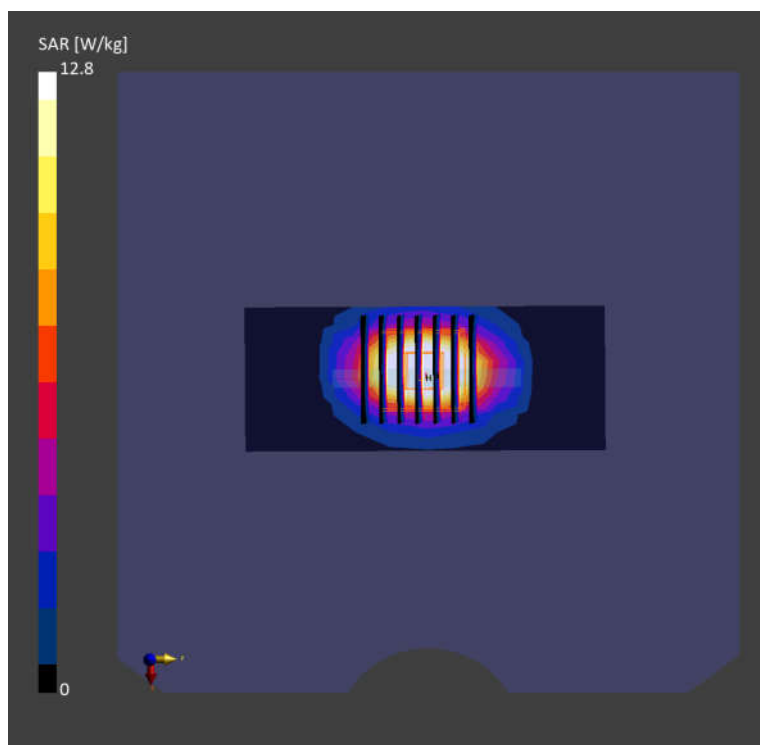

Date: 2026-02-17

System Check_2450MHz**DUT:D2450V2-SN:929**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.80$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.1 W/kg; SAR (10g) = 6.22 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 13.0 W/kg; SAR (10g) = 6.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

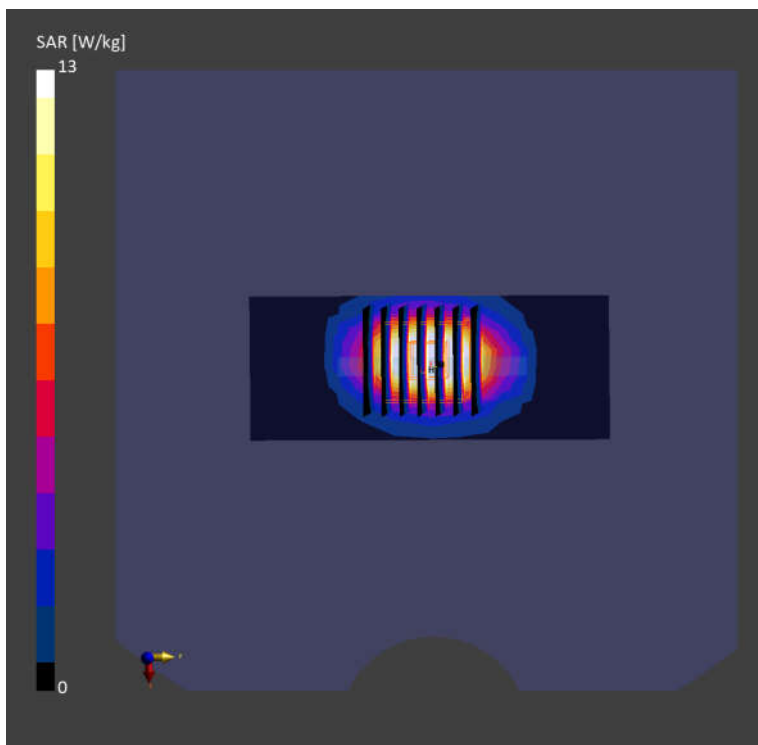

Date: 2026-02-14

System Check_5250MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.53$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.80, 5.57, 5.56); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.88 W/kg; SAR (10g) = 2.17 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 7.73 W/kg; SAR (10g) = 2.19 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.1 %

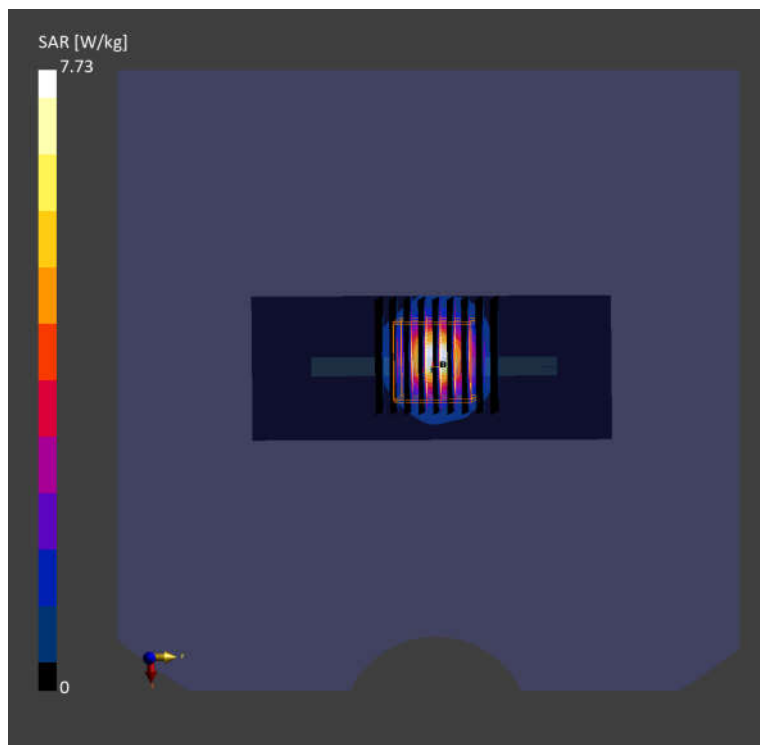

Date: 2026-02-16

System Check_5250MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.5$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.80, 5.57, 5.56); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.08 W/kg; SAR (10g) = 2.27 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 8.15 W/kg; SAR (10g) = 2.29 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.1 %

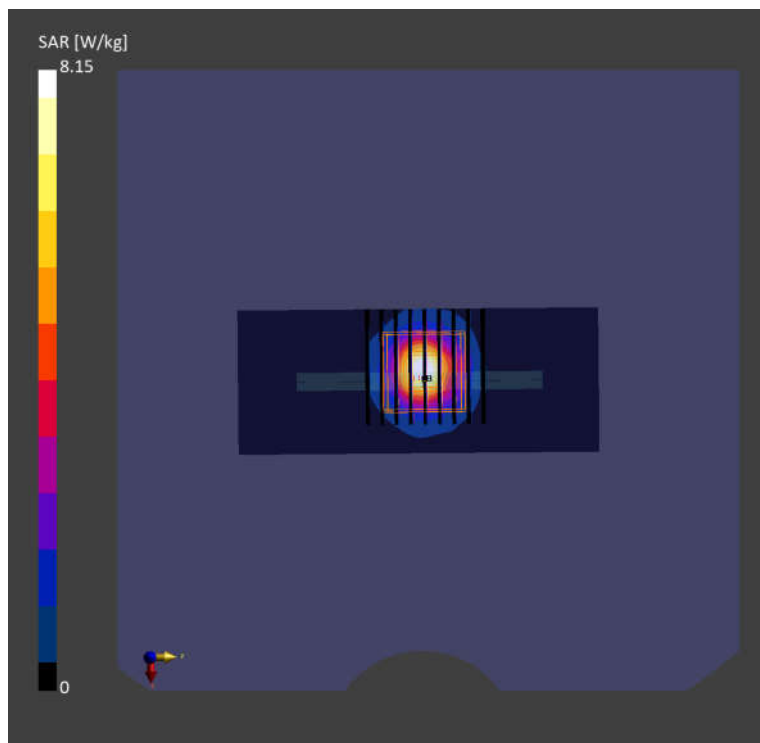

Date: 2026-02-18

System Check_5600MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.87$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.91 W/kg; SAR (10g) = 2.34 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 7.85 W/kg; SAR (10g) = 2.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.1 %

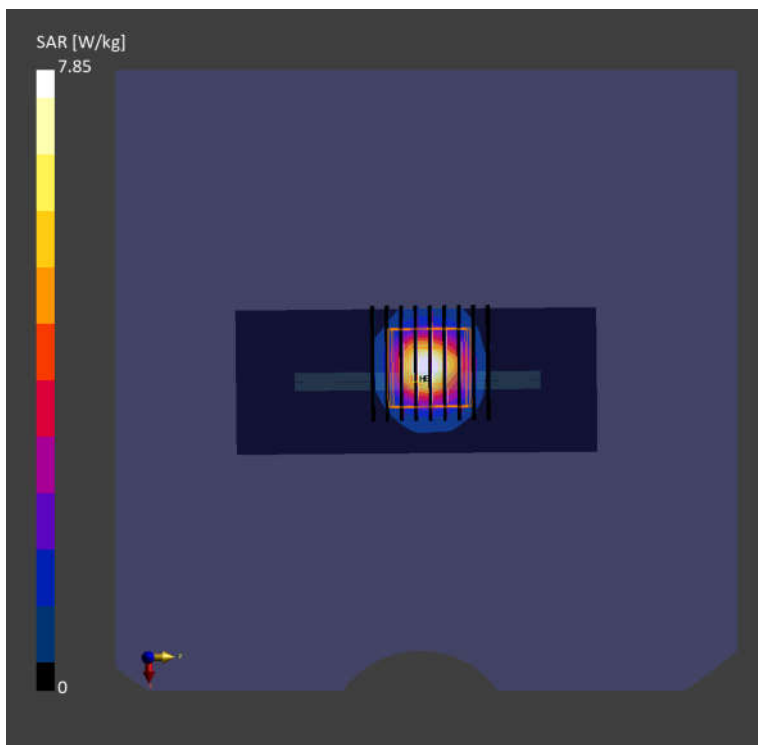

Date: 2026-02-20

System Check_5600MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.88$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.11 W/kg; SAR (10g) = 2.44 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 8.28 W/kg; SAR (10g) = 2.36 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.1 %

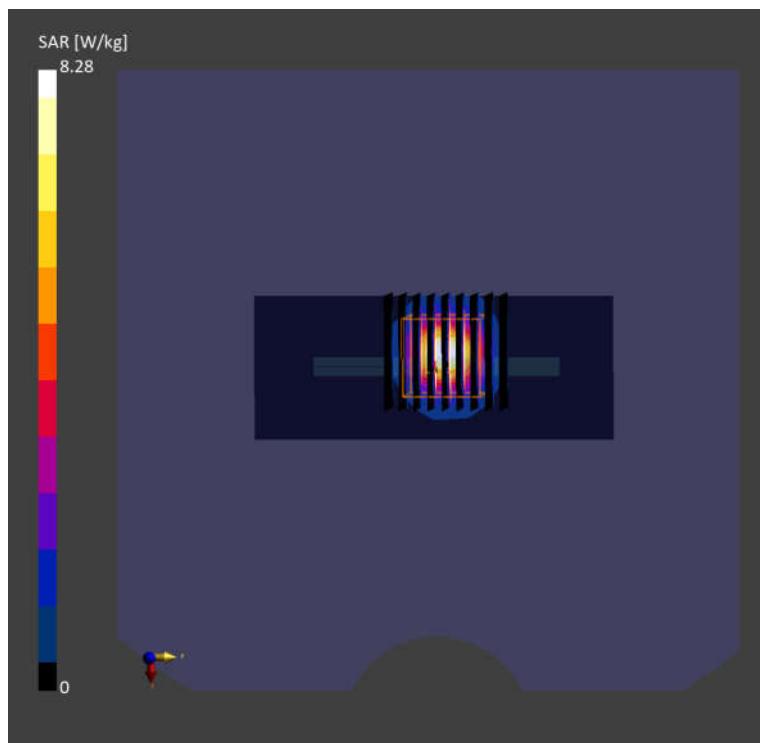

Date: 2026-02-22

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.18$ S/m; $\epsilon_r = 34.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.22, 5.02, 5.01); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.82 W/kg; SAR (10g) = 2.35 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 7.75 W/kg; SAR (10g) = 2.24 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 58.4 %

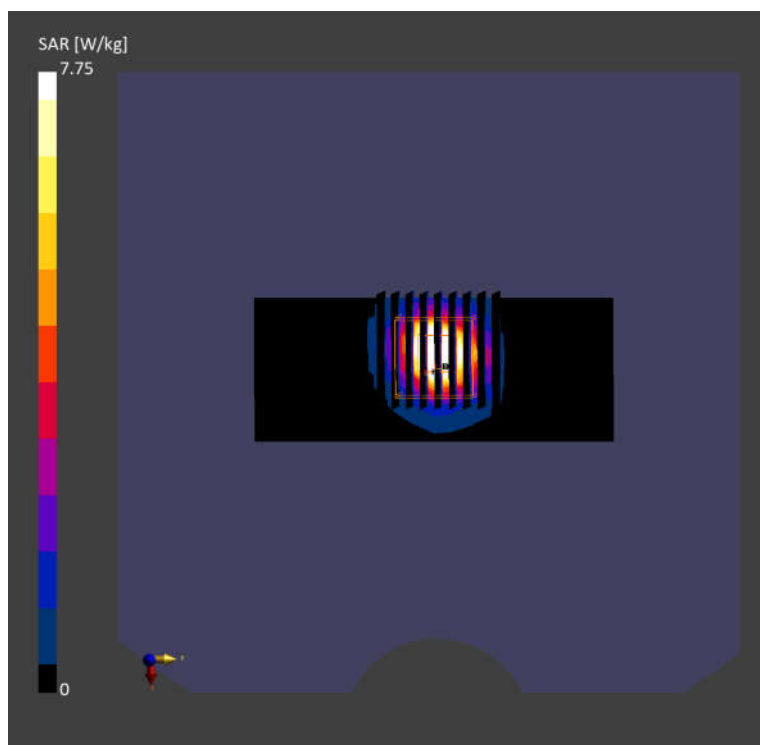

Date: 2026-02-24

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.11$ S/m; $\epsilon_r = 34.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.22, 5.02, 5.01); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.12 W/kg; SAR (10g) = 2.38 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.07 dB

SAR (1g) = 8.08 W/kg; SAR (10g) = 2.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 58.4 %

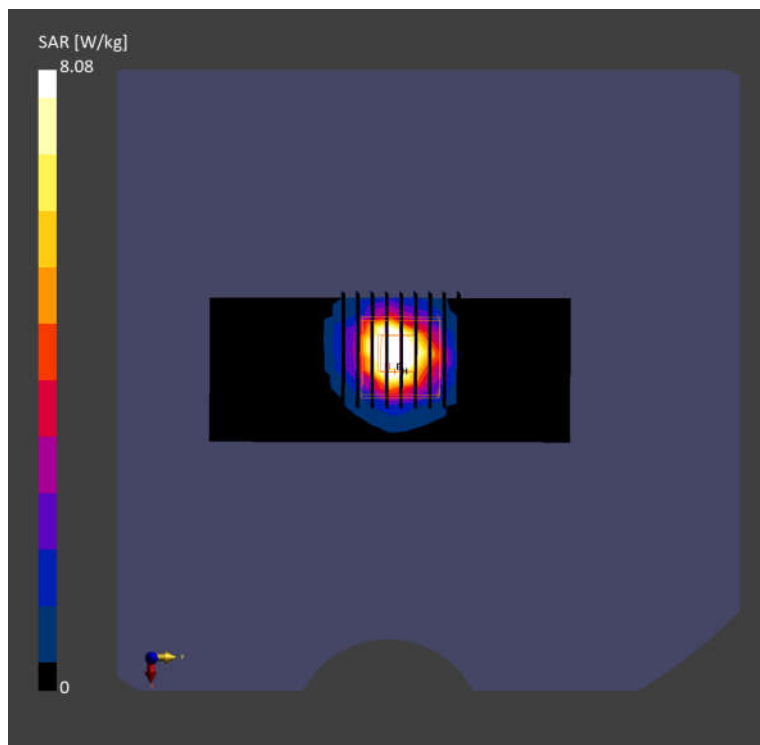

Date: 2026-02-21

System Check_2450MHz**DUT:D2450V2-SN:929**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.77$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.1 W/kg; SAR (10g) = 6.11 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.07 dB

SAR (1g) = 13.2 W/kg; SAR (10g) = 6.11 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

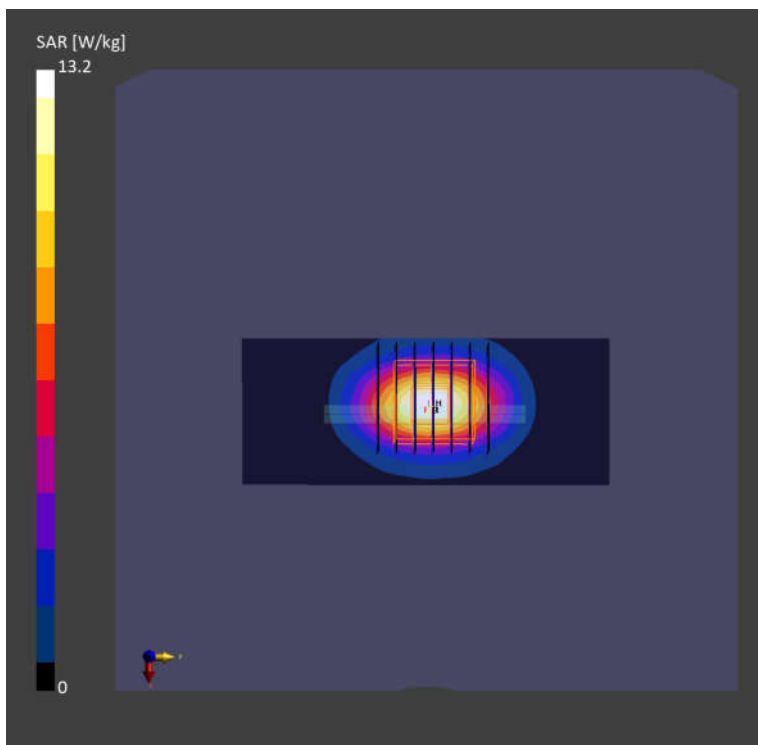

Date: 2026-02-26

System Check_2450MHz**DUT:D2450V2-SN:929**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.79$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
 SAR (1g) = 13.0 W/kg; SAR (10g) = 6.14 W/kg;


Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 13.0 W/kg; SAR (10g) = 6.08 W/kg

Smallest distance from peaks to all points 3 dB below = 8.8 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

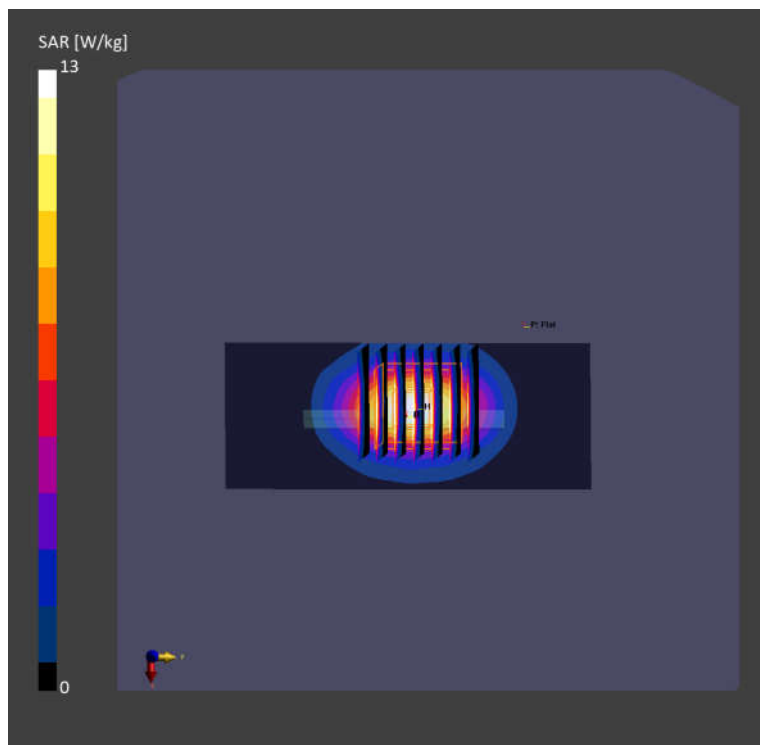

Date: 2026-02-18

System Check_5250MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.59$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.08, 5.97, 6.00); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.84 W/kg; SAR (10g) = 2.29 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 8.24 W/kg; SAR (10g) = 2.33 W/kg

Smallest distance from peaks to all points 3 dB below = 7.1 mm

Ratio of SAR at M2 to SAR at M1 = 67.6 %

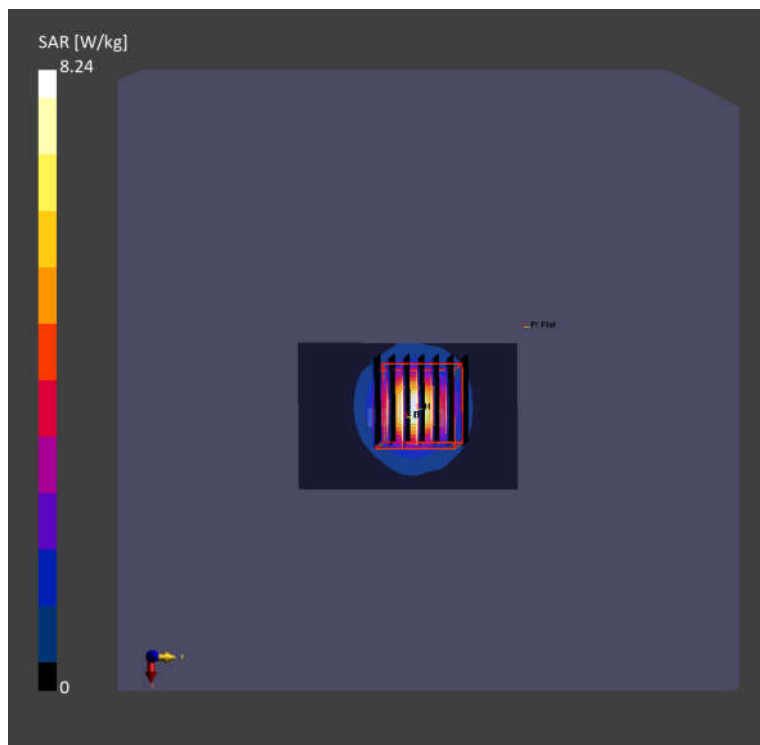

Date: 2026-02-20

System Check_5250MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.54$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.08, 5.97, 6.00); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.81 W/kg; SAR (10g) = 2.29 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 8.17 W/kg; SAR (10g) = 2.25 W/kg

Smallest distance from peaks to all points 3 dB below = 7.5 mm

Ratio of SAR at M2 to SAR at M1 = 67.2 %

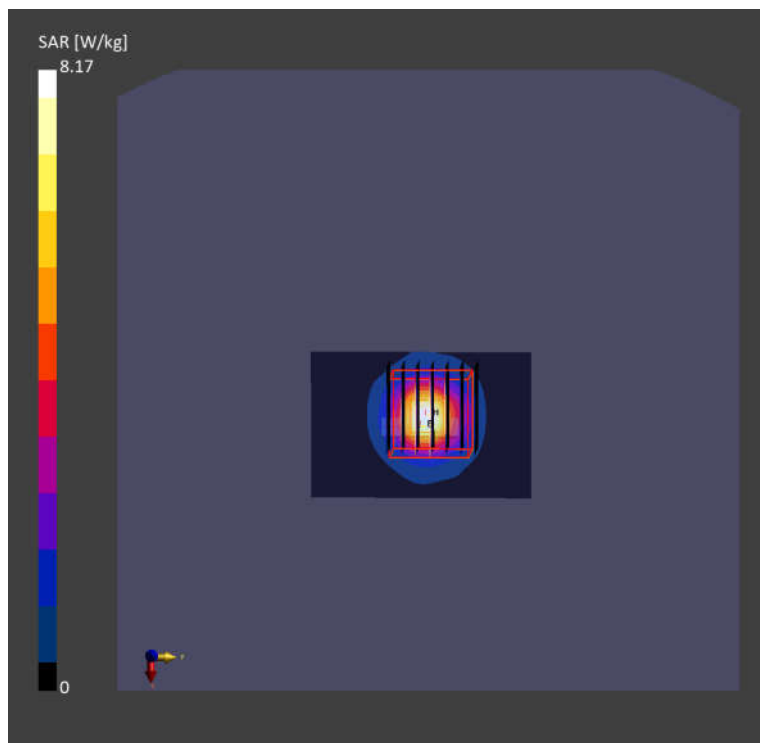

Date: 2026-02-19

System Check_5600MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.96$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.54, 5.44, 5.47); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.47 W/kg; SAR (10g) = 2.46 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.05 dB

SAR (1g) = 8.41 W/kg; SAR (10g) = 2.43 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.9 %

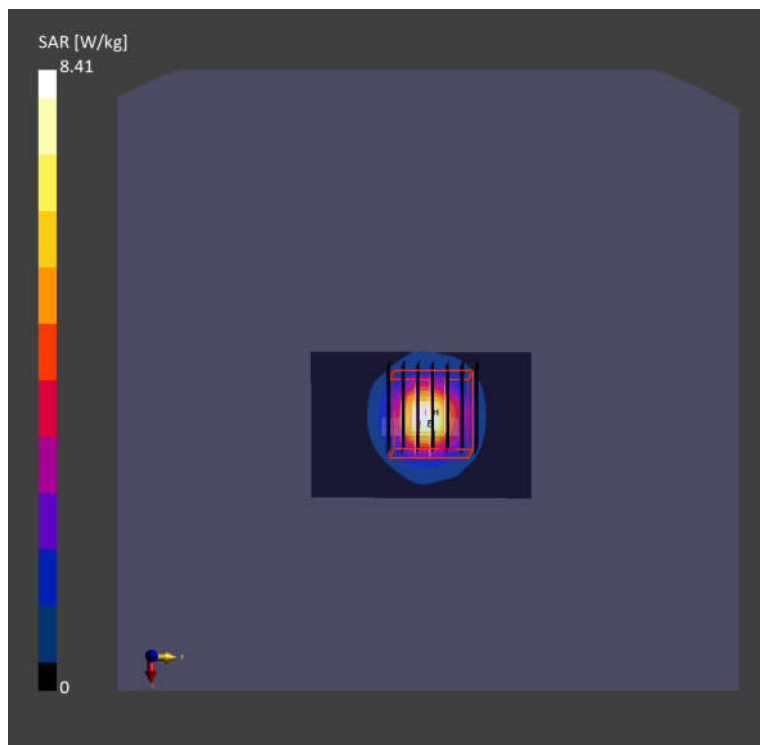

Date: 2026-02-23

System Check_5600MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.92$ S/m; $\epsilon_r = 36.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.54, 5.44, 5.47); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.47 W/kg; SAR (10g) = 2.44 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 8.25 W/kg; SAR (10g) = 2.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.8 mm

Ratio of SAR at M2 to SAR at M1 = 64.8 %

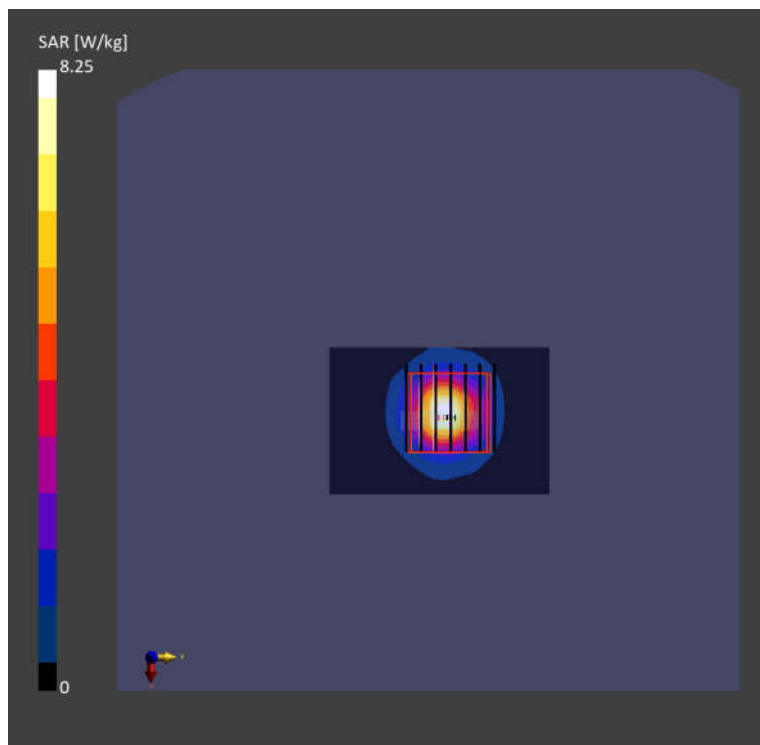

Date: 2026-02-21

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.17$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.52, 5.42, 5.44); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=100 mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
 SAR (1g) = 7.88 W/kg; SAR (10g) = 2.26 W/kg;


Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.07 dB

SAR (1g) = 8.18 W/kg; SAR (10g) = 2.30 W/kg

Smallest distance from peaks to all points 3 dB below = 7.5 mm

Ratio of SAR at M2 to SAR at M1 = 63.1 %

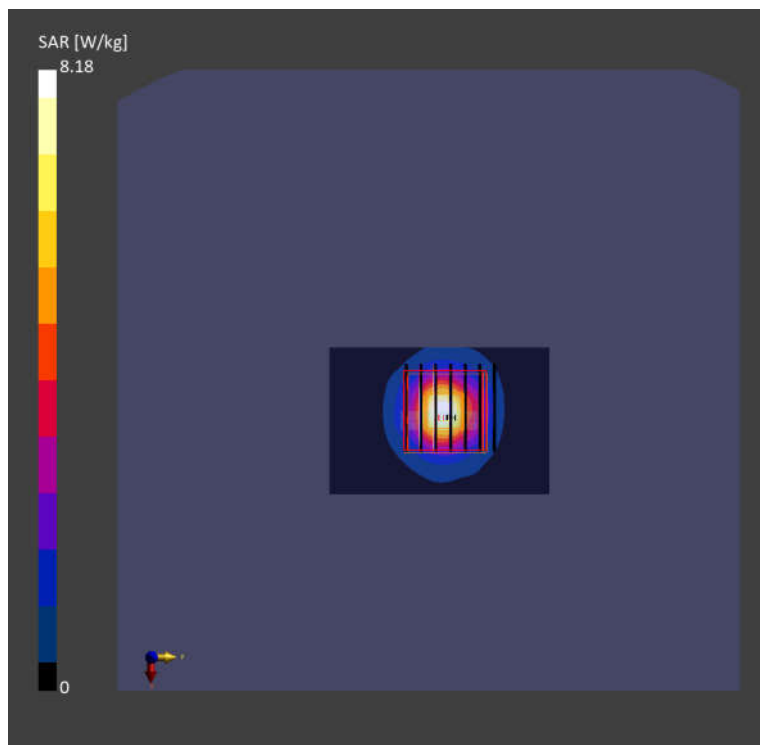

Date: 2026-02-25

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.15$ S/m; $\epsilon_r = 36.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.52, 5.42, 5.44); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=100 mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
 SAR (1g) = 7.86 W/kg; SAR (10g) = 2.28 W/kg;


Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.11 dB

SAR (1g) = 8.11 W/kg; SAR (10g) = 2.23 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 63.5 %

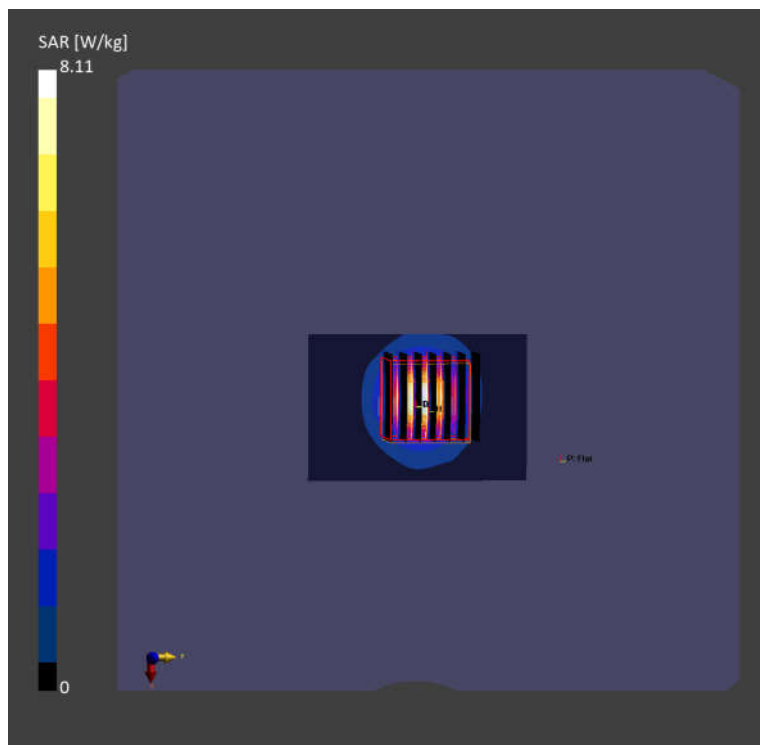

System Check_2450MHz**DUT:D2450V2-SN:929**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.80	38.9

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 - 1024	HBBL-600-10000 ,	EX3DV4 - SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-14	2026-02-14
psSAR1g [W/Kg]	13.4	13.9
psSAR10g [W/Kg]	6.21	6.32
Power Drift [dB]	-0.08	-0.11

SAR Pattern

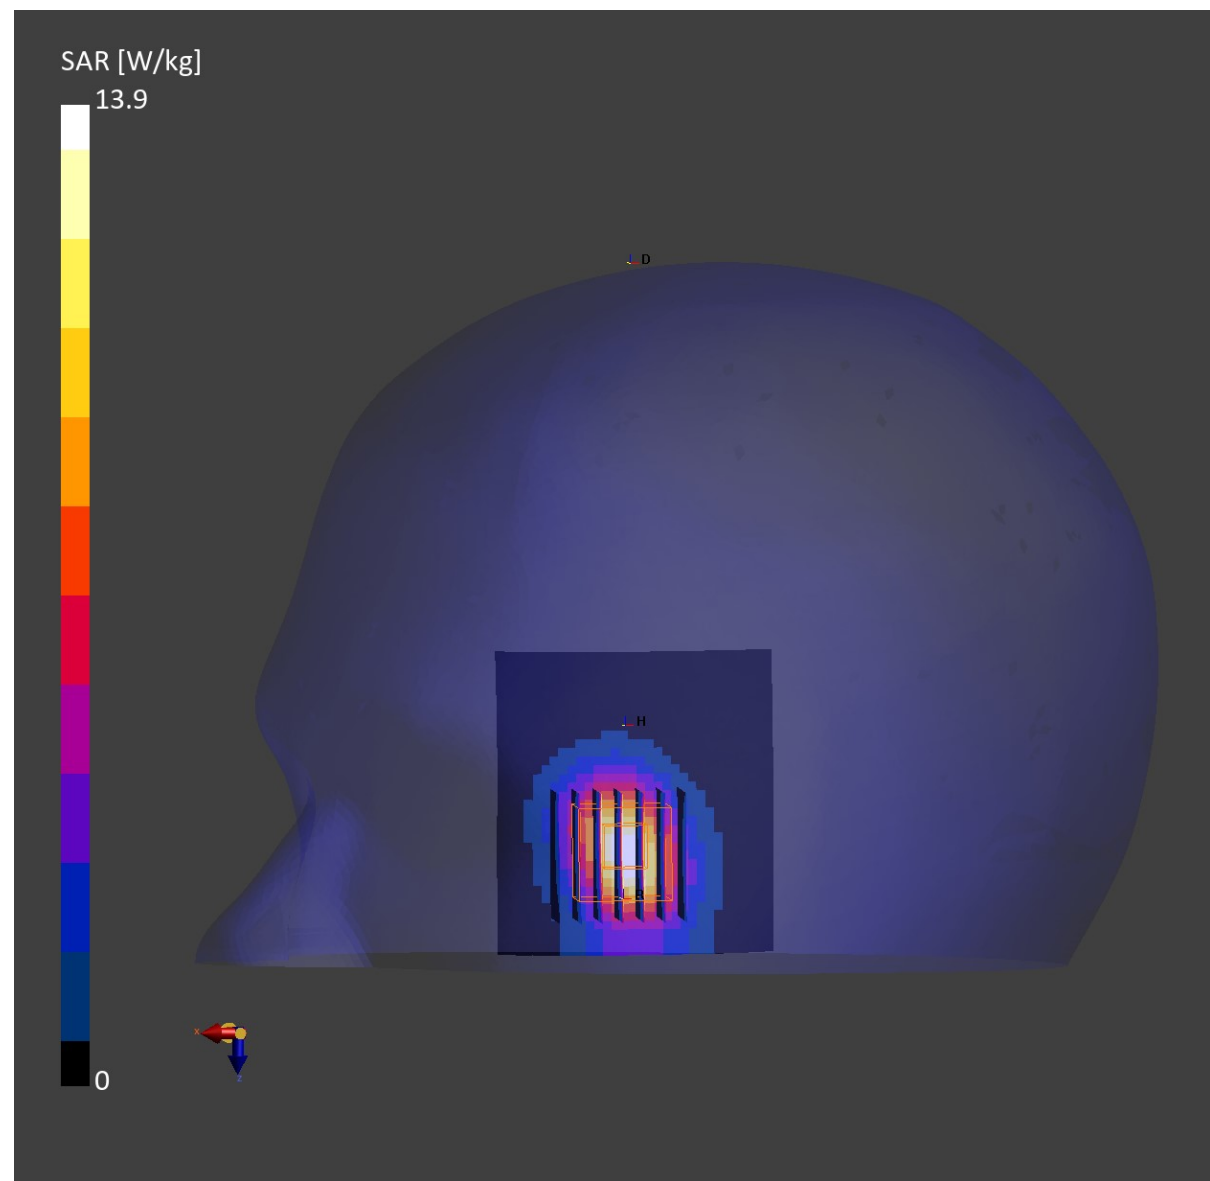

System Check_2450MHz**DUT:D2450V2-SN:929**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.85	40.0

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-18	2026-02-18
psSAR1g [W/Kg]	12.4	12.7
psSAR10g [W/Kg]	6.01	6.07
Power Drift [dB]	0.05	-0.04

SAR Pattern

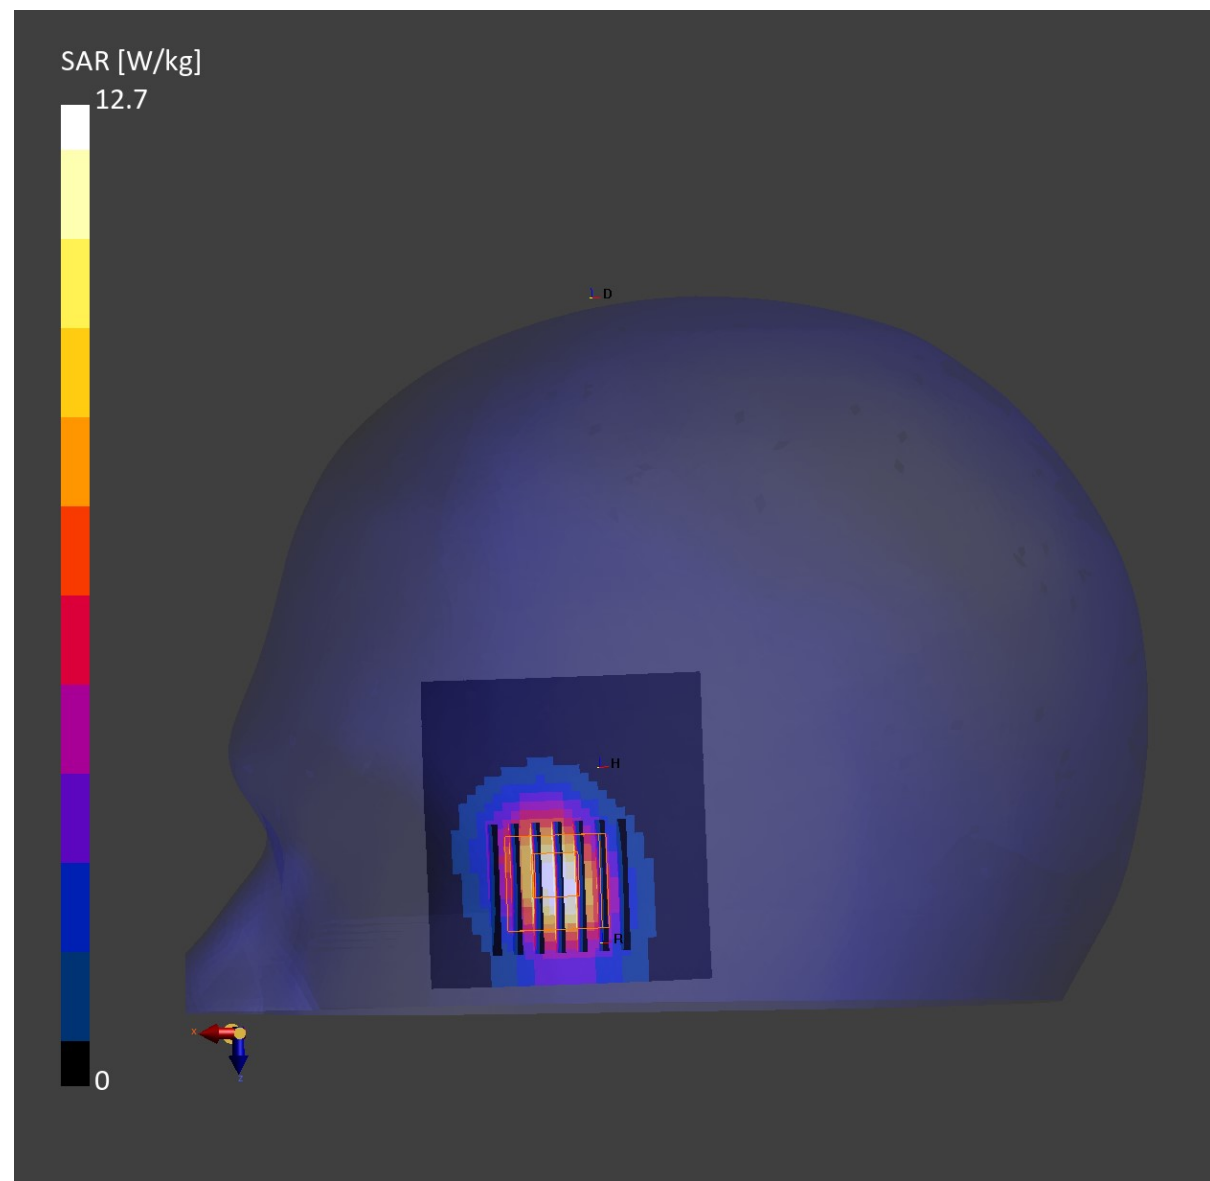

System Check_2450MHz**DUT:D2450V2-SN:929**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.83	39.8

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-19	2026-02-19
psSAR1g [W/Kg]	13.1	13.4
psSAR10g [W/Kg]	6.11	6.19
Power Drift [dB]	-0.08	-0.02

SAR Pattern

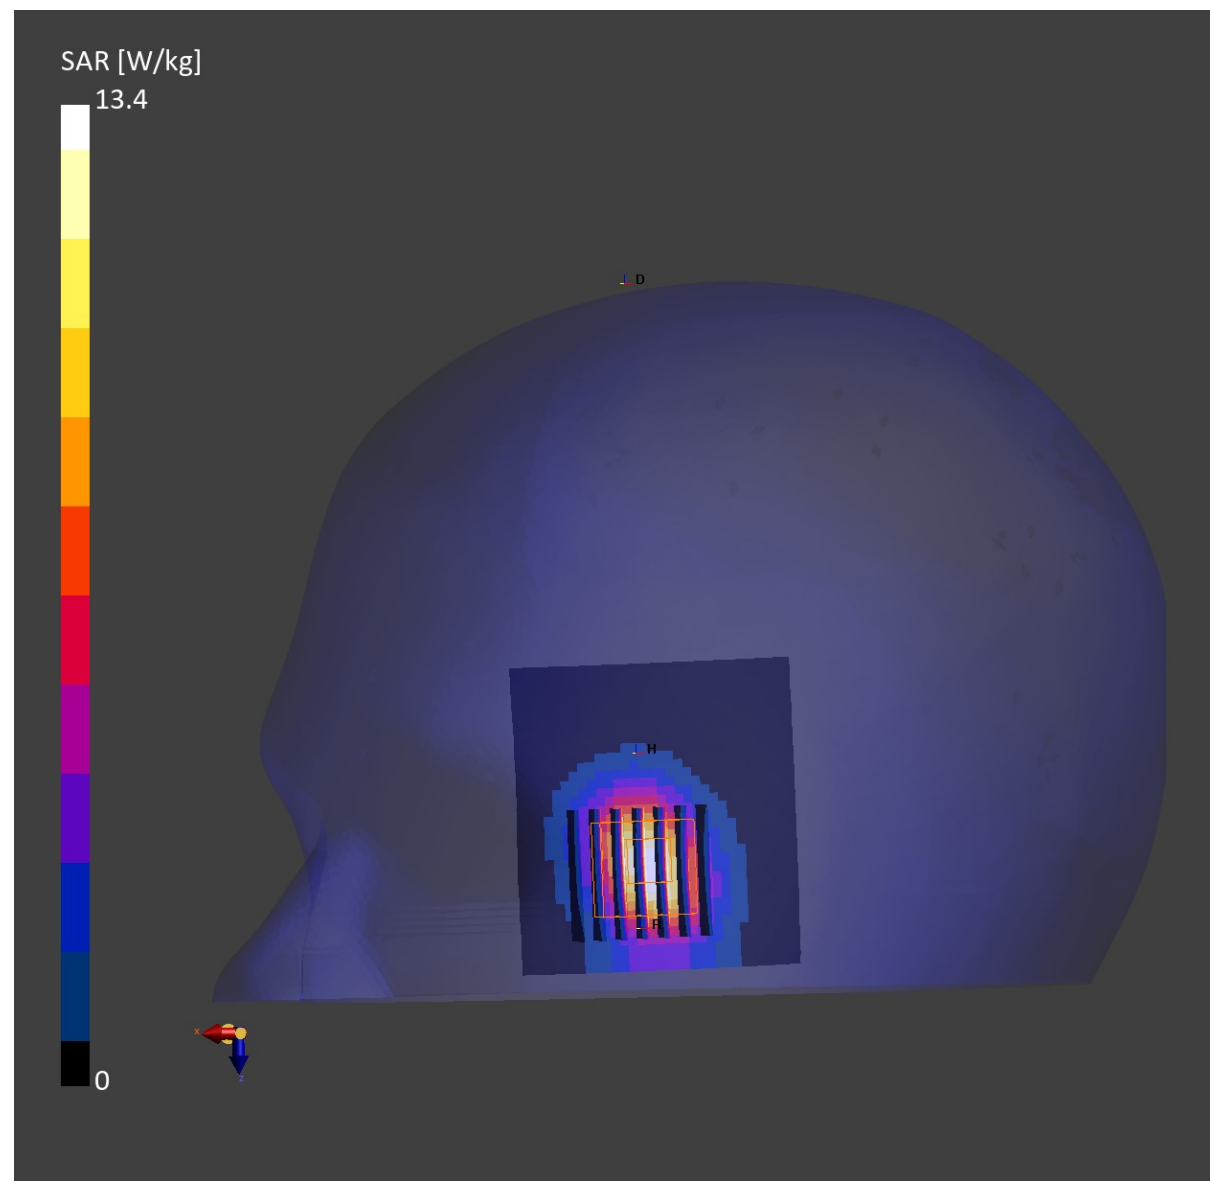

System Check_2450MHz**DUT:D2450V2-SN:929**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.78	40.0

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28

Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-25	2026-02-25
psSAR1g [W/Kg]	13.3	13.6
psSAR10g [W/Kg]	6.06	6.22
Power Drift [dB]	0.07	-0.09

SAR Pattern

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.22	35.2

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-15	2026-02-15
psSAR1g [W/Kg]	1.78	1.84
psSAR10g [W/Kg]	0.629	0.645
Power Drift [dB]	-0.05	-0.11

SAR Pattern

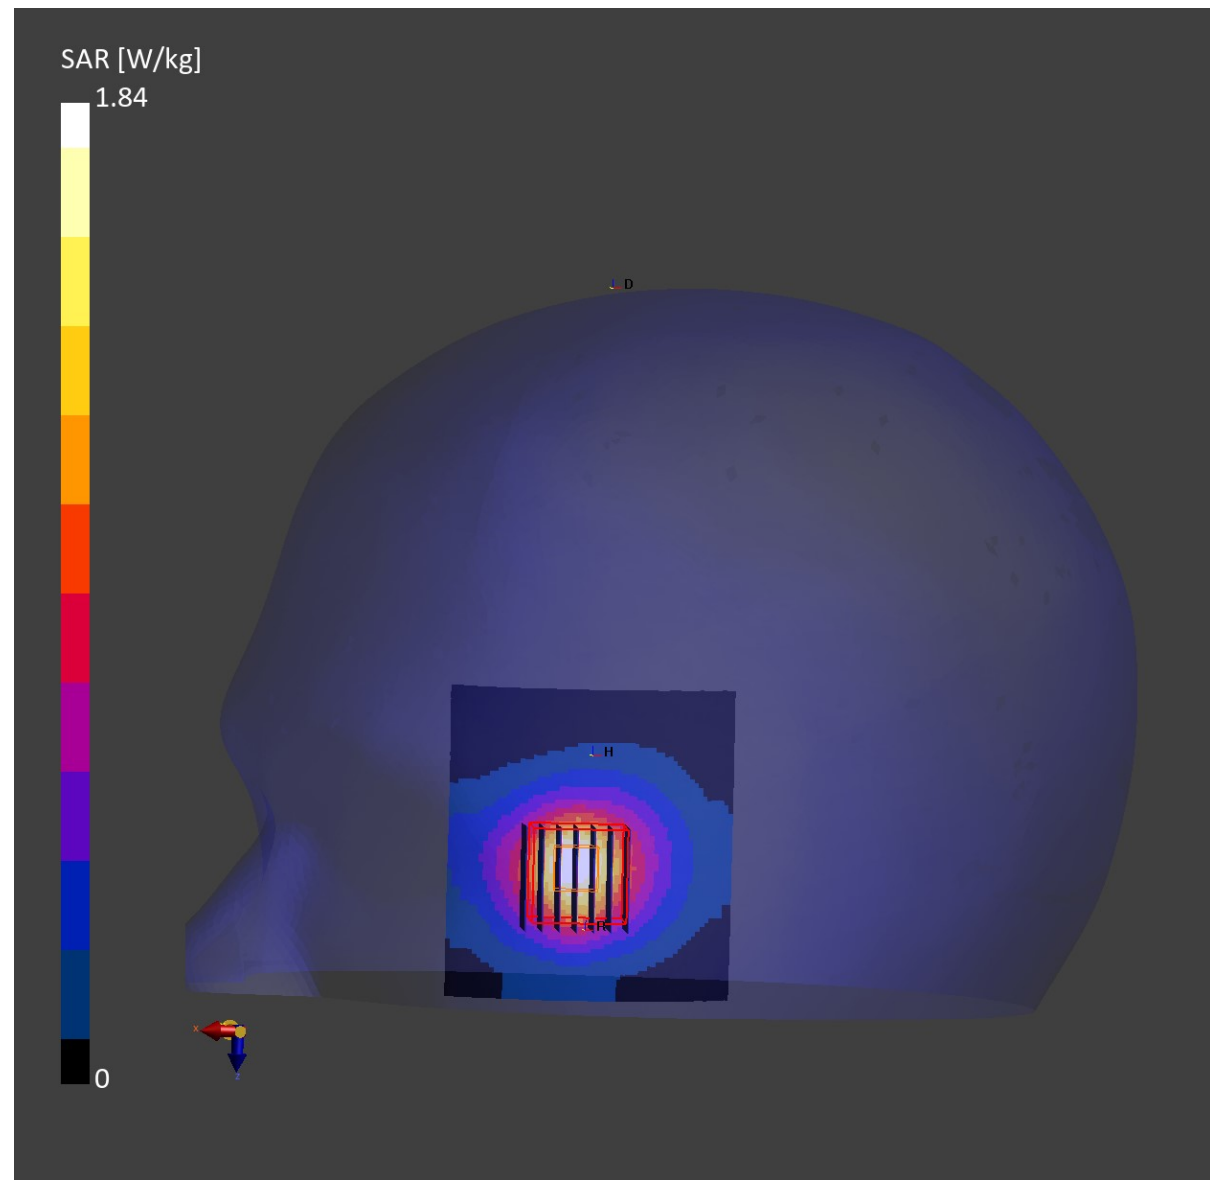

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.13	35.1

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-16	2026-02-16
psSAR1g [W/Kg]	1.72	1.76
psSAR10g [W/Kg]	0.615	0.626
Power Drift [dB]	-0.07	-0.05

SAR Pattern

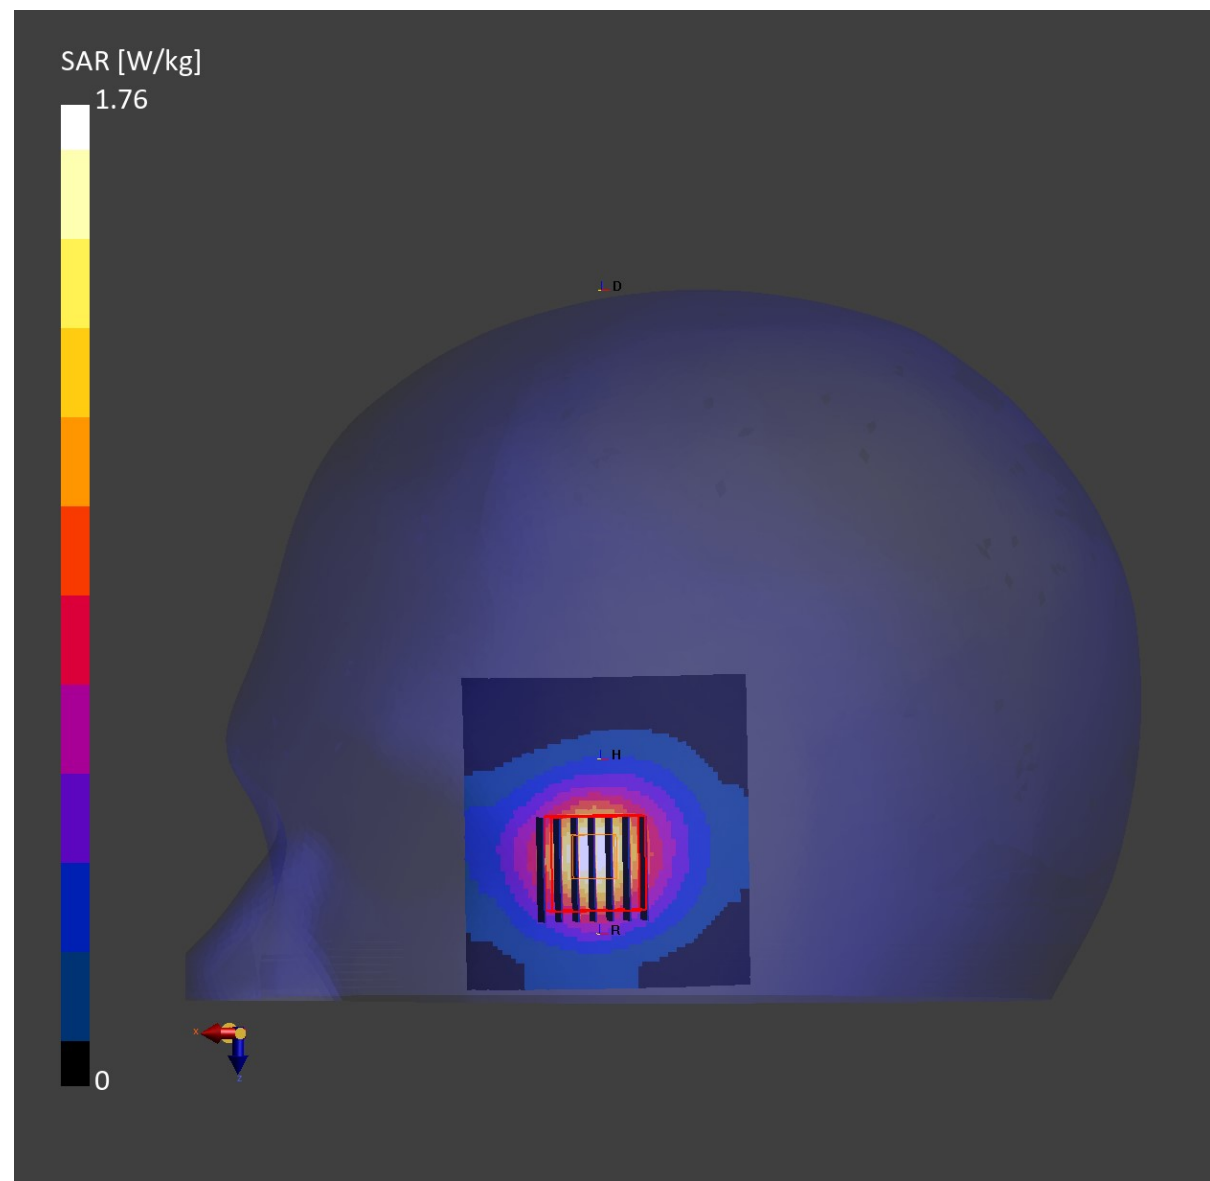

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.20	36.8

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-18	2026-02-18
psSAR1g [W/Kg]	1.58	1.69
psSAR10g [W/Kg]	0.599	0.607
Power Drift [dB]	-0.04	0.07

SAR Pattern

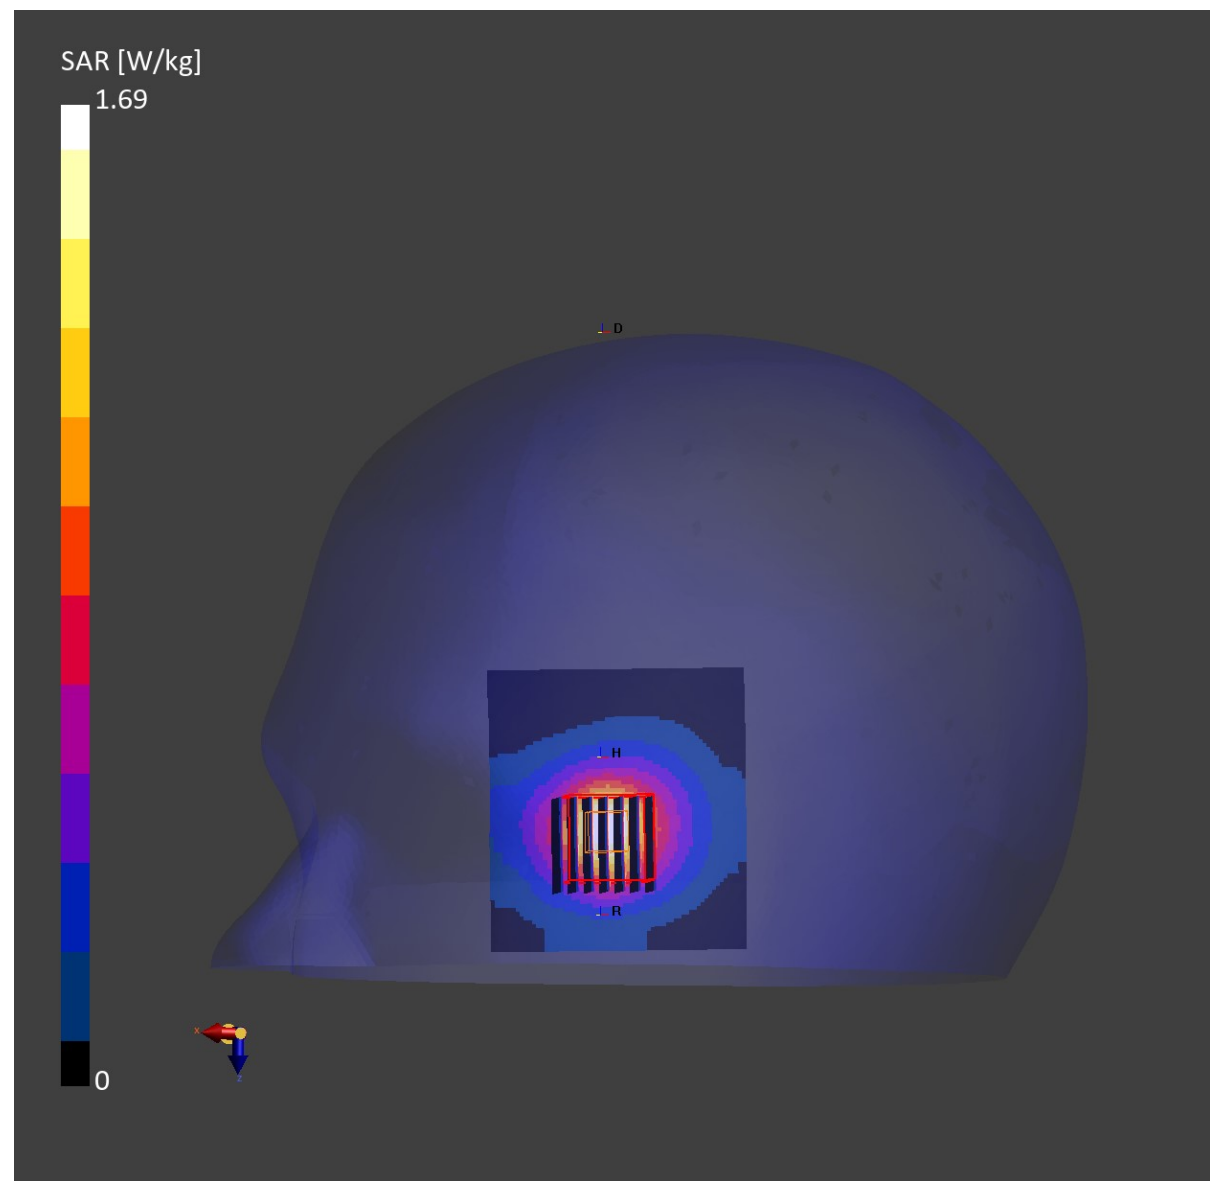

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.12	34.9

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28

Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-02-21	2026-02-21
psSAR1g [W/Kg]	1.72	1.73
psSAR10g [W/Kg]	0.609	0.618
Power Drift [dB]	-0.01	-0.04

SAR Pattern

