



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D750V3-1117\_Mar25**

## CALIBRATION CERTIFICATE

Object

**D750V3 - SN: 1117**

Calibration procedure(s)

**QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date

**March 12, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)            | Scheduled Cal |
|--------------------------------------------|------------|---------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)             | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 06-Feb-25 (No. 4030A315009541)        | Feb-26        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 29-Jan-25 (No. 4030A315009658)        | Jan-26        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)             | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sep-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sep-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)        | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)     | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|                                                                                                                 |                  |                       |                        |
|-----------------------------------------------------------------------------------------------------------------|------------------|-----------------------|------------------------|
|                                                                                                                 | Name             | Function              | Signature              |
| Calibrated by                                                                                                   | Krešimir Franjić | Laboratory Technician |                        |
| Approved by                                                                                                     | Sven Kühn        | Technical Manager     |                        |
|                                                                                                                 |                  |                       | Issued: March 12, 2025 |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |                  |                       |                        |



Accredited by the Swiss Accreditation Service (SAS)  
**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 15 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 6mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 750MHz $\pm$ 1MHz        |                                     |

## HSL parameters at 750 MHz

The following parameters and calculations were applied.

|                                    | Temperature        | Permittivity  | Conductivity         |
|------------------------------------|--------------------|---------------|----------------------|
| Nominal HSL parameters             | 22.0 °C            | 41.9          | 0.890 mho/m          |
| Measured HSL parameters            | (22.0 $\pm$ 0.2)°C | 42.7 $\pm$ 6% | 0.890 mho/m $\pm$ 6% |
| HSL temperature change during test | < 0.5 °C           |               |                      |

## SAR result with HSL at 750 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of HSL | Condition          |                               |
|--------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                   | 24 dBm input power | 2.16 W/kg                     |
| SAR for nominal HSL parameters                   | normalized to 1W   | 8.60 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of HSL | Condition          |                               |
|----------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                     | 24 dBm input power | 1.40 W/kg                     |
| SAR for nominal HSL parameters                     | normalized to 1W   | 5.57 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with HSL at 750 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 52.2 $\Omega$ – 3.3 j $\Omega$ |
| Return Loss | -28.2 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.035 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole          | Frequency [MHz] | TSL | Power [dBm] |
|-----------------|-----------------|-----|-------------|
| D750V3 - SN1117 | 750             | HSL | -24         |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 15                 |      | CW, 0---   | 750, 0                          | 9.55              | 0.89                   | 42.7             |

Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|---------------|--------------------|-----------------------------|---------------------------|
| Flat V4.9 mod | HSL, 2025-03-12    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip-Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 6.0 x 6.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS = 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-03-12          |
| psSAR1g [W/Kg]      | 2.16                |
| psSAR10g [W/Kg]     | 1.40                |
| Power Drift [dB]    | -0.04               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

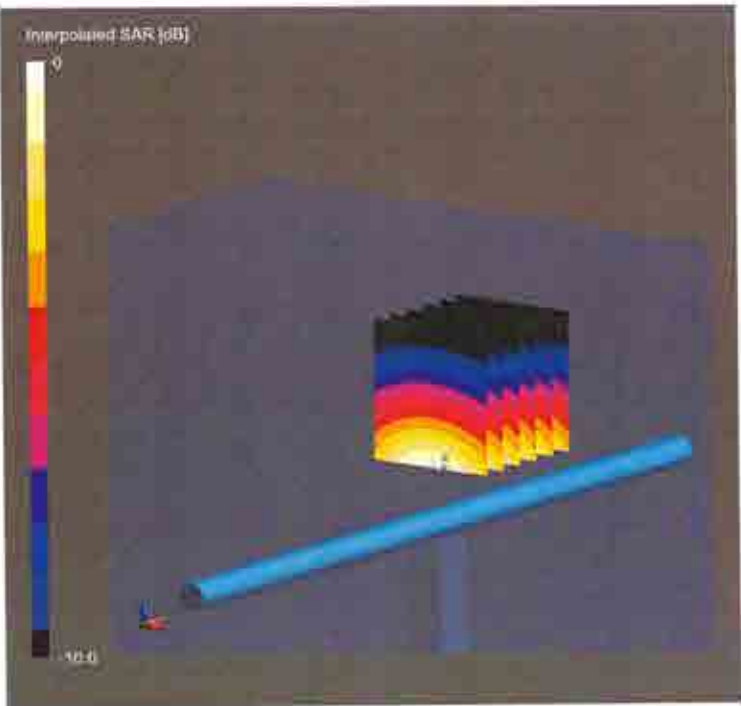

0 dB = 3.31 W/Kg

Impedance Measurement Plot for HSL

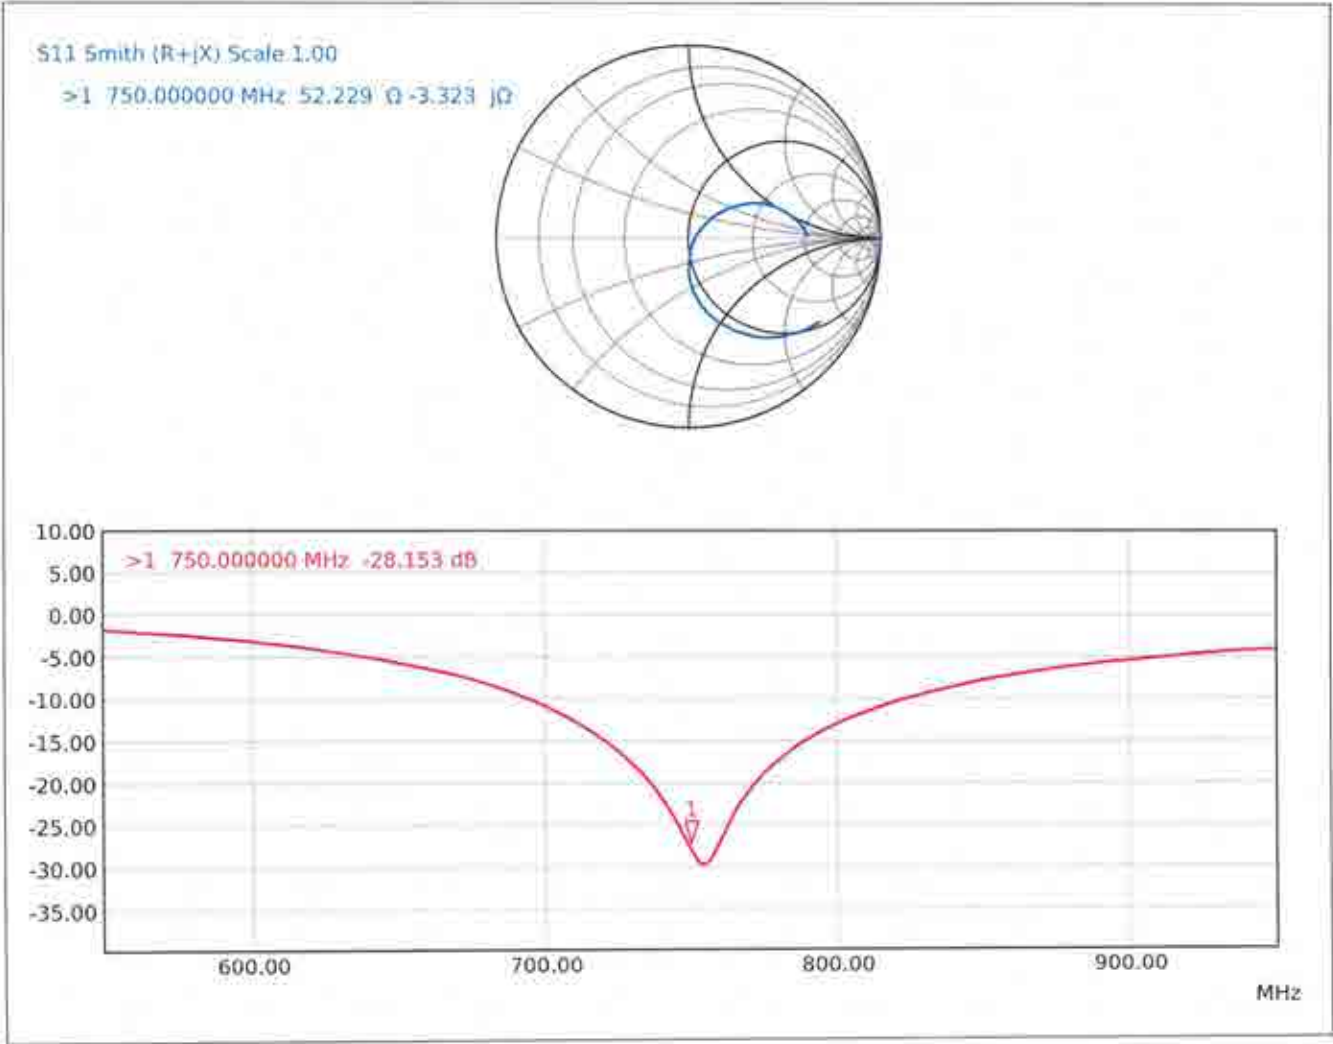



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D750V3-1107\_Jun25**

## CALIBRATION CERTIFICATE

Object **D750V3 - SN: 1107**

Calibration procedure(s) **QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date **June 11, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|-----------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T    | SN: 100967 | 26-Mar-25 (No. 217-04290)              | Mar-26        |
| Power Sensor R&S NRP18A     | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40 | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| 3.5mm mismatch combination  | SN: 1152   | 24-Mar-25 (No. 217-04293)              | Mar-26        |
| OCP DAK-12                  | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                 | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4lp                      | SN: 1836   | 17-Apr-25 (No. DAE4lp-1836_Apr25)      | Apr-26        |

| Secondary Standards          | ID         | Check Date (In house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Setup 1                 | SN: 1000   | 27-May-25 (No. 675-ACAD_Source_Box-250527) | May-26          |
| Signal Generator R&S SMB100A | SN: 182081 | 27-May-25 (No. 675-CAL16-S4588-250527)     | May-26          |
| Mismatch; SMA                | SN: 1102   | 24-Apr-25 (No. 675-Mismatch_SMA-250424)    | Apr-26          |
| OCP DAK-12                   | SN: 1029   | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)       | Feb-26          |
| OCP DAK-3.5                  | SN: 1336   | 09-Dec-24 (No. OCP-DAK3.5-1336_Dec24)      | Dec-25          |

|               |            |                       |           |
|---------------|------------|-----------------------|-----------|
|               | Name       | Function              | Signature |
| Calibrated by | Paulo Pina | Laboratory Technician |           |
| Approved by   | Sven Kühn  | Technical Manager     |           |

Issued: June 11, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 15 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 6mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 750MHz $\pm$ 1MHz        |                                     |

## HSL parameters at 750 MHz

The following parameters and calculations were applied.

|                                    | Temperature         | Permittivity  | Conductivity         |
|------------------------------------|---------------------|---------------|----------------------|
| Nominal HSL parameters             | 22.0 °C             | 41.9          | 0.890 mho/m          |
| Measured HSL parameters            | (22.0 $\pm$ 0.2) °C | 43.0 $\pm$ 6% | 0.910 mho/m $\pm$ 6% |
| HSL temperature change during test | < 0.5 °C            |               |                      |

## SAR result with HSL at 750 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of HSL | Condition          |                               |
|--------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                   | 24 dBm input power | 2.22 W/kg                     |
| SAR for nominal HSL parameters                   | normalized to 1W   | 8.84 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of HSL | Condition          |                               |
|----------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                     | 24 dBm input power | 1.46 W/kg                     |
| SAR for nominal HSL parameters                     | normalized to 1W   | 5.81 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 750 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 52.8 $\Omega$ – 3.0 j $\Omega$ |
| Return Loss | -28.0 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.031 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole          | Frequency [MHz] | TSL | Power [dBm] |
|-----------------|-----------------|-----|-------------|
| D750V3 - SN1107 | 750             | HSL | 24          |

Exposure Conditions

| Phantom Section: TSL | Test Distance [mm] | Band    | Group: UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 15                 | CW, 0-- |            | 750, 0                          | 9.55              | 0.91                   | 43.0             |

Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|---------------|--------------------|-----------------------------|---------------------------|
| Flat V4.9 mod | HSL, 2025-06-11    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2025-04-17 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 6.0 x 6.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-06-11          |
| psSAR1g [W/Kg]      | 2.22                |
| psSAR10g [W/Kg]     | 1.46                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

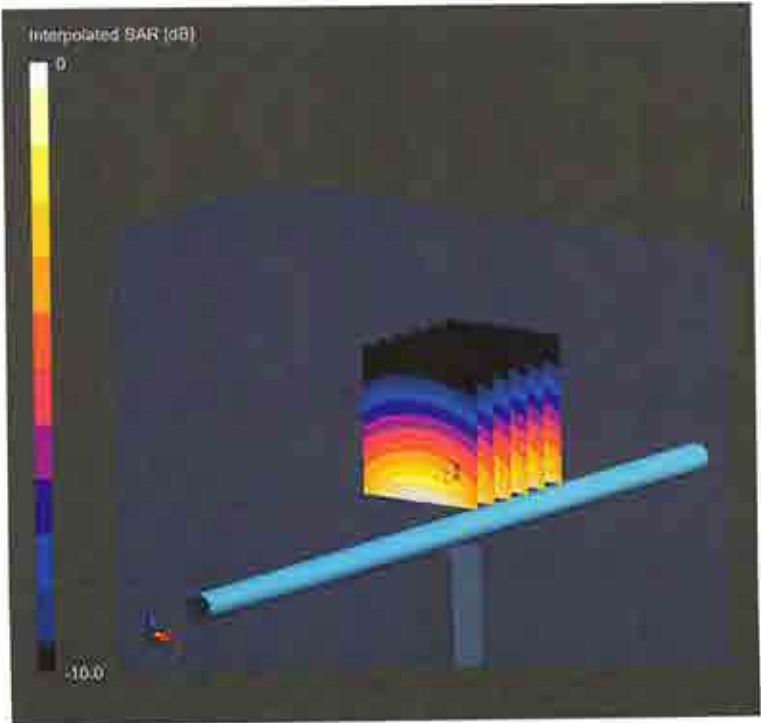

0 dB = 3.38 W/Kg

Impedance Measurement Plot for HSL

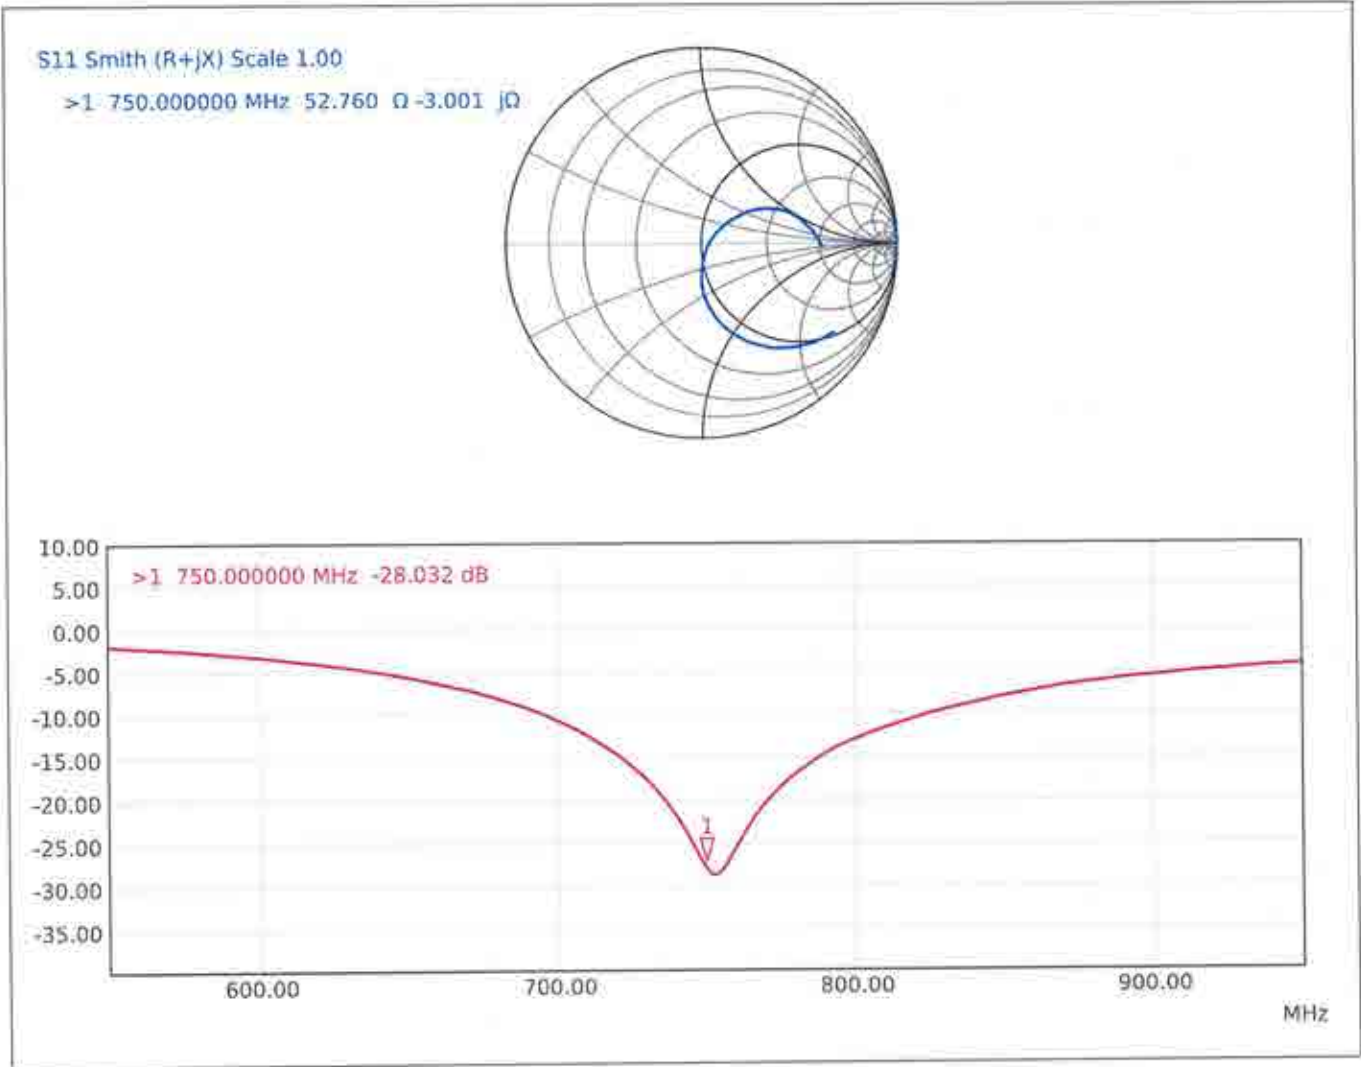

**Calibration Laboratory of****Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland

**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**Accreditation No.: **SCS 0108**

Client

**Sporton**

Taoyuan City

Certificate No.

**D835V2-4d060\_Feb25****CALIBRATION CERTIFICATE**Object **D835V2 - SN: 4d060**Calibration procedure(s) **QA CAL-05.v12  
Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**Calibration date **February 17, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (In house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|                                                                                                                 | Name         | Function              | Signature                 |
|-----------------------------------------------------------------------------------------------------------------|--------------|-----------------------|---------------------------|
| Calibrated by                                                                                                   | Leif Klysner | Laboratory Technician |                           |
| Approved by                                                                                                     | Sven Kühn    | Technical Manager     |                           |
|                                                                                                                 |              |                       | Issued: February 18, 2025 |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |              |                       |                           |

## Calibration Laboratory of

Schmid & Partner  
Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 15 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 6mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 835MHz $\pm$ 1MHz        |                                     |

## Head TSL parameters at 835 MHz

The following parameters and calculations were applied.

|                                         | Temperature        | Permittivity  | Conductivity         |
|-----------------------------------------|--------------------|---------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C            | 41.5          | 0.900 mho/m          |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2)°C | 41.4 $\pm$ 6% | 0.900 mho/m $\pm$ 6% |
| Head TSL temperature change during test | < 0.5 °C           |               |                      |

## SAR result with Head TSL at 835 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                               |
|-------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                   | 24 dBm input power | 2.33 W/kg                     |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 9.28 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                               |
|---------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                     | 24 dBm input power | 1.51 W/kg                     |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 6.01 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 835 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 52.3 $\Omega$ – 2.6 j $\Omega$ |
| Return Loss | -29.4 dB                       |

**General Antenna Parameters and Design**

|                                  |         |
|----------------------------------|---------|
| Electrical Delay (one direction) | 1.39 ns |
|----------------------------------|---------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D835V2 - SN4d060 | 835             | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 15                 |      | CW, 0      | 835, 0                          | -9.51             | 0.90                   | 41.4             |

Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|---------------|--------------------|-----------------------------|---------------------------|
| Flat V4.9 mod | HSL, 2025-02-17    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 6.0 x 6.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS = 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-02-17          |
| psSAR1g [W/Kg]      | 2.33                |
| psSAR10g [W/Kg]     | 1.51                |
| Power Drift [dB]    | 0.01                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

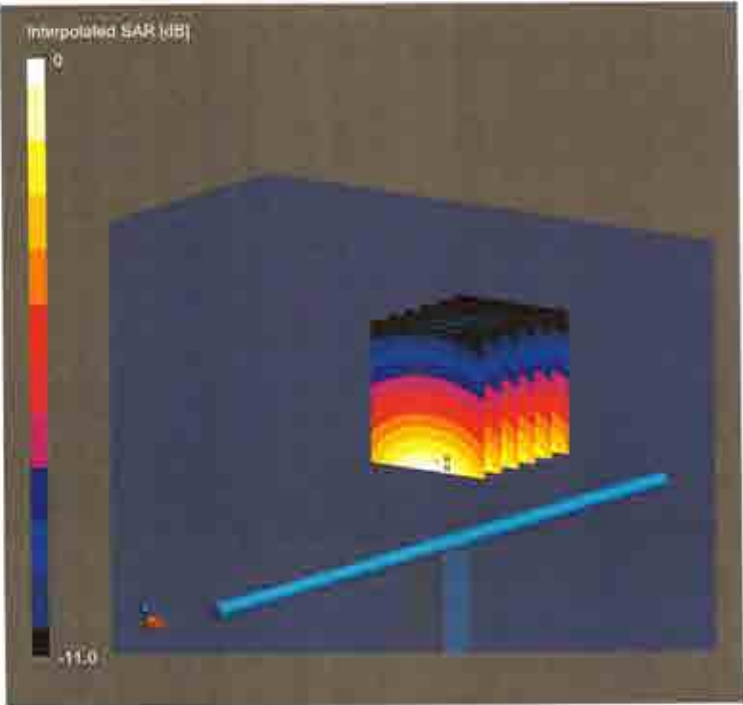

0 dB = 3.60 W/Kg

Impedance Measurement Plot for Head TSL

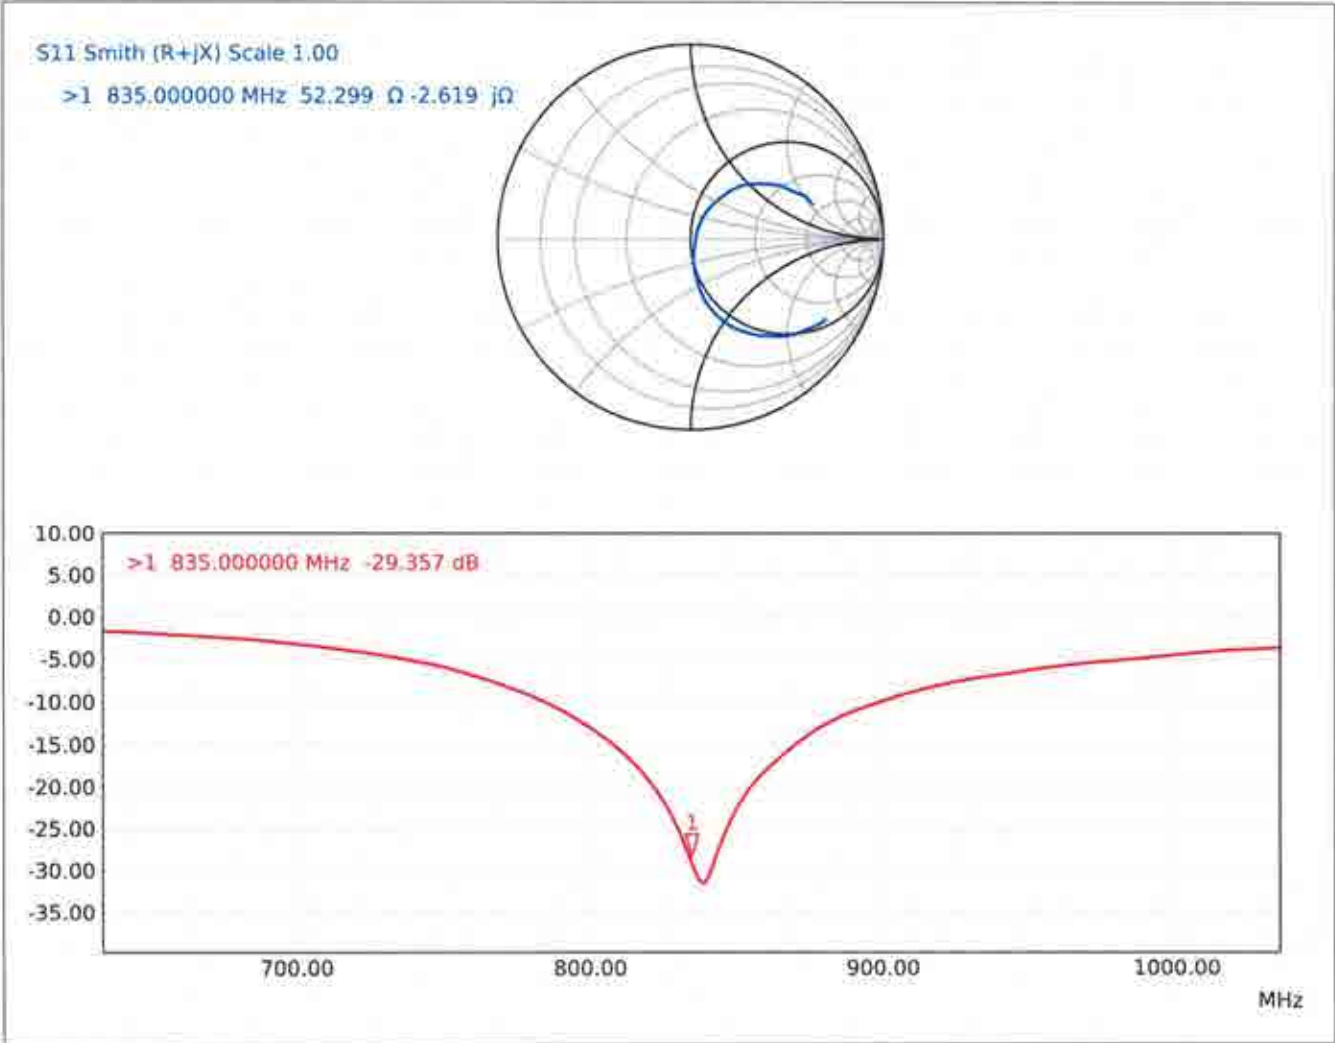

## D835V2, serial no. 4D060 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.


### <Justification of the extended calibration>

| D835V2 – serial no. 4D060   |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
| 835MHZ                      |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 02.17.2025<br>(Cal. Report) | -29.357          |           | 52.299               |             | -2.619                    |             |
| 02.16.2026<br>(extended)    | -28.371          | 3.359     | 51.525               | -0.774      | -1.3591                   | 1.2599      |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D835V2, serial no. 4D060 (Data of Measurement : 02.16.2026)

835 MHz - Head

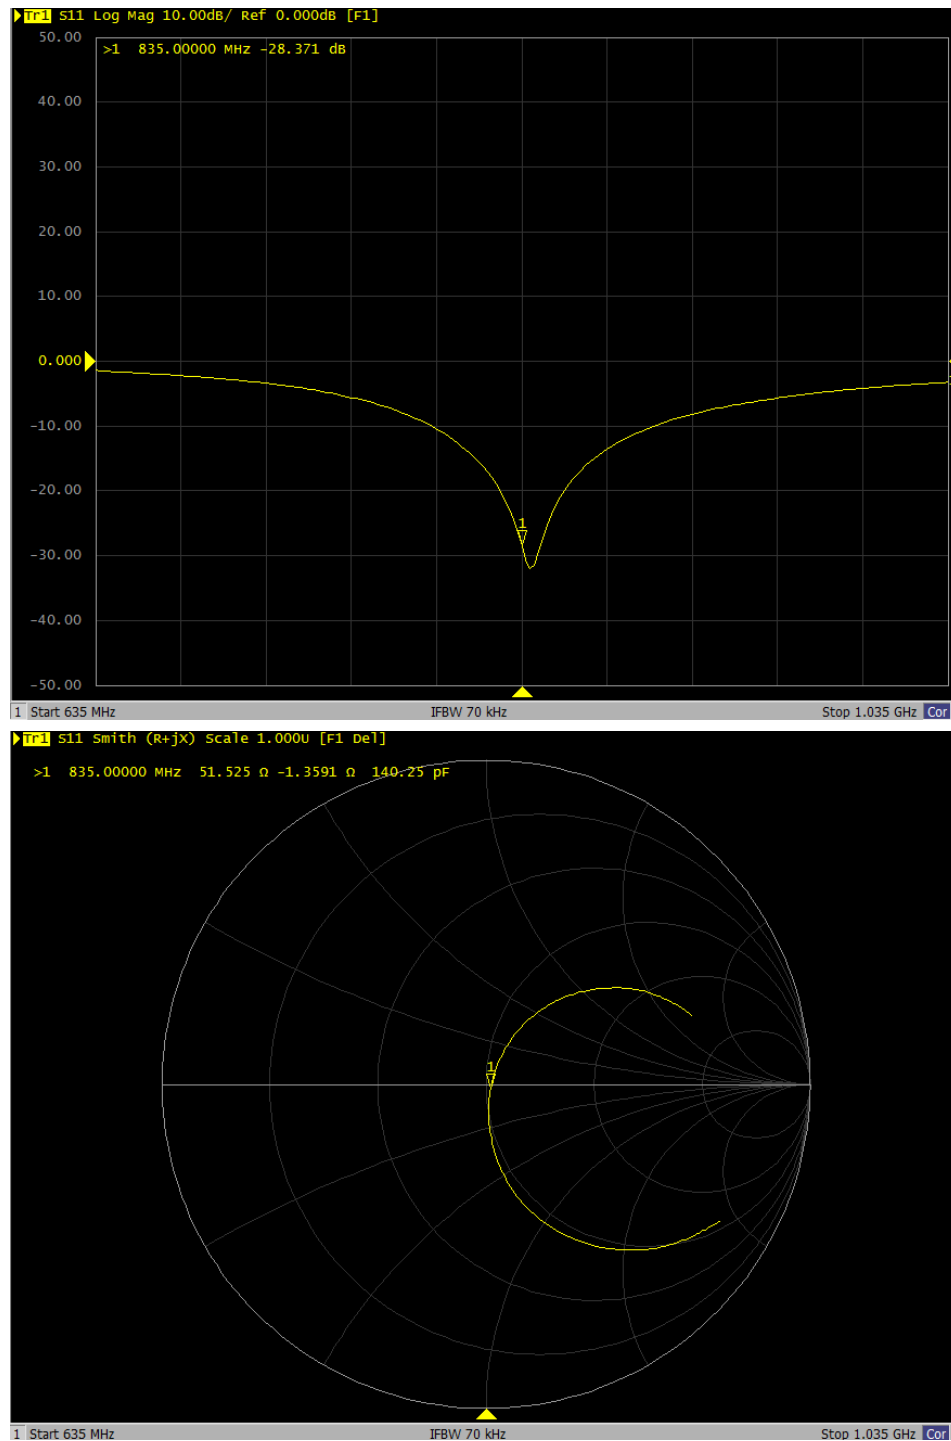



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

Sporton  
Taoyuan City

Certificate No.

D835V2-4d167\_Dec25

## CALIBRATION CERTIFICATE

Object

D835V2 - SN: 4d167

Calibration procedure(s)

QA CAL-05.v13

Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz

Calibration date

December 2, 2025

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|-----------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP40T     | SN: 101861 | 29-Apr-25 (No. 2025-001450)            | Apr-26        |
| Power Sensor R&S NRP18A     | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40 | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| 3.5mm mismatch combination  | SN: 1152   | 24-Mar-25 (No. 217-04293)              | Mar-26        |
| OCP DAK-12                  | SN: 1016   | 16-Sept-25 (No. OCP-DAK12-1016_Sep25)  | Sep-26        |
| OCP DAK-3.5                 | SN: 1249   | 16-Sept-25 (No. OCP-DAK3.5-1249_Sep25) | Sep-26        |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                      | SN: 1836   | 26-Nov-25 (No. DAE4ip-1836_Nov25)      | Nov-26        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Setup 1                 | SN: 1000   | 27-May-25 (No. 675-ACAD_Source_Box-250527) | May-26          |
| Signal Generator R&S SMB100A | SN: 182081 | 27-May-25 (No. 675-CAL16-S4588-250527)     | May-26          |
| Mismatch: SMA                | SN: 1102   | 24-Apr-25 (No. 675-Mismatch_SMA-250424)    | Apr-26          |
| OCP DAK-12                   | SN: 1029   | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)       | Feb-26          |
| OCP DAK-3.5                  | SN: 1336   | 09-Dec-24 (No. OCP-DAK3.5-1336_Dec24)      | Dec-25          |

|                                                                                                                 | Name       | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|------------|-----------------------|-----------|
| Calibrated by                                                                                                   | Paulo Pina | Laboratory Technician |           |
| Approved by                                                                                                     | Sven Kühn  | Technical Manager     |           |
| Issued: December 2, 2025                                                                                        |            |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |            |                       |           |



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY8 Module SAR       | 17.0.2      |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 15 mm                  | with spacer |
| Frequency                    | 835MHz $\pm$ 1MHz      |             |

## HSL parameters at 835 MHz

The following parameters and calculations were applied.

|                                    | Temperature         | Permittivity  | Conductivity        |
|------------------------------------|---------------------|---------------|---------------------|
| Nominal HSL parameters             | 22.0 °C             | 41.5          | 0.90 mho/m          |
| Measured HSL parameters            | (22.0 $\pm$ 0.2) °C | 41.6 $\pm$ 6% | 0.91 mho/m $\pm$ 6% |
| HSL temperature change during test | < 0.5 °C            |               |                     |

## SAR result with HSL at 835 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of HSL | Condition          |                               |
|--------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                   | 24 dBm input power | 2.35 W/kg                     |
| SAR for nominal HSL parameters                   | normalized to 1W   | 9.36 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of HSL | Condition          |                               |
|----------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                     | 24 dBm input power | 1.52 W/kg                     |
| SAR for nominal HSL parameters                     | normalized to 1W   | 6.05 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 835 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 52.5 $\Omega$ – 3.1 j $\Omega$ |
| Return Loss | -28.2 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.392 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D835V2 - SN4d167 | 835             | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, ULD | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 15                 |      | CW, 0—     | 835, 0                          | 9.51              | 0.91                   | 41.6             |

Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|---------------|--------------------|-----------------------------|---------------------------|
| Flat V4.9 mod | HSL, 2025-12-02    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2025-11-26 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 6.0 x 6.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |

Measurement Results



|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-12-02          |
| psSAR1g [W/Kg]      | 2.35                |
| psSAR10g [W/Kg]     | 1.52                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

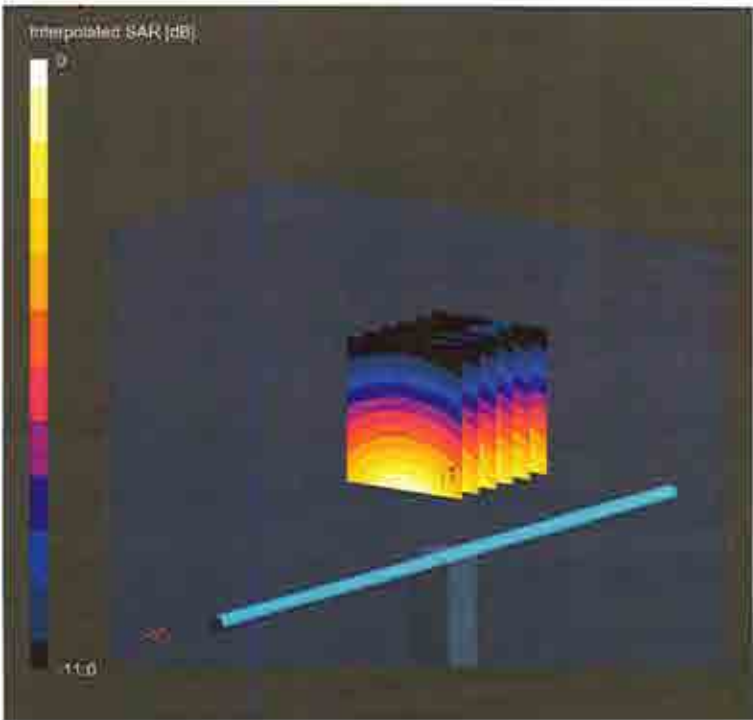

0 dB = 3.65 W/Kg

## Impedance Measurement Plot for HSL

S11 Smith (R+jX) Scale 1.00
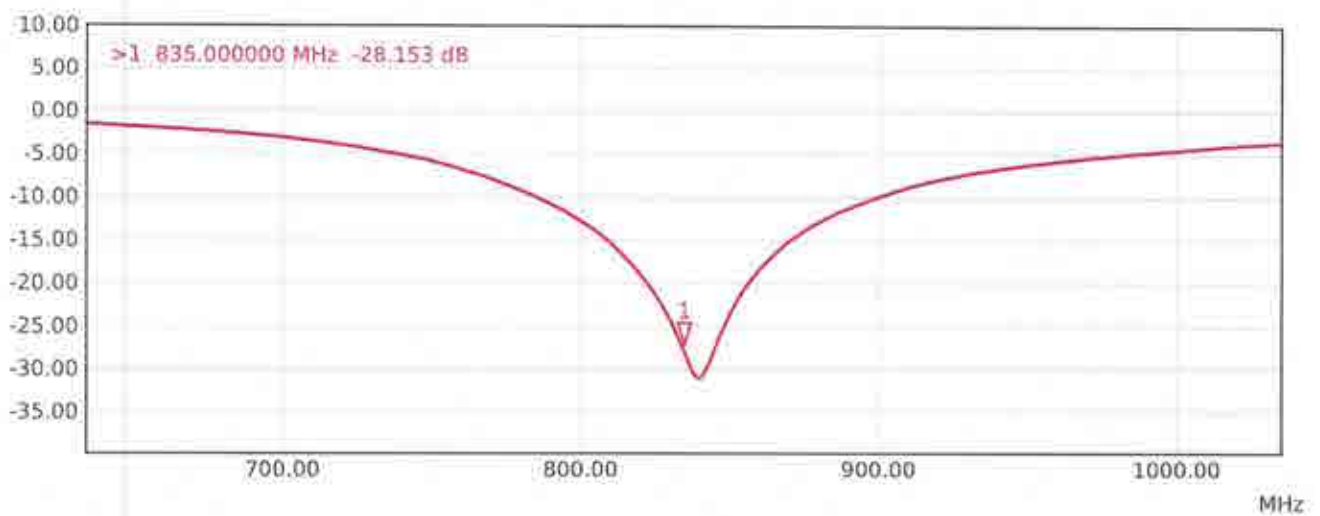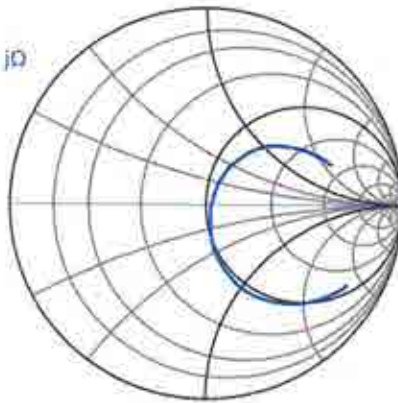
>1 835.000000 MHz 52.500  $\Omega$  -3.137  $j\Omega$ 



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D1750V2-1112\_Feb25**

## CALIBRATION CERTIFICATE

Object

**D1750V2 - SN: 1112**

Calibration procedure(s)

**QA CAL-05.v12**

**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date

**February 20, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               |                  |                       |
|---------------|------------------|-----------------------|
|               | Name             | Function              |
| Calibrated by | Krešimir Franjić | Laboratory Technician |
| Approved by   | Sven Kühn        | Technical Manager     |

Signature

Issued: February 20, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of

Schmid & Partner  
Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

## Glossary

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 10 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 6mm; dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 1750MHz $\pm$ 1MHz       |                                     |

## Head TSL parameters at 1750 MHz

The following parameters and calculations were applied.

|                                         | Temperature        | Permittivity  | Conductivity        |
|-----------------------------------------|--------------------|---------------|---------------------|
| Nominal Head TSL parameters             | 22.0 °C            | 40.1          | 1.37 mho/m          |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2)°C | 39.7 $\pm$ 6% | 1.32 mho/m $\pm$ 6% |
| Head TSL temperature change during test | < 0.5 °C           |               |                     |

## SAR result with Head TSL at 1750 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                               |
|-------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                   | 24 dBm input power | 9.12 W/kg                     |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 36.3 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                               |
|---------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                     | 24 dBm input power | 4.84 W/kg                     |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 19.3 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 1750 MHz**

|             |                             |
|-------------|-----------------------------|
| Impedance   | $51.2 \Omega + 1.8 j\Omega$ |
| Return Loss | -33.2 dB                    |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.212 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency (MHz) | TSL | Power (dBm) |
|------------------|-----------------|-----|-------------|
| D1750V2 - SN1112 | 1750            | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance (mm) | Band | Group, UID | Frequency (MHz), Channel Number | Conversion Factor | TSL Conductivity (S/m) | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 1750, 0                         | 7.96              | 1.32                   | 39.7             |

Hardware Setup

| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-02-20    | EX3DV4 - SN7345, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents (mm)   | 10 x 30 x 30    |
| Grid Steps (mm)     | 6.0 x 6.0 x 1.5 |
| Sensor Surface (mm) | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS - 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-02-20          |
| psSAR1g (W/Kg)      | 9.12                |
| psSAR10g (W/Kg)     | 4.84                |
| Power Drift (dB)    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor (dB) |                     |
| TSL Correction      | Positive / Negative |



0 dB = 15.7 W/Kg

## Impedance Measurement Plot for Head TSL

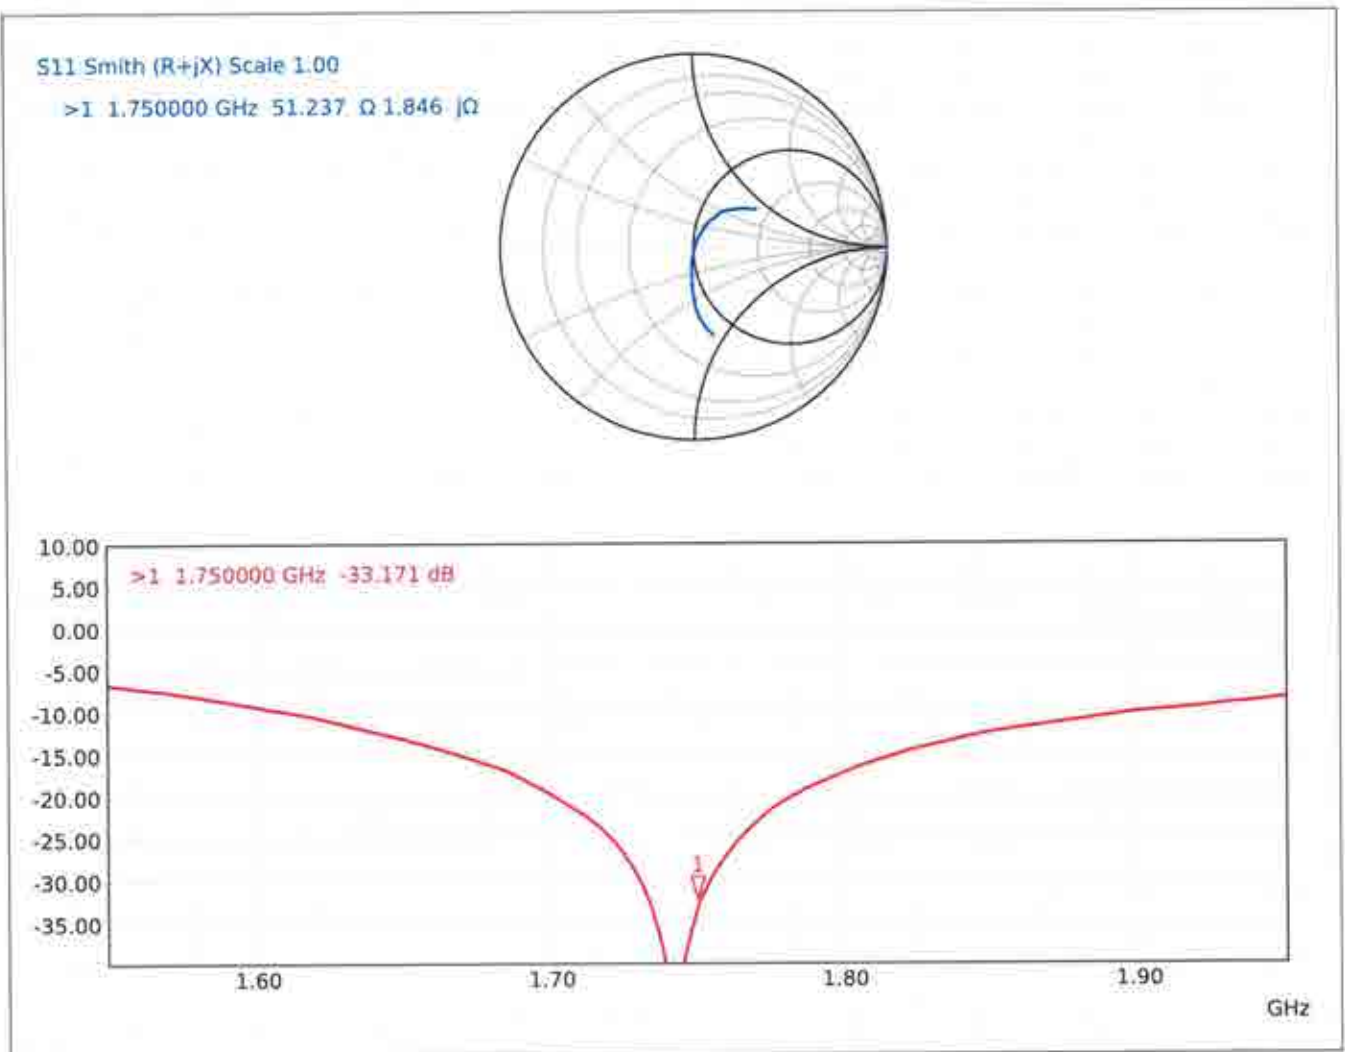



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D1750V2-1112\_Feb25**

## CALIBRATION CERTIFICATE

Object

**D1750V2 - SN: 1112**

Calibration procedure(s)

**QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date

**February 20, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .


Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               |                  |                       |
|---------------|------------------|-----------------------|
|               | Name             | Function              |
| Calibrated by | Krešimir Franjić | Laboratory Technician |
| Approved by   | Sven Kühn        | Technical Manager     |

Signature



Issued: February 20, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 10 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 6mm; dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 1750MHz $\pm$ 1MHz       |                                     |

## Head TSL parameters at 1750 MHz

The following parameters and calculations were applied.

|                                         | Temperature        | Permittivity  | Conductivity        |
|-----------------------------------------|--------------------|---------------|---------------------|
| Nominal Head TSL parameters             | 22.0 °C            | 40.1          | 1.37 mho/m          |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2)°C | 39.7 $\pm$ 6% | 1.32 mho/m $\pm$ 6% |
| Head TSL temperature change during test | < 0.5 °C           |               |                     |

## SAR result with Head TSL at 1750 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                               |
|-------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                   | 24 dBm input power | 9.12 W/kg                     |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 36.3 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                               |
|---------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                     | 24 dBm input power | 4.84 W/kg                     |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 19.3 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 1750 MHz**

|             |                             |
|-------------|-----------------------------|
| Impedance   | $51.2 \Omega + 1.8 j\Omega$ |
| Return Loss | -33.2 dB                    |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.212 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency (MHz) | TSL | Power (dBm) |
|------------------|-----------------|-----|-------------|
| D1750V2 - SN1112 | 1750            | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance (mm) | Band | Group, UID | Frequency (MHz), Channel Number | Conversion Factor | TSL Conductivity (S/m) | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 1750, 0                         | 7.96              | 1.32                   | 39.7             |

Hardware Setup

| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-02-20    | EX3DV4 - SN7345, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents (mm)   | 10 x 30 x 30    |
| Grid Steps (mm)     | 6.0 x 6.0 x 1.5 |
| Sensor Surface (mm) | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS - 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-02-20          |
| psSAR1g (W/Kg)      | 9.12                |
| psSAR10g (W/Kg)     | 4.84                |
| Power Drift (dB)    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor (dB) |                     |
| TSL Correction      | Positive / Negative |



0 dB = 15.7 W/Kg

## Impedance Measurement Plot for Head TSL

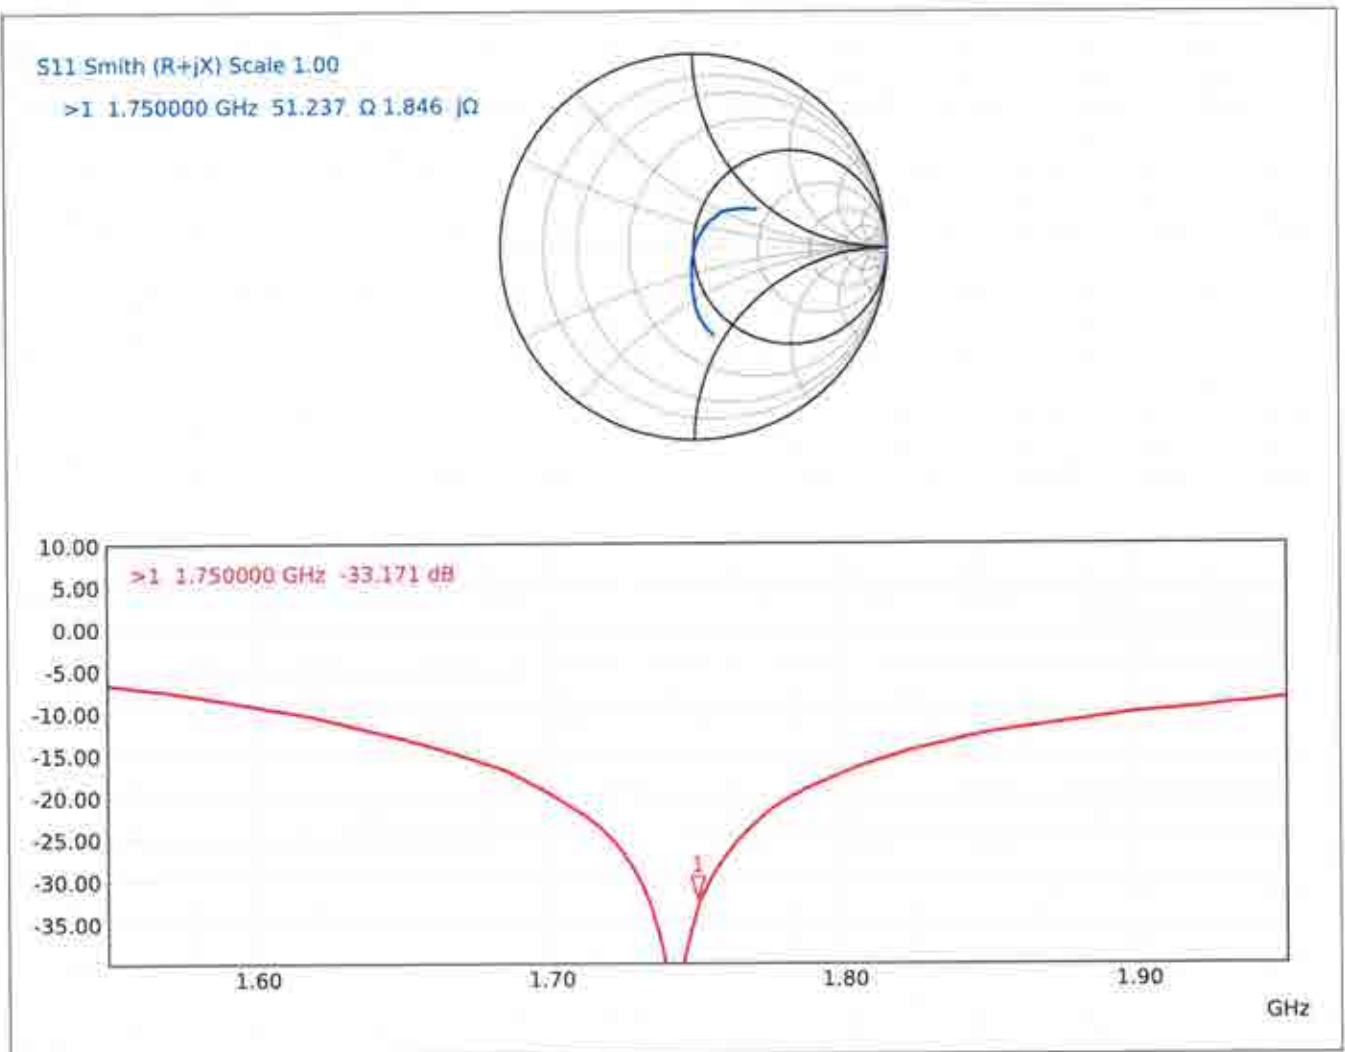

## D1750V2, serial no. 1112 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.


### <Justification of the extended calibration>

| D1750V2 – serial no. 1112   |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
|                             | 1750MHZ          |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 02.20.2025<br>(Cal. Report) | -33.2            |           | 51.2                 |             | 1.8                       |             |
| 02.19.2026<br>(extended)    | -31.841          | -4.09     | 50.261               | -0.939      | 1.99                      | 0.19        |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D1750 V2, serial no. 1112 (Data of Measurement : 02.19.2026)

1750MHz - Head

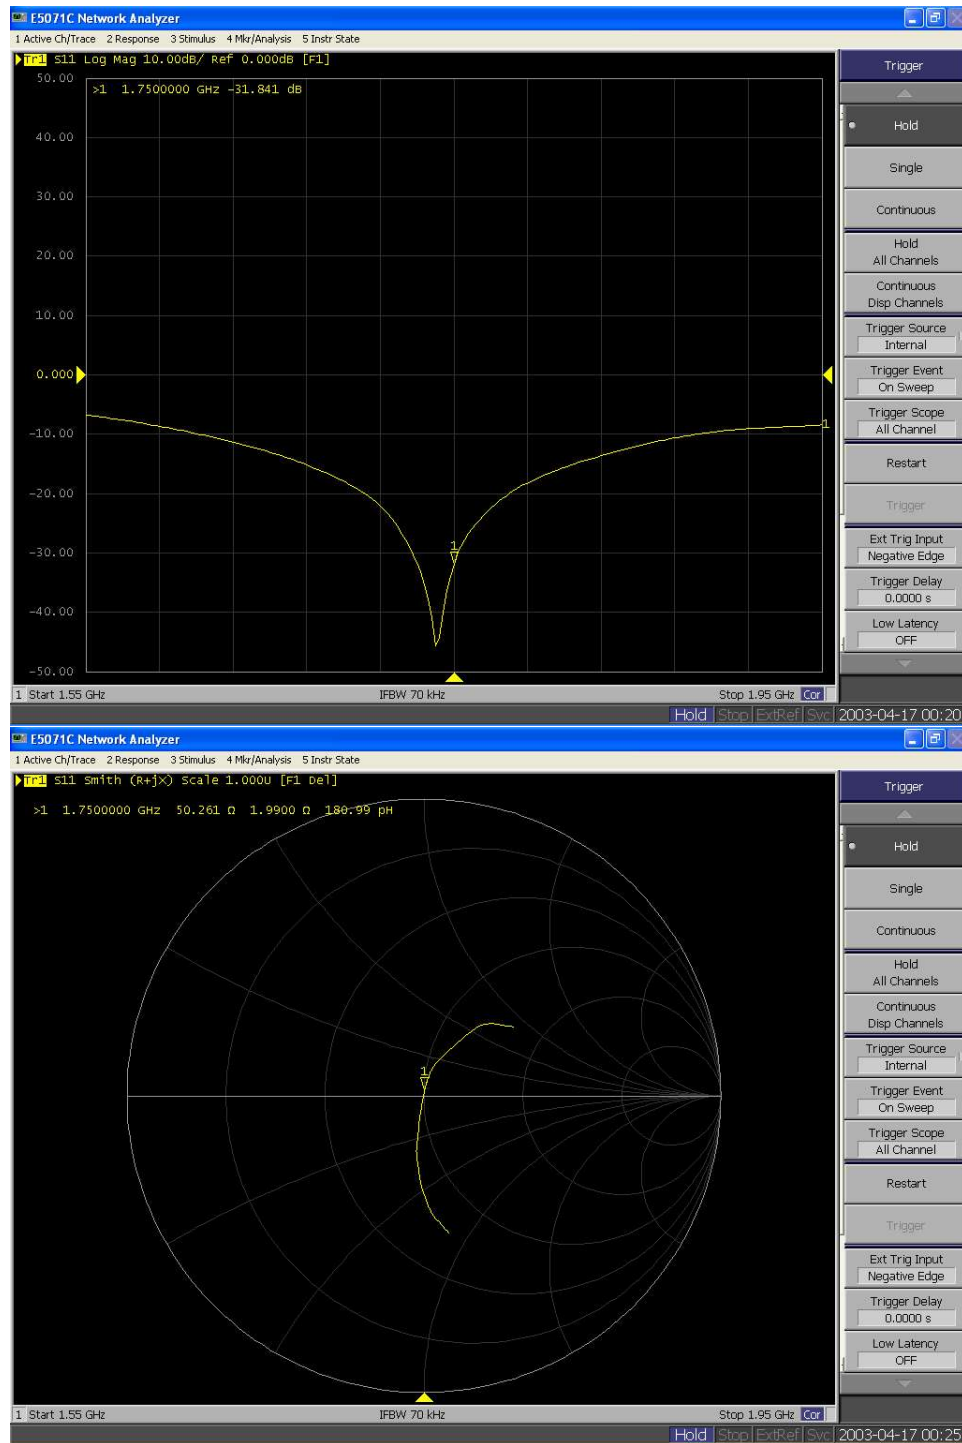



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client  
**Sporton**  
Taoyuan City

Certificate No. **D1900V2-5d041\_Aug24**

## CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d041**

Calibration procedure(s) **QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date **August 15, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)            | Scheduled Cal |
|--------------------------------------------|------------|---------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)             | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 21-Mar-24 (No. 4030A315007801)        | Mar-25        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 25-Jan-24 (No. 4030-315007551)        | Jan-25        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)             | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 05-Oct-23 (No. OCP-DAK12-1016_Oct23)  | Oct-24        |
| OCP DAK-3.5                                | SN: 1249   | 05-Oct-23 (No. OCP-DAK3.5-1249_Oct23) | Oct-24        |
| Reference Probe EX3DV4                     | SN: 7349   | 03-Jun-24 (No. EX3-7349_Jun24)        | Jun-25        |
| DAE4ip                                     | SN: 1836   | 10-Jan-24 (No. DAE4ip-1836_Jan24)     | Jan-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 0001-300719404)             | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               |                   |                       |           |
|---------------|-------------------|-----------------------|-----------|
|               | Name              | Function              | Signature |
| Calibrated by | Krešimir Franjlić | Laboratory Technician |           |
| Approved by   | Sven Kühn         | Technical Manager     |           |

Issued: August 16, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 10 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 6mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 1900MHz $\pm$ 1MHz       |                                     |

## Head TSL parameters at 1900 MHz

The following parameters and calculations were applied.

|                                         | Temperature        | Permittivity  | Conductivity        |
|-----------------------------------------|--------------------|---------------|---------------------|
| Nominal Head TSL parameters             | 22.0 °C            | 40.0          | 1.40 mho/m          |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2)°C | 41.2 $\pm$ 6% | 1.40 mho/m $\pm$ 6% |
| Head TSL temperature change during test | < 0.5 °C           |               |                     |

## SAR result with Head TSL at 1900 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                               |
|-------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                   | 24 dBm input power | 9.84 W/kg                     |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 39.2 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                               |
|---------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                     | 24 dBm input power | 5.21 W/kg                     |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 20.7 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 1900 MHz**

|             |                             |
|-------------|-----------------------------|
| Impedance   | $51.4 \Omega + 6.2 j\Omega$ |
| Return Loss | -24.1 dB                    |

**General Antenna Parameters and Design**

|                                  |        |
|----------------------------------|--------|
| Electrical Delay (one direction) | 1,2 ns |
|----------------------------------|--------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole            | Frequency [MHz] | TSL | Power [dBrm] |
|-------------------|-----------------|-----|--------------|
| D1900V2 - SN5d041 | 1900            | HSL | -24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- | 1900, 0    |                                 | 7.73              | 1.40                   | 41.2             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MPP V8.0 Center | HSL 2024-08-15     | EX3DV4 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 6.0 x 6.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS - 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-08-15          |
| psSAR1g [W/Kg]      | 3.84                |
| psSAR10g [W/Kg]     | 5.21                |
| Power Drift [dB]    | 0.01                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

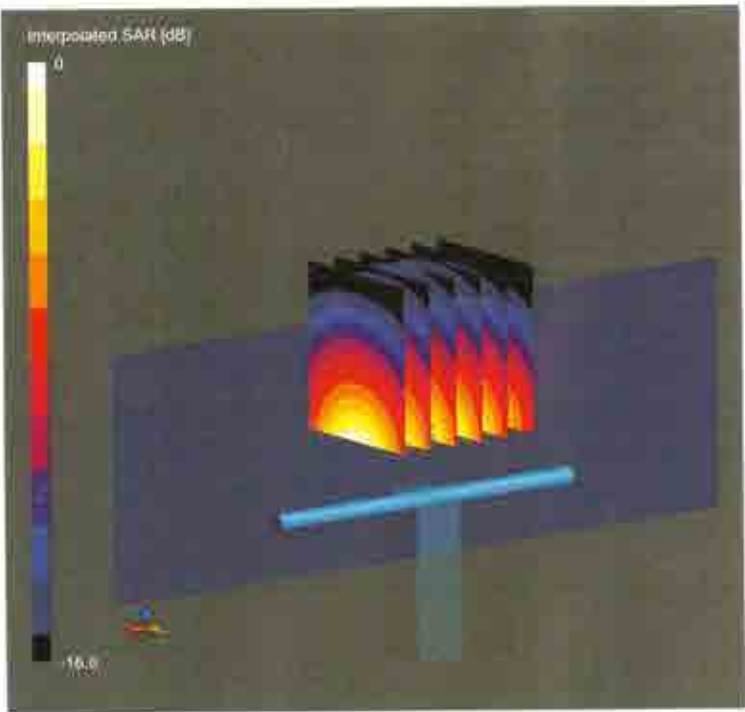

0 dB = 17.3 W/Kg

Impedance Measurement Plot for Head TSL

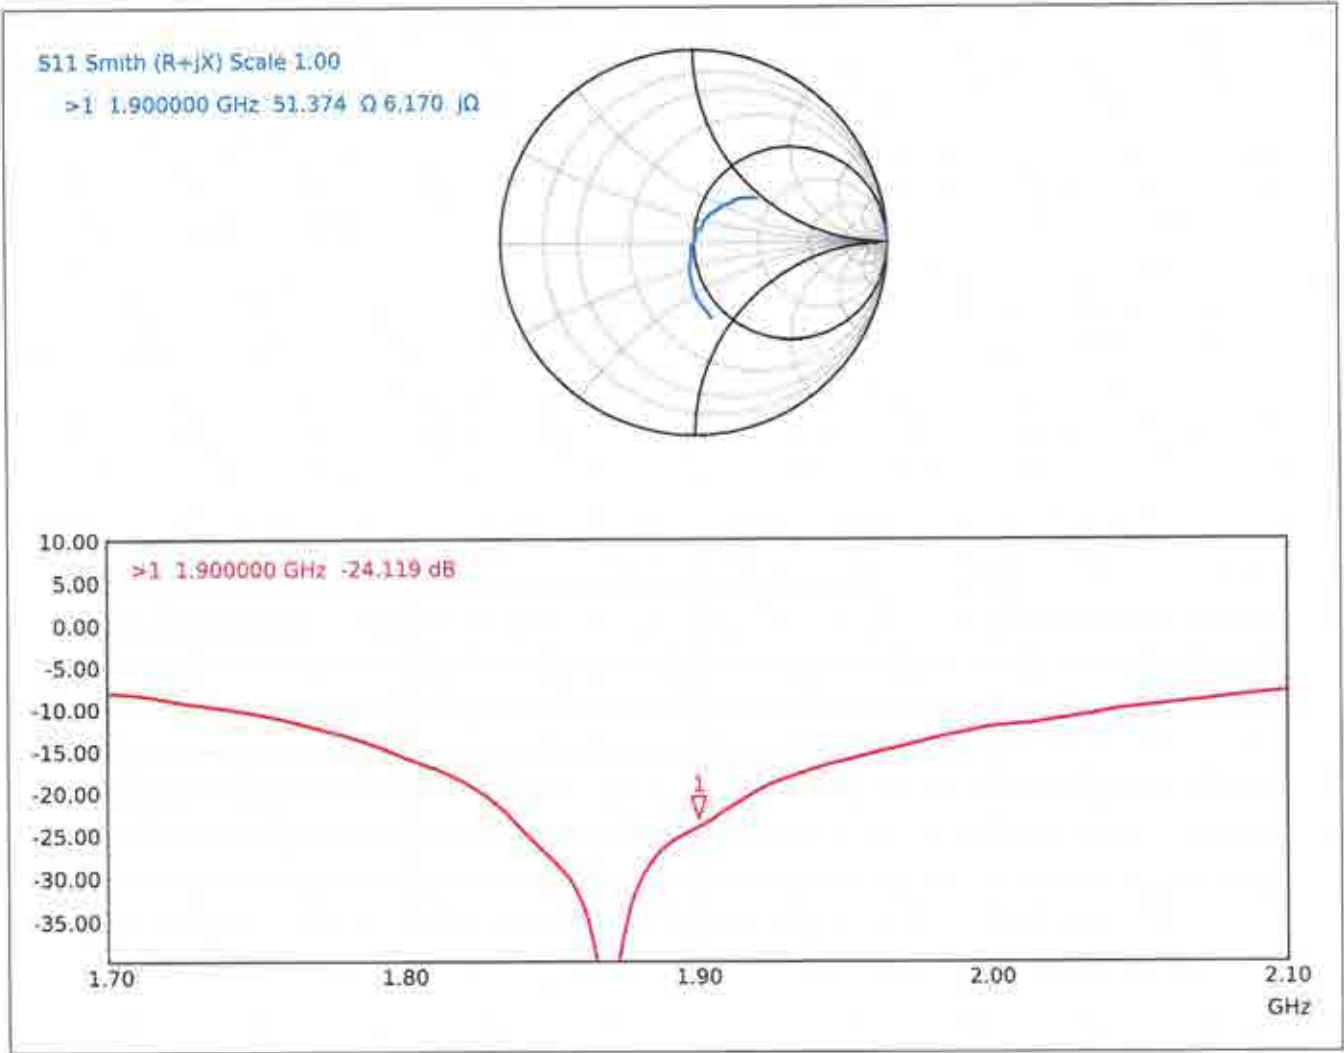

## D1900V2, serial no. 5d041 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.



### <Justification of the extended calibration>

| D1900V2 – serial no. 5d041  |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
|                             | 1900MHZ          |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 08.15.2024<br>(Cal. Report) | -24.1            |           | 51.4                 |             | +6.2                      |             |
| 08.14.2025<br>(extended)    | -24.032          | -0.28     | 52.419               | 1.019       | +6.2849                   | 0.0849      |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D1900 V2, serial no. 5d041 (Data of Measurement : 08.14.2025)

1900MHz - Head

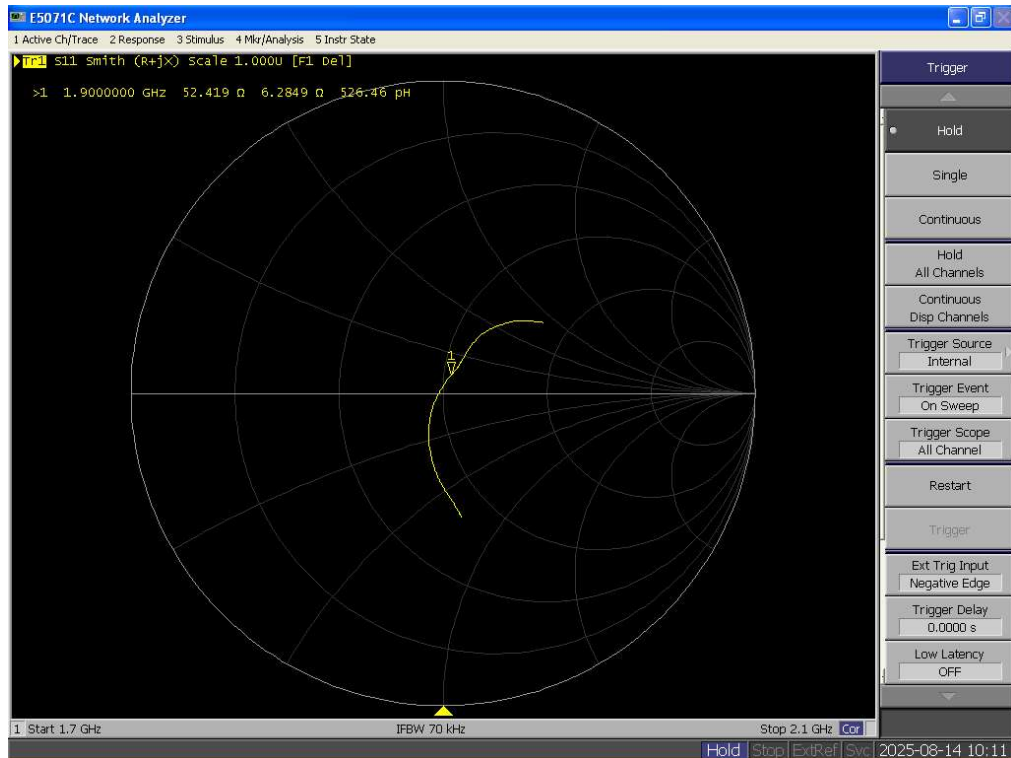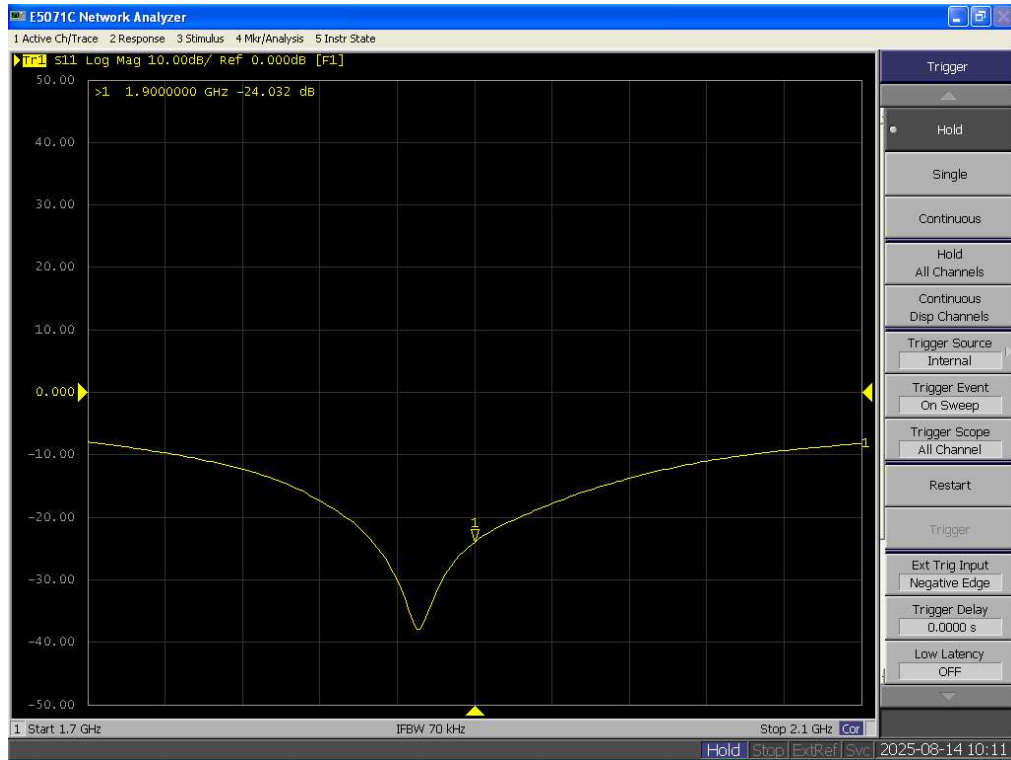



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Sporton**  
**Taoyuan City**

Certificate No. **D1900V2-5d185\_Jun25**

## CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d185**

Calibration procedure(s) **QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date **June 11, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|-----------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T    | SN: 100967 | 26-Mar-25 (No. 217-04290)              | Mar-26        |
| Power Sensor R&S NRP18A     | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40 | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| 3.5mm mismatch combination  | SN: 1152   | 24-Mar-25 (No. 217-04293)              | Mar-26        |
| OCP DAK-12                  | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                 | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                      | SN: 1836   | 17-Apr-25 (No. DAE4ip-1836_Apr25)      | Apr-26        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Setup 1                 | SN: 1000   | 27-May-25 (No. 675-ACAD_Source_Box-250527) | May-26          |
| Signal Generator R&S SMB100A | SN: 182081 | 27-May-25 (No. 675-CAL16-S4588-250527)     | May-26          |
| Mismatch; SMA                | SN: 1102   | 24-Apr-25 (No. 675-Mismatch_SMA-250424)    | Apr-26          |
| OCP DAK-12                   | SN: 1029   | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)       | Feb-26          |
| OCP DAK-3.5                  | SN: 1336   | 09-Dec-24 (No. OCP-DAK3.5-1336_Dec24)      | Dec-25          |

|               |            |                       |           |
|---------------|------------|-----------------------|-----------|
|               | Name       | Function              | Signature |
| Calibrated by | Paulo Pina | Laboratory Technician |           |
| Approved by   | Sven Kühn  | Technical Manager     |           |

Issued: June 11, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 10 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 6mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 1900MHz $\pm$ 1MHz       |                                     |

## HSL parameters at 1900 MHz

The following parameters and calculations were applied.

|                                    | Temperature         | Permittivity  | Conductivity        |
|------------------------------------|---------------------|---------------|---------------------|
| Nominal HSL parameters             | 22.0 °C             | 40.0          | 1.40 mho/m          |
| Measured HSL parameters            | (22.0 $\pm$ 0.2) °C | 40.2 $\pm$ 6% | 1.38 mho/m $\pm$ 6% |
| HSL temperature change during test | < 0.5 °C            |               |                     |

## SAR result with HSL at 1900 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of HSL | Condition          |                               |
|--------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                   | 24 dBm input power | 9.94 W/kg                     |
| SAR for nominal HSL parameters                   | normalized to 1W   | 39.6 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of HSL | Condition          |                               |
|----------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                     | 24 dBm input power | 5.23 W/kg                     |
| SAR for nominal HSL parameters                     | normalized to 1W   | 20.8 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 1900 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 53.2 $\Omega$ + 4.0 j $\Omega$ |
| Return Loss | -26.1 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.203 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole            | Frequency [MHz] | TSL | Power [dBm] |
|-------------------|-----------------|-----|-------------|
| D1900V2 - 5N5d185 | 1900            | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0---   | 1900, 0                         | 7.68              | 1.38                   | 40.2             |

Hardware Setup


| Phantom        | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Right | HSL, 2025-06-11    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2025-04-17 |

Scans Setup


|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 6.0 x 6.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS +/- 6p      |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-06-11          |
| psSAR1g [W/Kg]      | 9.94                |
| psSAR10g [W/Kg]     | 5.23                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

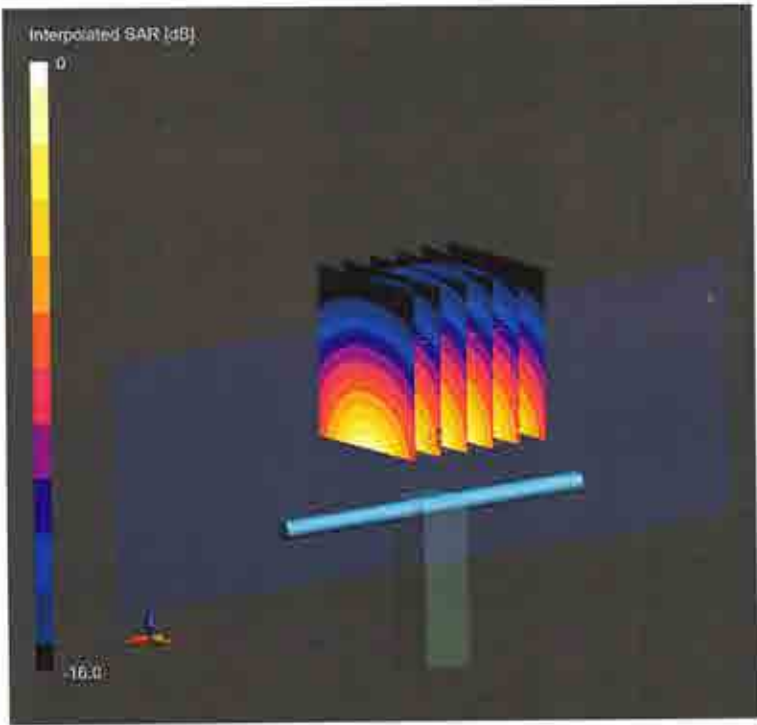

Impedance Measurement Plot for HSL

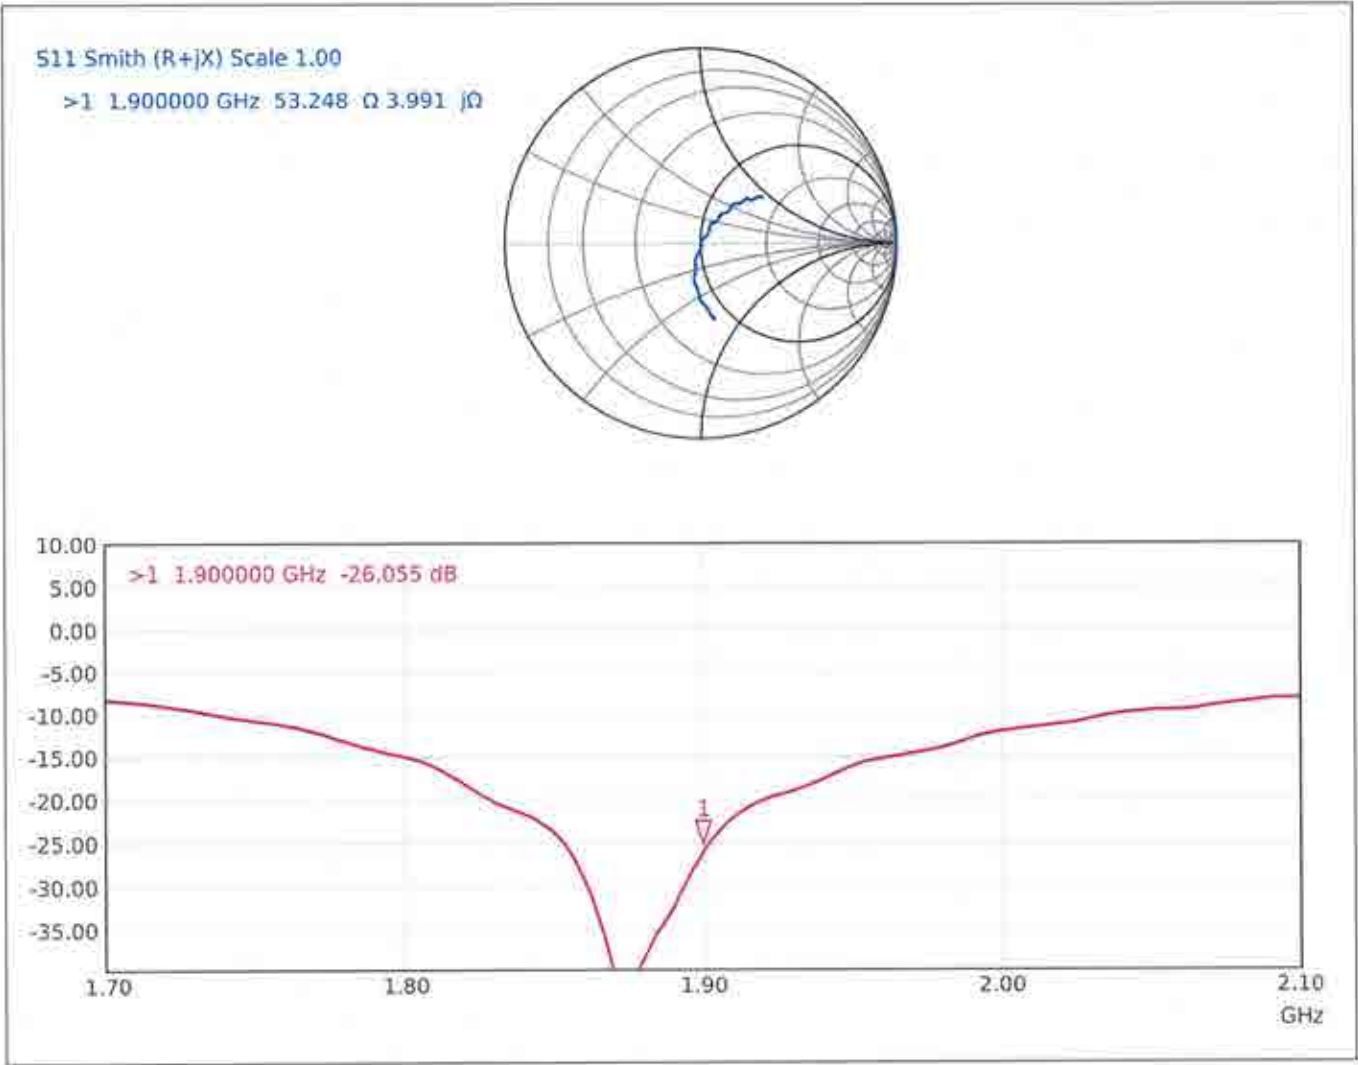



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D2300V2-1006\_Jan25**

## CALIBRATION CERTIFICATE

Object

**D2300V2 - SN: 1006**

Calibration procedure(s)

**QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date

**January 14, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 22-Jul-24 (No. 4030A315008547)         | Jul-25        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 25-Jan-24 (No. 4030-315007551)         | Jan-25        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|                                                                                                                 | Name       | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|------------|-----------------------|-----------|
| Calibrated by                                                                                                   | Paulo Pina | Laboratory Technician |           |
| Approved by                                                                                                     | Sven Kühn  | Technical Manager     |           |
| Issued: January 14, 2025                                                                                        |            |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the Laboratory. |            |                       |           |



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |                                     |
|-------------------------------------|--------------------------|-------------------------------------|
| <b>DASY Version</b>                 | DASY8 Module SAR         | 16.4.0                              |
| <b>Extrapolation</b>                | Advanced Extrapolation   |                                     |
| <b>Phantom</b>                      | Modular Flat Phantom     |                                     |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with spacer                         |
| <b>Zoom Scan Resolution</b>         | dx, dy = 5mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| <b>Frequency</b>                    | 2300MHz $\pm$ 1MHz       |                                     |

## Head TSL parameters at 2300 MHz

The following parameters and calculations were applied.

|                                                | Temperature        | Permittivity  | Conductivity        |
|------------------------------------------------|--------------------|---------------|---------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C            | 39.5          | 1.67 mho/m          |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2)°C | 38.5 $\pm$ 6% | 1.71 mho/m $\pm$ 6% |
| <b>Head TSL temperature change during test</b> | < 0.5 °C           |               |                     |

## SAR result with Head TSL at 2300 MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                               |
|-------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                         | 24 dBm input power | 12.1 W/kg                     |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | 48.2 W/kg $\pm$ 17.0% (k = 2) |

| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                               |
|---------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                           | 24 dBm input power | 5.83 W/kg                     |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 23.2 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 2300 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 49.0 $\Omega$ – 3.1 j $\Omega$ |
| Return Loss | -29.5 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.168 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D2300V2 - SN1006 | 2300            | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- |            | 2300, 0                         | 7.48              | 1.71                   | 38.5             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-01-14    | EX3DV# - SN7349, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-01-14          |
| psSAR1g [W/Kg]      | 12.1                |
| psSAR10g [W/Kg]     | 5.81                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

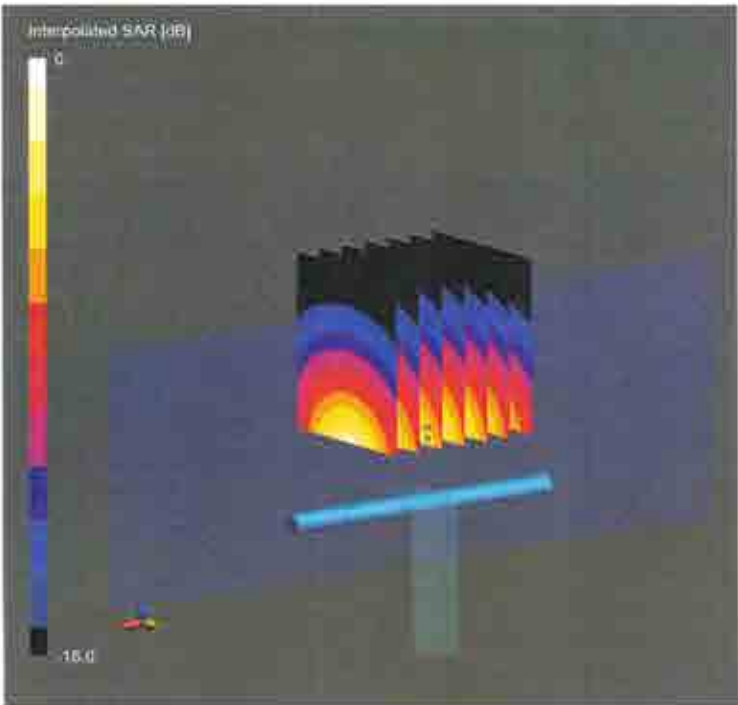

0 dB = 24.5 W/Kg

## Impedance Measurement Plot for Head TSL

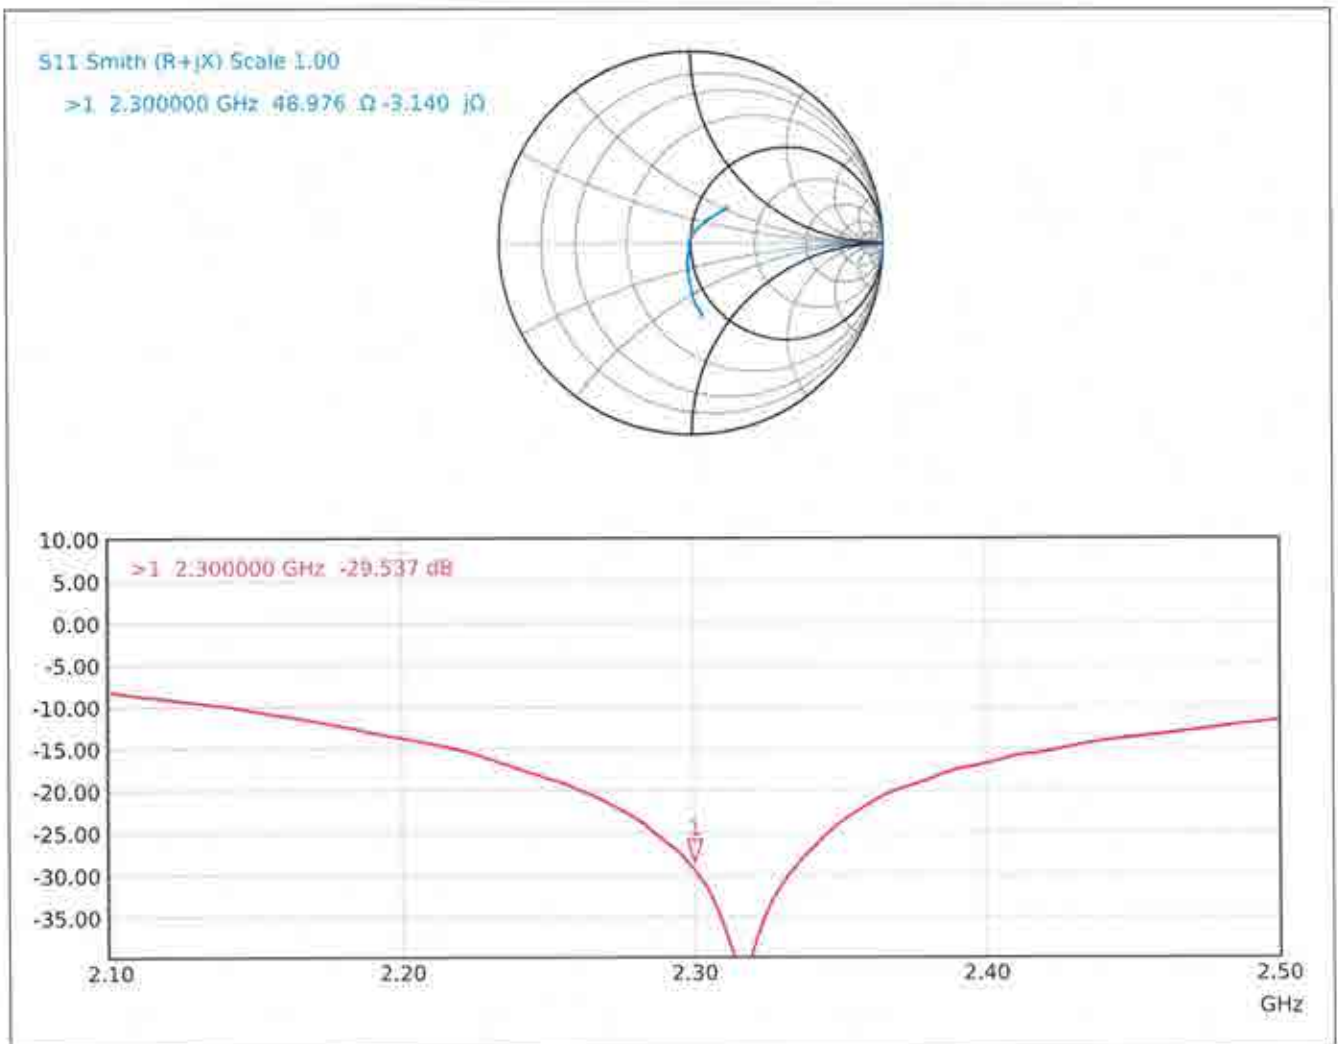

## D2300V2, serial no. 1006 Extended Dipole Calibrations

If dipoles are verified in return loss ( $<-20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.


### <Justification of the extended calibration>

| D2300V2 – serial no. 1006   |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
|                             | 2300MHZ          |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 01.14.2025<br>(Cal. Report) | -29.5            |           | 49                   |             | -3.1                      |             |
| 01.13.2026<br>(extended)    | -32.045          | -7.94     | 47.184               | -1.816      | -4.5402                   | -1.4402     |

The return loss is  $<-20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D2300 V2, serial no. 1006 (Data of Measurement : 01.13.2026)

2300MHz - Head

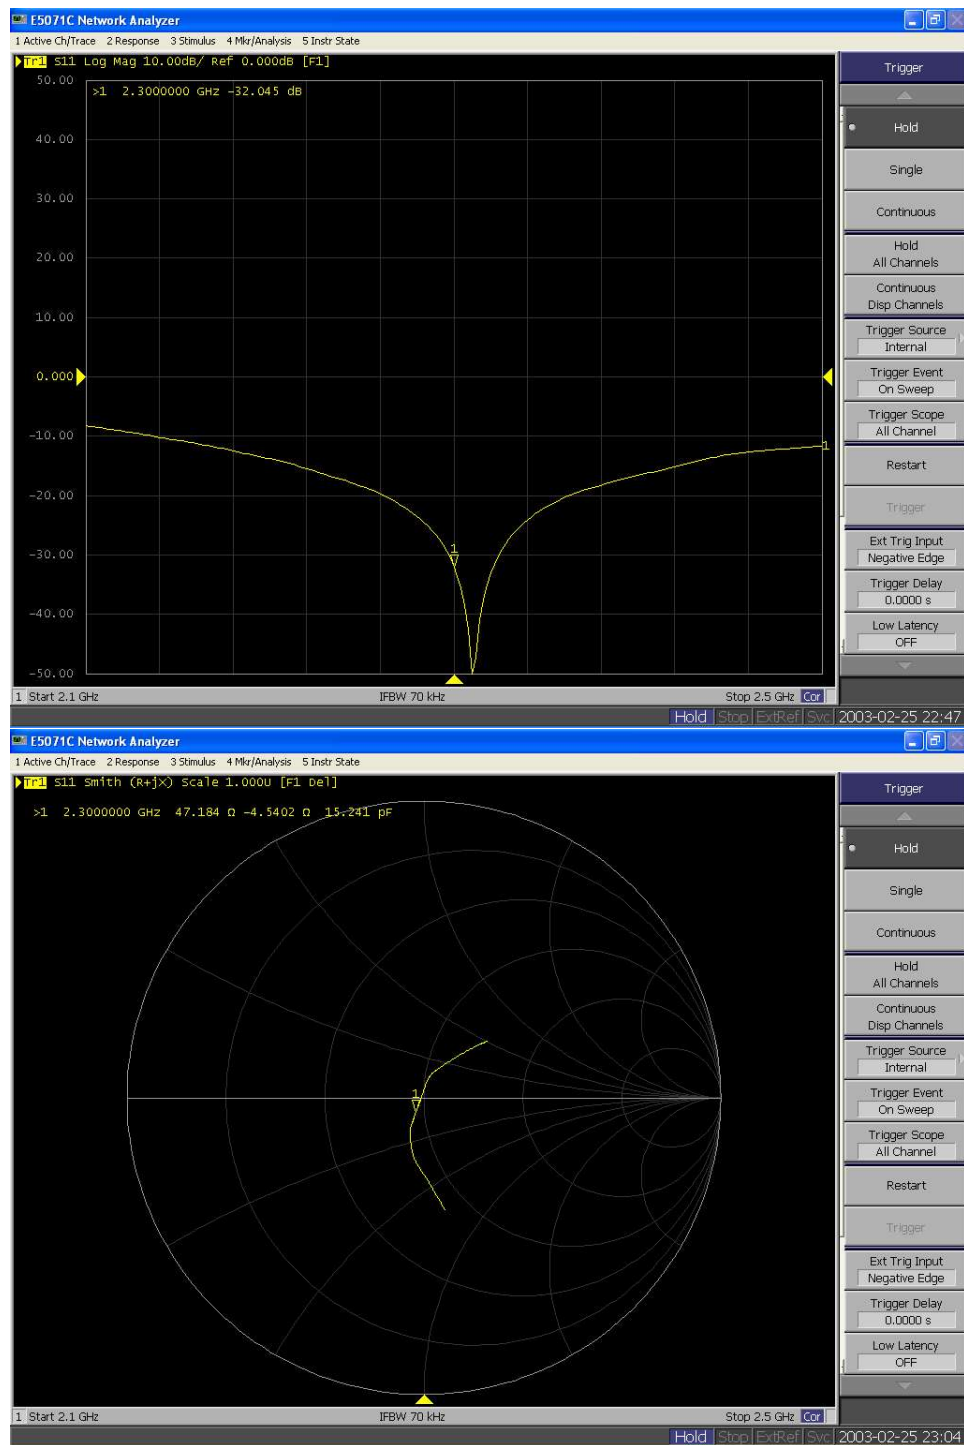

**Calibration Laboratory of****Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland

**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates****Accreditation No.: SCS 0108**

Client

**Sporton**

Taoyuan City

Certificate No.

**D2600V2-1008\_Aug24****CALIBRATION CERTIFICATE**Object **D2600V2 - SN: 1008**Calibration procedure(s) **QA CAL-05.v12  
Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**Calibration date **August 15, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)            | Scheduled Cal |
|--------------------------------------------|------------|---------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)             | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 21-Mar-24 (No. 4030A315007801)        | Mar-25        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 25-Jan-24 (No. 4030-315007551)        | Jan-25        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)             | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 05-Oct-23 (No. OCP-DAK12-1016_Oct23)  | Oct-24        |
| OCP DAK-3.5                                | SN: 1249   | 05-Oct-23 (No. OCP-DAK3.5-1249_Oct23) | Oct-24        |
| Reference Probe EX3DV4                     | SN: 7349   | 03-Jun-24 (No. EX3-7349_Jun24)        | Jun-25        |
| DAE4ip                                     | SN: 1836   | 10-Jan-24 (No. DAE4ip-1836_Jan24)     | Jan-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 0001-300719404)             | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               |                  |                       |
|---------------|------------------|-----------------------|
|               | Name             | Function              |
| Calibrated by | Krešimir Franjić | Laboratory Technician |
| Approved by   | Sven Kühn        | Technical Manager     |

Signature

Issued: August 16, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of

Schmid & Partner  
Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 10 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 5mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 2600MHz ±1MHz            |                                     |

Head TSL parameters at 2600 MHz

The following parameters and calculations were applied.

|                                         |               |              |                |
|-----------------------------------------|---------------|--------------|----------------|
|                                         | Temperature   | Permittivity | Conductivity   |
| Nominal Head TSL parameters             | 22.0 °C       | 39.0         | 1.96 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 37.3 ±6%     | 2.00 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

SAR result with Head TSL at 2600 MHz

|                                                       |                    |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
| SAR for nominal Head TSL parameters                   | 24 dBm input power | 14.0 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 55.7 W/kg ±17.0% (k = 2) |

|                                                         |                    |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
| SAR for nominal Head TSL parameters                     | 24 dBm input power | 6.35 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 25.3 W/kg ±16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 2600 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 49.0 $\Omega$ – 3.7 j $\Omega$ |
| Return Loss | -28.2 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.153 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D2600V2 - SN1008 | 2600            | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- |            | 2600, 0                         | 7.29              | 2.00                   | 37.3             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-08-15    | EX3DV4 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-08-15          |
| psSAR1g [W/Kg]      | 14.0                |
| psSAR10g [W/Kg]     | 6.35                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

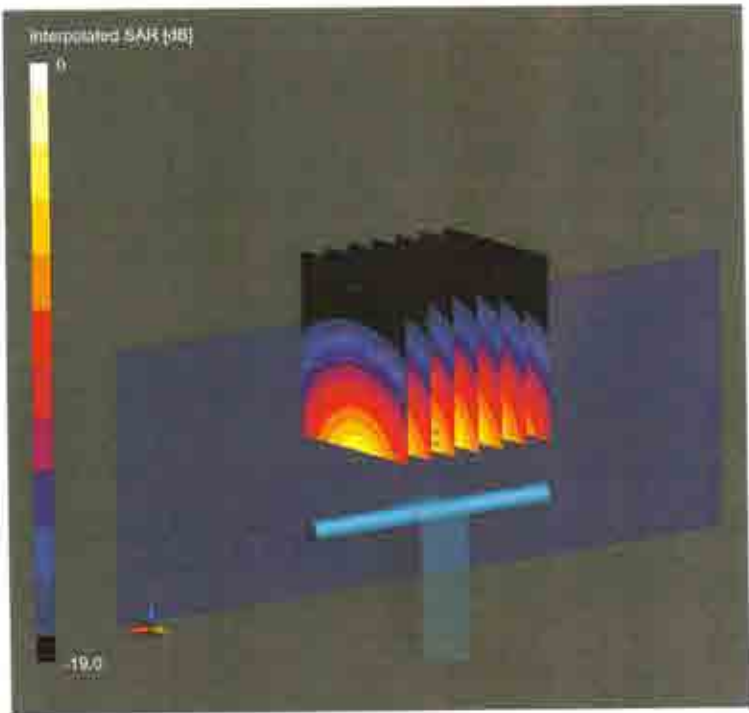

0 dB = 30.2 W/Kg

## Impedance Measurement Plot for Head TSL

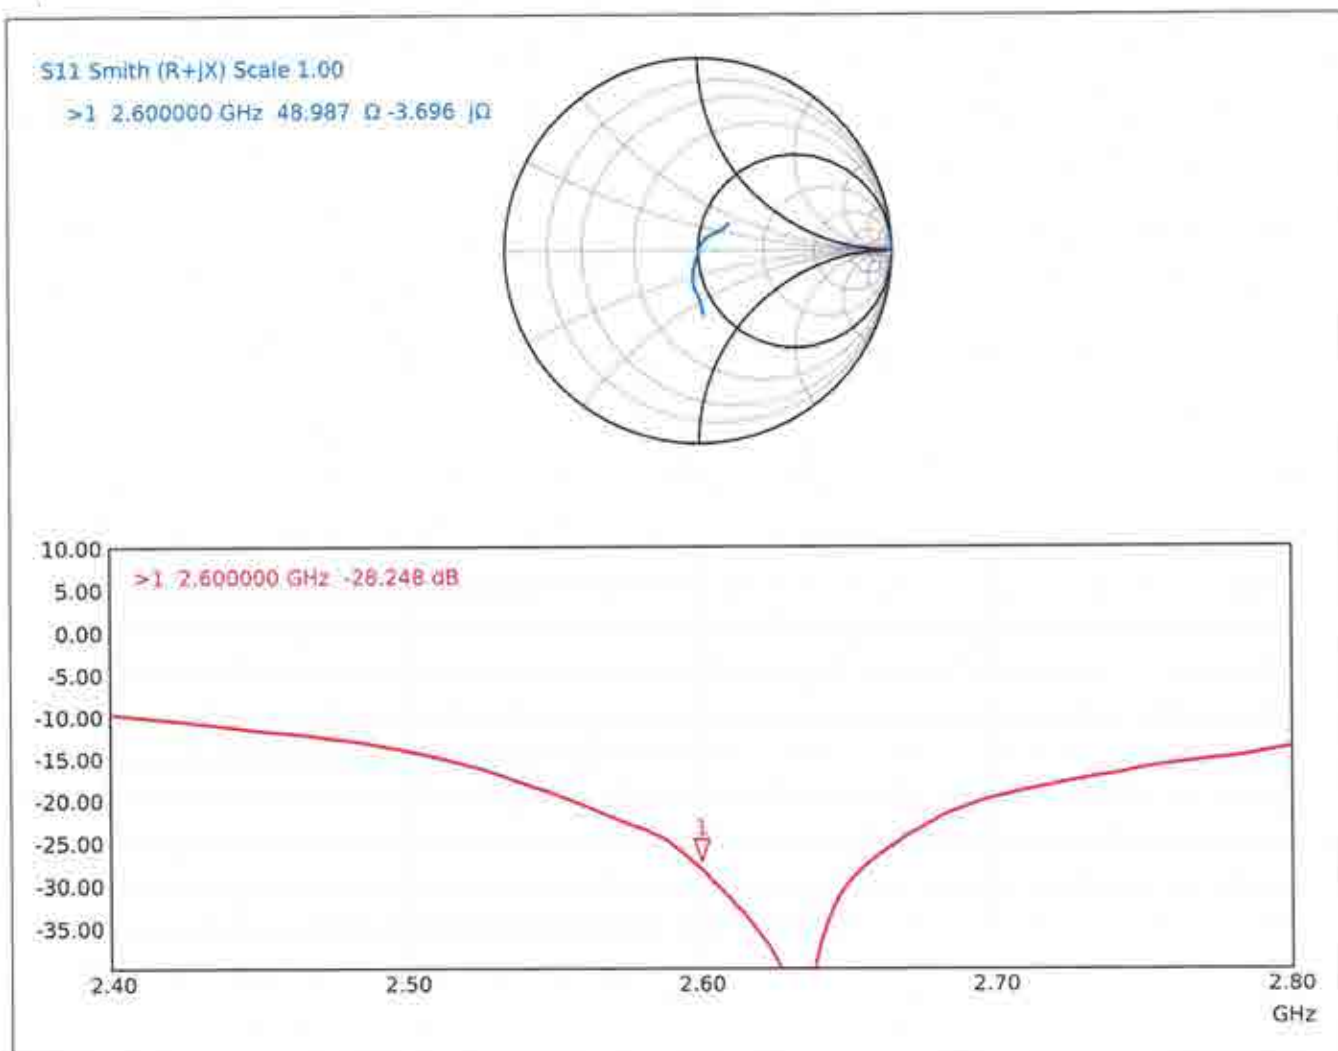

## D2600V2, serial no. 1008 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.


### <Justification of the extended calibration>

| D2600V2 – serial no. 1008   |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
|                             | 2600MHZ          |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 08.15.2024<br>(Cal. Report) | -28.2            |           | 49.0                 |             | -3.7                      |             |
| 08.14.2025<br>(extended)    | -27.546          | -2.31     | 45.688               | -3.312      | -3.654                    | 0.046       |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D2600 V2, serial no. 1008 (Data of Measurement : 08.14.2025)

2600MHz - Head

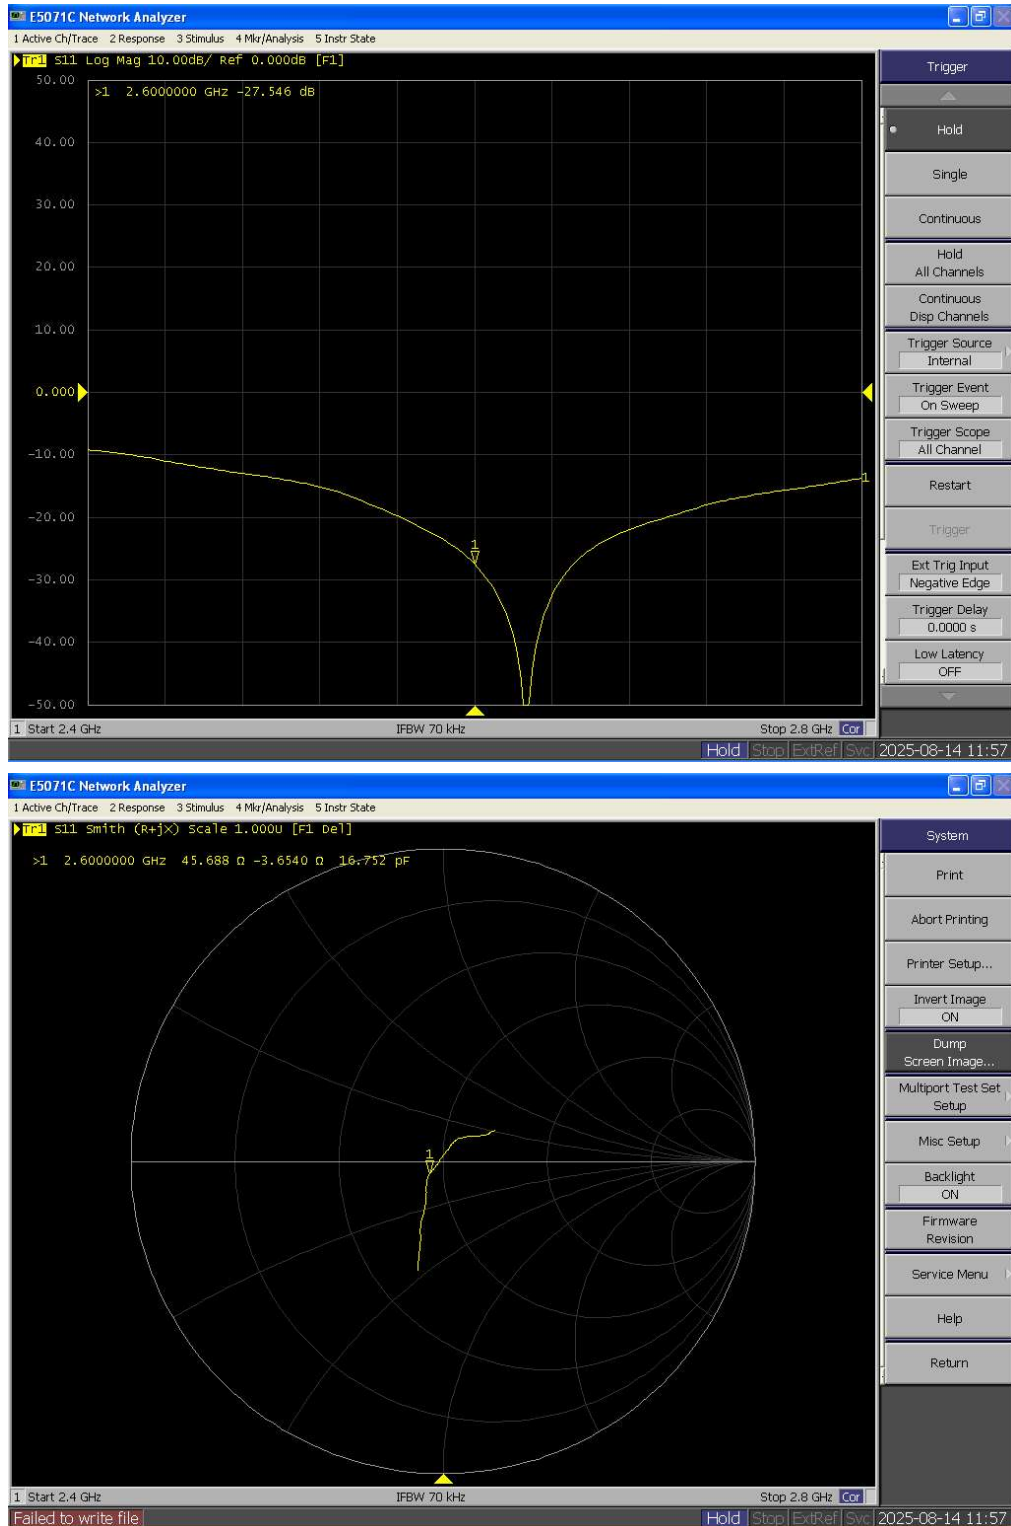

**Calibration Laboratory of****Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland

**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D3500V2-1014\_Jan25****CALIBRATION CERTIFICATE**

Object

**D3500V2 - SN: 1014**

Calibration procedure(s)

**QA CAL-22.v7****Calibration Procedure for SAR Validation Sources between 3 - 10 GHz**

Calibration date

**January 15, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 22-Jul-24 (No. 4030A315008547)         | Jul-25        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 25-Jan-24 (No. 4030-315007551)         | Jan-25        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               | Name       | Function              | Signature |
|---------------|------------|-----------------------|-----------|
| Calibrated by | Paulo Pina | Laboratory Technician |           |
| Approved by   | Sven Kühn  | Technical Manager     |           |

Issued: January 16, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |                                     |
|-------------------------------------|--------------------------|-------------------------------------|
| <b>DASY Version</b>                 | DASY8 Module SAR         | 16.4.0                              |
| <b>Extrapolation</b>                | Advanced Extrapolation   |                                     |
| <b>Phantom</b>                      | Modular Flat Phantom     |                                     |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with spacer                         |
| <b>Zoom Scan Resolution</b>         | dx, dy = 5mm, dz = 1.4mm | Graded Ratio = 1.5 mm (Z direction) |
| <b>Frequency</b>                    | 3500MHz $\pm$ 1MHz       |                                     |

## Head TSL parameters at 3500 MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity  | Conductivity        |
|------------------------------------------------|---------------------|---------------|---------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 37.9          | 2.91 mho/m          |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 37.9 $\pm$ 6% | 2.93 mho/m $\pm$ 6% |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            |               |                     |

## SAR result with Head TSL at 3500 MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                               |
|-------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                         | 20 dBm input power | 6.57 W/kg                     |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | 65.7 W/kg $\pm$ 19.9% (k = 2) |

| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                               |
|---------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                           | 20 dBm input power | 2.49 W/kg                     |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 24.9 W/kg $\pm$ 19.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 3500 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 54.0 $\Omega$ – 4.1 j $\Omega$ |
| Return Loss | -25.2 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.133 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D3500V2 - SN1014 | 3500            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0---   | 3500, 0                         | 6.63              | 2.93                   | 37.9             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-01-15    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 28 x 28 x 28    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS = 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-01-15          |
| psSAR1g [W/Kg]      | 6.57                |
| psSAR10g [W/Kg]     | 2.49                |
| Power Drift [dB]    | -0.04               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

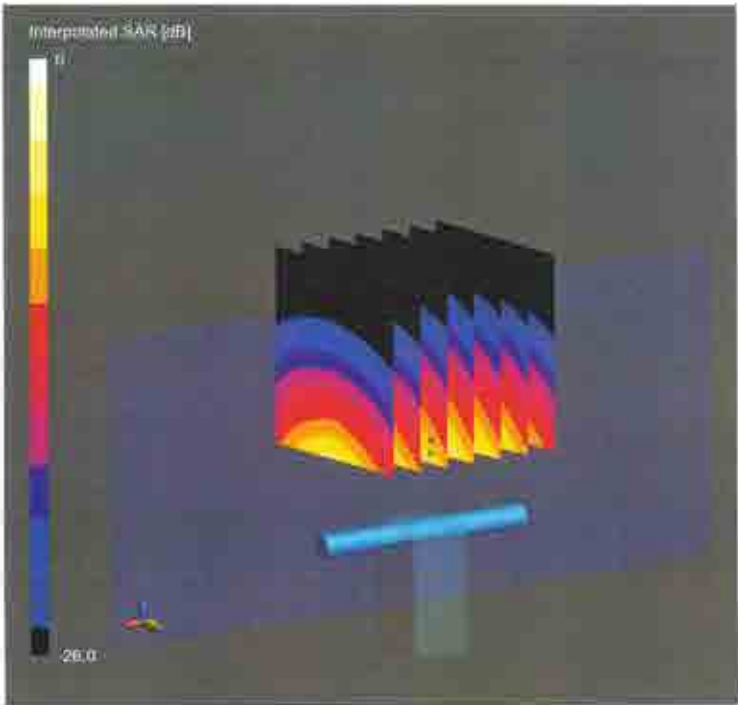

0 dB = 17.2 W/Kg

## Impedance Measurement Plot for Head TSL

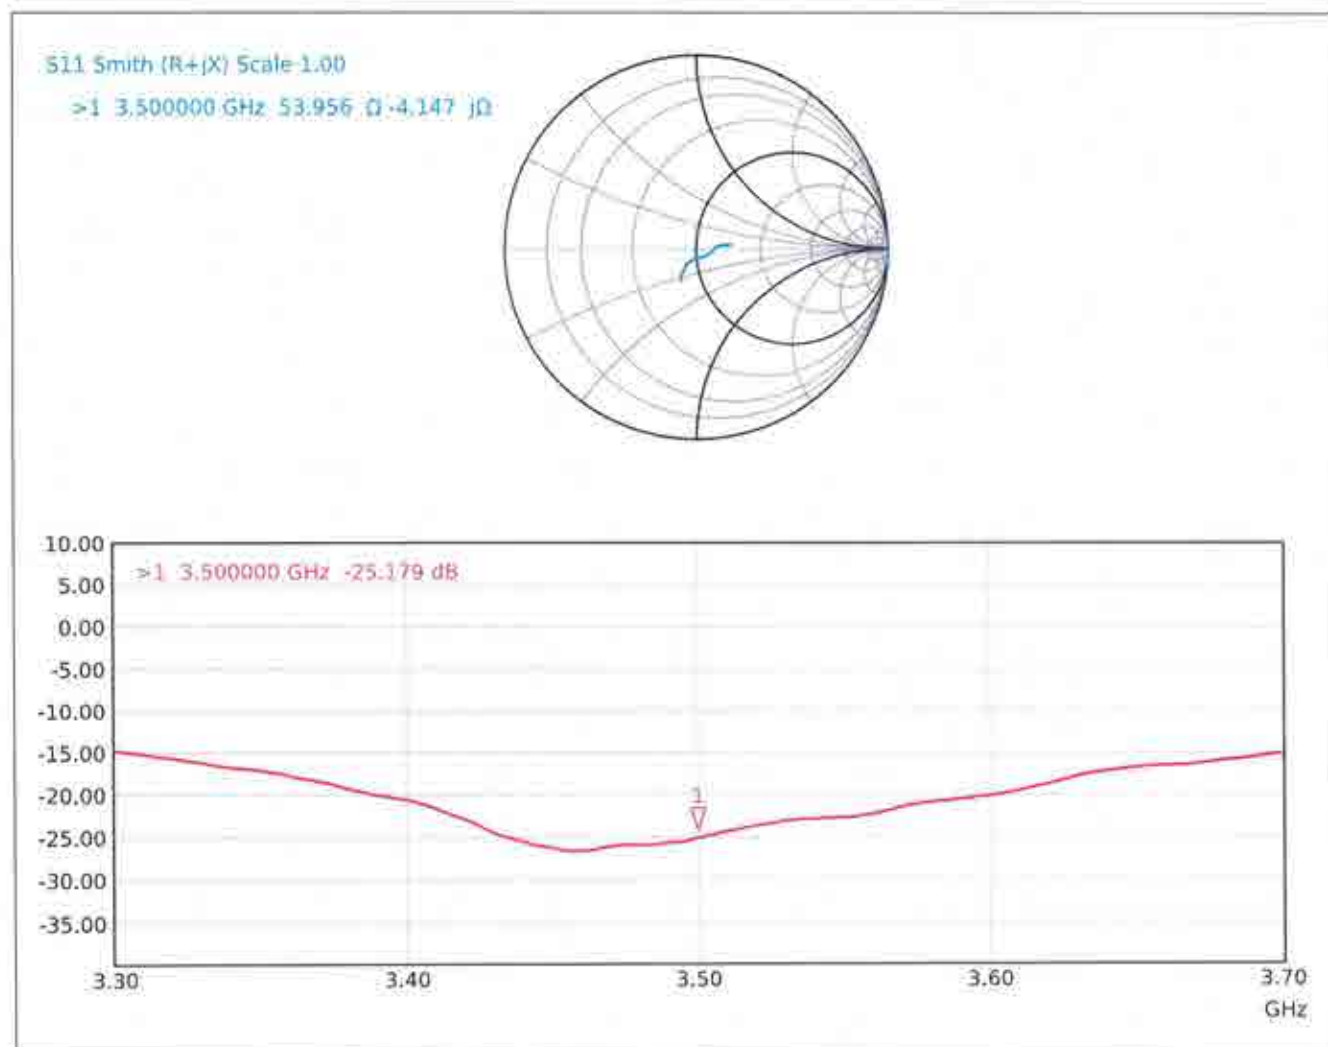

## D3500V2, serial no. 1014 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.



### <Justification of the extended calibration>

| D3500V2 – serial no. 1014   |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
| 3500MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 01.15.2025<br>(Cal. Report) | -25.2            |           | 54                   |             | -4.1                      |             |
| 01.14.2026<br>(extended)    | -25.713          | -1.99     | 56.234               | 2.234       | -4.4629                   | -0.3629     |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D3500 V2, serial no. 1014 (Data of Measurement : 01.14.2026)

3500MHz - Head

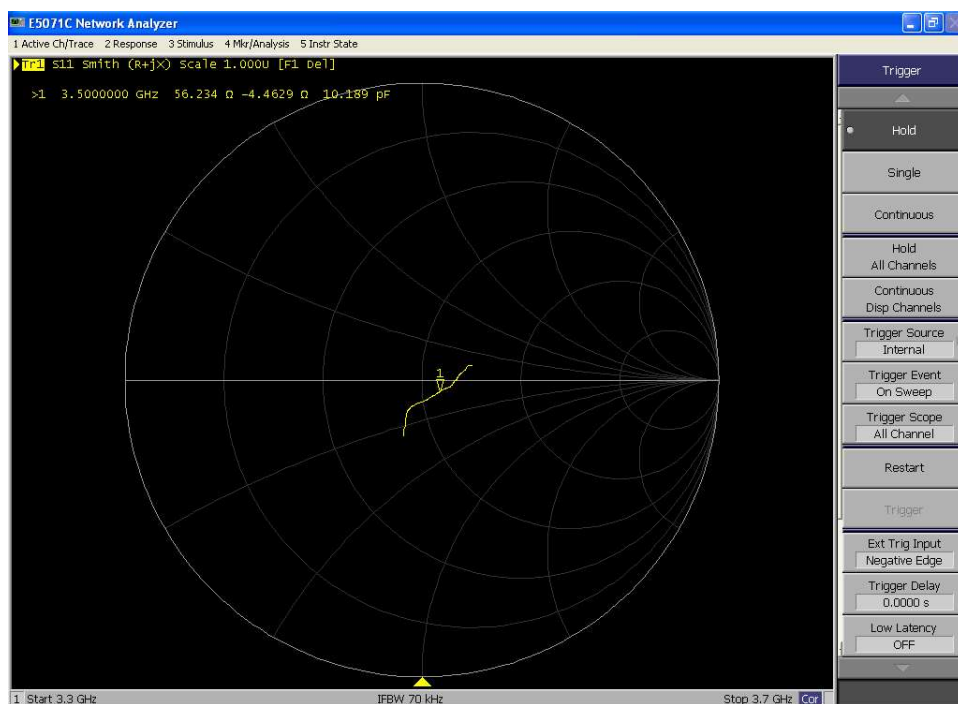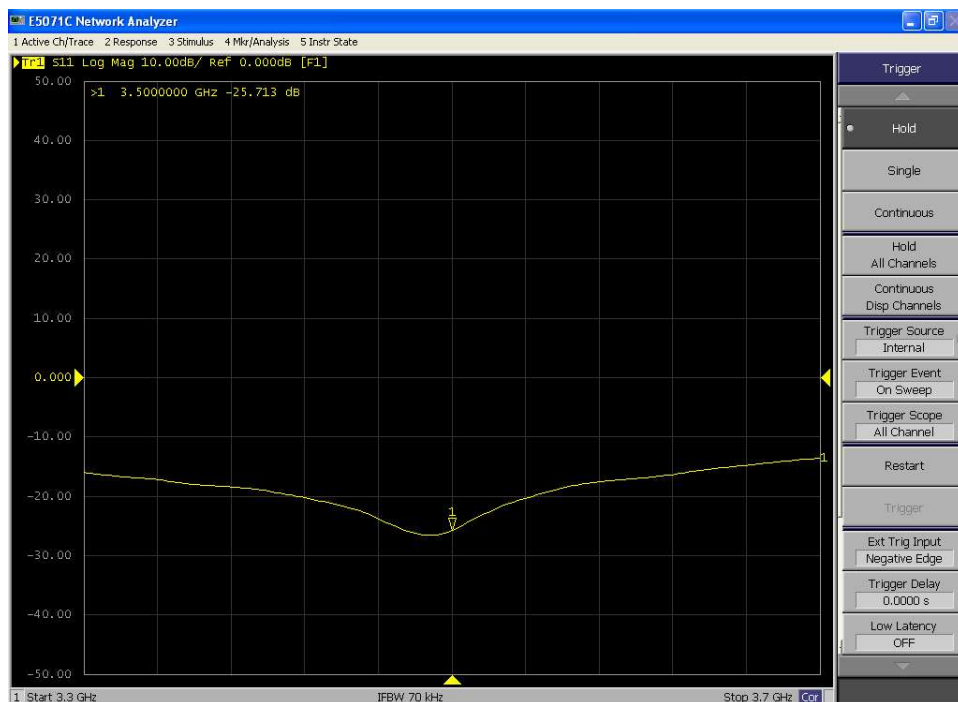



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
 Taoyuan City

Certificate No.

**D3700V2-1006\_Jun25**

## CALIBRATION CERTIFICATE

Object

**D3700V2 - SN: 1006**

Calibration procedure(s)

**QA CAL-22.v7**

**Calibration Procedure for SAR Validation Sources between 3 - 10 GHz**

Calibration date

**June 12, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|-----------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T    | SN: 100967 | 26-Mar-25 (No. 217-04290)              | Mar-26        |
| Power Sensor R&S NRP18A     | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40 | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| 3.5mm mismatch combination  | SN: 1152   | 24-Mar-25 (No. 217-04293)              | Mar-26        |
| OCP DAK-12                  | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                 | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                      | SN: 1836   | 17-Apr-25 (No. DAE4ip-1836_Apr25)      | Apr-26        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Setup 1                 | SN: 1000   | 27-May-25 (No. 675-ACAD_Source_Box-250527) | May-26          |
| Signal Generator R&S SMB100A | SN: 182081 | 27-May-25 (No. 675-CAL16-S4588-250527)     | May-26          |
| Mismatch: SMA                | SN: 1102   | 24-Apr-25 (No. 675-Mismatch_SMA-250424)    | Apr-26          |
| OCP DAK-12                   | SN: 1029   | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)       | Feb-26          |
| OCP DAK-3.5                  | SN: 1336   | 09-Dec-24 (No. OCP-DAK3.5-1336_Dec24)      | Dec-25          |

|               |            |                       |           |
|---------------|------------|-----------------------|-----------|
|               | Name       | Function              | Signature |
| Calibrated by | Paulo Pina | Laboratory Technician |           |
| Approved by   | Sven Kühn  | Technical Manager     |           |

Issued: June 12, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 10 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 5mm, dz = 1.4mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 3700MHz ±1MHz            |                                     |

HSL parameters at 3700 MHz

The following parameters and calculations were applied.

|                                    |               |              |                |
|------------------------------------|---------------|--------------|----------------|
|                                    | Temperature   | Permittivity | Conductivity   |
| Nominal HSL parameters             | 22.0 °C       | 37.7         | 3.12 mho/m     |
| Measured HSL parameters            | (22.0 ±0.2)°C | 38.8 ±6%     | 3.11 mho/m ±6% |
| HSL temperature change during test | < 0.5 °C      |              |                |

SAR result with HSL at 3700 MHz

|                                                  |                    |                          |
|--------------------------------------------------|--------------------|--------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of HSL | Condition          |                          |
| SAR for nominal HSL parameters                   | 20 dBm input power | 6.99 W/kg                |
| SAR for nominal HSL parameters                   | normalized to 1W   | 69.9 W/kg ±19.9% (k = 2) |

|                                                    |                    |                          |
|----------------------------------------------------|--------------------|--------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of HSL | Condition          |                          |
| SAR for nominal HSL parameters                     | 20 dBm input power | 2.56 W/kg                |
| SAR for nominal HSL parameters                     | normalized to 1W   | 25.6 W/kg ±19.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 3700 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 50.6 $\Omega$ – 7.8 j $\Omega$ |
| Return Loss | -22.2 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.137 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency (MHz) | TSL | Power (dBr) |
|------------------|-----------------|-----|-------------|
| D3700V2 - SN1006 | 3700            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance (mm) | Band | Group, UID | Frequency (MHz), Channel Number | Conversion Factor | TSL Conductivity (S/m) | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW   | 0---       | 3700, 6                         | 6.45              | 3.11                   | 38.8             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-06-12    | EX3DV4 - SN7349, 2025-01-10 | DAI4lp Sn1836, 2025-04-17 |

Scans Setup


|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents (mm)   | 28 x 28 x 28    |
| Grid Steps (mm)     | 5.0 x 5.0 x 1.4 |
| Sensor Surface (mm) | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-06-12          |
| psSAR1g (W/Kg)      | 6.99                |
| psSAR10g (W/Kg)     | 2.56                |
| Power Drift (dB)    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor (dB) |                     |
| TSL Correction      | Positive / Negative |

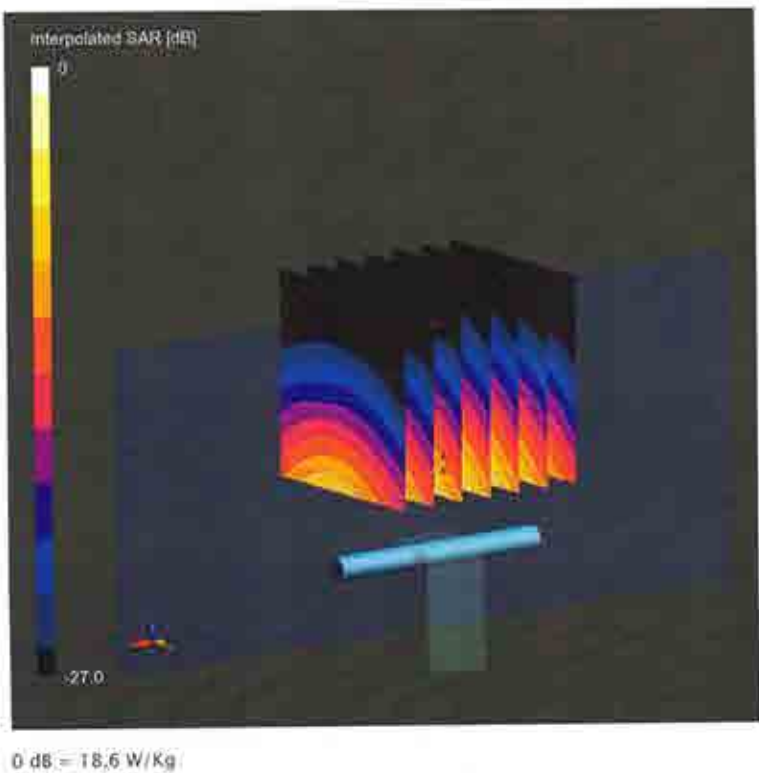

Impedance Measurement Plot for HSL

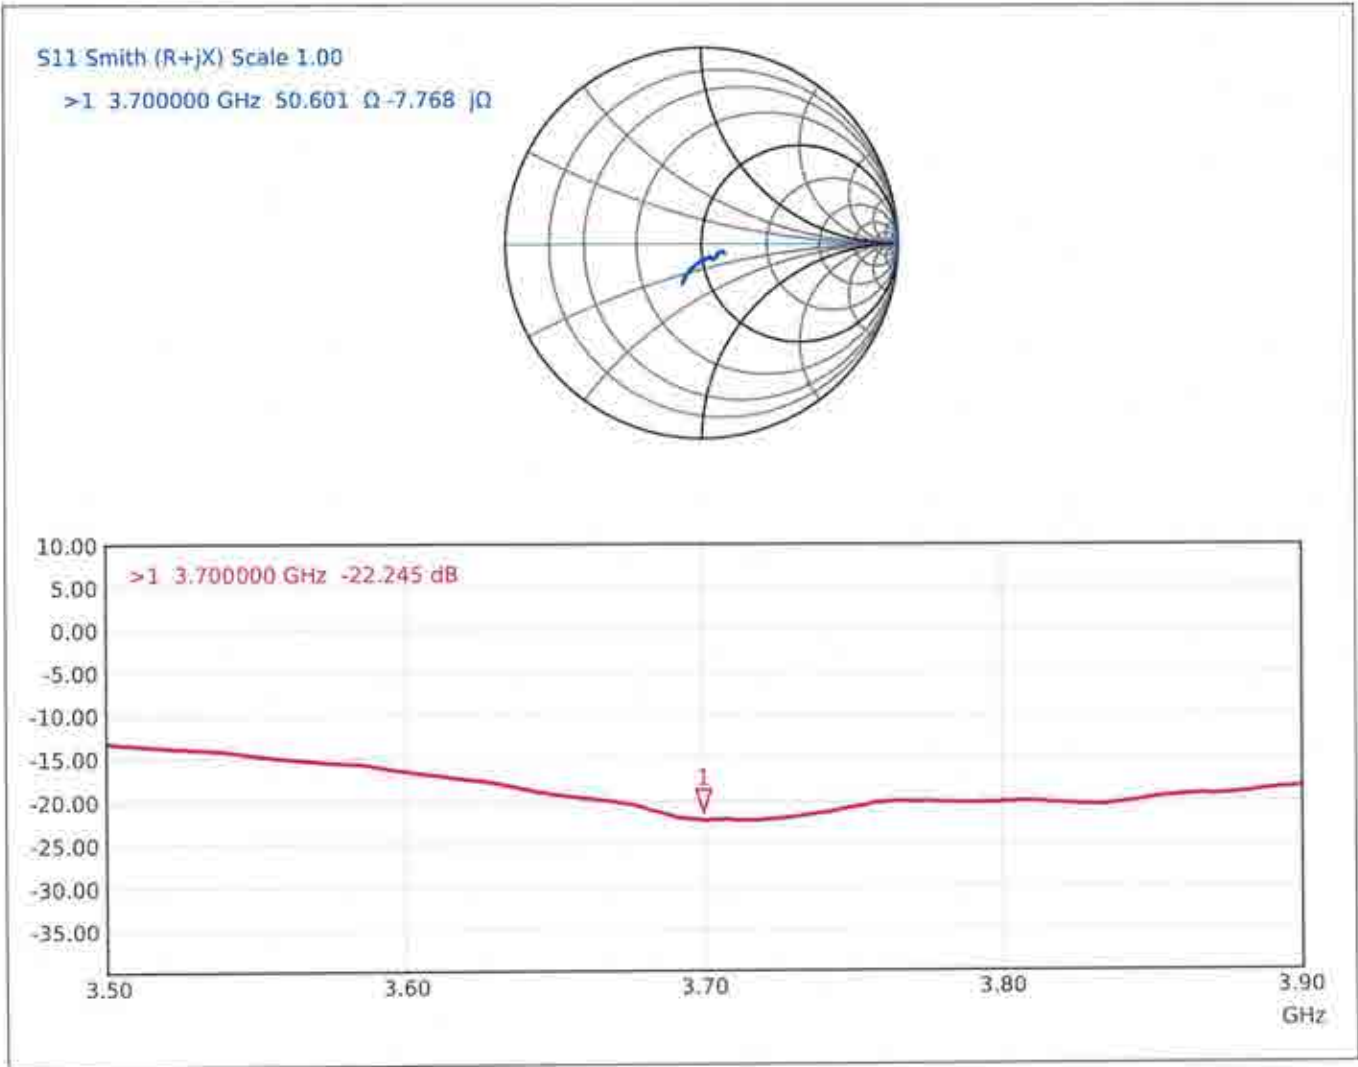



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Client **Sporton**  
**Taoyuan City**

Certificate No. **D3900V2-1092\_May23**

## CALIBRATION CERTIFICATE

Object **D3900V2 - SN:1092**

Calibration procedure(s) **QA CAL-22.v7**  
**Calibration Procedure for SAR Validation Sources between 3-10 GHz**

Calibration date: **May 15, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)      | Scheduled Calibration |
|-----------------------------|--------------------|---------------------------------|-----------------------|
| Power meter NRP2            | SN: 104778         | 30-Mar-23 (No. 217-03804/03805) | Mar-24                |
| Power sensor NRP-Z91        | SN: 103244         | 30-Mar-23 (No. 217-03804)       | Mar-24                |
| Power sensor NRP-Z91        | SN: 103245         | 30-Mar-23 (No. 217-03805)       | Mar-24                |
| Reference 20 dB Attenuator  | SN: BH9394 (20k)   | 30-Mar-23 (No. 217-03809)       | Mar-24                |
| Type-N mismatch combination | SN: 310982 / 06327 | 30-Mar-23 (No. 217-03810)       | Mar-24                |
| Reference Probe EX3DV4      | SN: 3503           | 07-Mar-23 (No. EX3-3503_Mar23)  | Mar-24                |
| DAE4                        | SN: 601            | 19-Dec-22 (No. DAE4-601_Dec22)  | Dec-23                |

| Secondary Standards             | ID #           | Check Date (in house)             | Scheduled Check        |
|---------------------------------|----------------|-----------------------------------|------------------------|
| Power meter E4419B              | SN: GB39512475 | 30-Oct-14 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: US37292783 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: MY41093315 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| RF generator R&S SMT-06         | SN: 100972     | 15-Jun-15 (in house check Oct-22) | In house check: Oct-24 |
| Network Analyzer Agilent E8358A | SN: US41080477 | 31-Mar-14 (in house check Oct-22) | In house check: Oct-24 |

Calibrated by: **Jeton Kastrati** Name: **Jeton Kastrati** Function: **Laboratory Technician**

Approved by: **Sven Kühn** Name: **Sven Kühn** Function: **Technical Manager**

Signature

Issued: May 17, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- DASY System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                                              |                                  |
|-------------------------------------|----------------------------------------------|----------------------------------|
| <b>DASY Version</b>                 | DASY52                                       | V52.10.4                         |
| <b>Extrapolation</b>                | Advanced Extrapolation                       |                                  |
| <b>Phantom</b>                      | Modular Flat Phantom V5.0                    |                                  |
| <b>Distance Dipole Center - TSL</b> | 10 mm                                        | with Spacer                      |
| <b>Zoom Scan Resolution</b>         | dx, dy = 4.0 mm, dz = 1.4 mm                 | Graded Ratio = 1.4 (Z direction) |
| <b>Frequency</b>                    | 3900 MHz $\pm$ 1 MHz<br>4100 MHz $\pm$ 1 MHz |                                  |

## Head TSL parameters at 3900 MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 37.5           | 3.32 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 37.0 $\pm$ 6 % | 3.23 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL at 3900 MHz

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                | 100 mW input power | 6.69 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>67.0 W/kg <math>\pm</math> 19.9 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
| SAR measured                                                  | 100 mW input power | 2.32 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>23.2 W/kg <math>\pm</math> 19.5 % (k=2)</b> |

## Head TSL parameters at 4100 MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 37.2           | 3.53 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 36.7 $\pm$ 6 % | 3.40 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL at 4100 MHz

|                                                             |                    |                                                |
|-------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                | 100 mW input power | 6.67 W/kg                                      |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>66.8 W/kg <math>\pm</math> 19.9 % (k=2)</b> |

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                                |
| SAR measured                                                  | 100 mW input power | 2.31 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>23.0 W/kg <math>\pm</math> 19.5 % (k=2)</b> |