



SAR
Dipole Performance Measurement
Report

EUT Type: SAR Validation Dipole and Waveguide

Model Name: DIP0G750,DIP0G835,DIP1G800,DIP1G900,DIP2G300,
DIP2G600

Brand Name: SATIMO

Test Conclusion: Pass

Test Date: 01 Jul . 2024 to 02 Jul. 2025

Date of Issue: 02 Jul. 2025

Testing Engineer :

Xin Liu

(Xin.Liu)

Technical Manager :

Shi fan-long

(Shifan. Long)

Authorized Signatory :

Bovey Yang

(Bovey Yang)





ISSUED BY
Shenzhen STS Test Services Co., Ltd.

Kind of Equipment	Manufacturer	Type No.	Serial No.	Last Calibration	Calibrated Until
PC	Acer	N/A	N/A	N/A	N/A
E-Field Probe	MVG	SSE2	SN 07/21 EPGO352	2024.02.14	2025.02.13
Dielectric Probe Kit	MVG	SCLMP	SN 32/14 OCPG67	2023.10.25	2024.10.24
Phantom1	MVG	SAM	SN 32/14 SAM115	N/A	N/A
Phantom3	MVG	SAM	SN 21/21 ELLI48	N/A	N/A
Attenuator	Agilent	99899	DC-18GHz	N/A	N/A
Directional coupler	Narda	4226-20	3305	N/A	N/A
Network Analyzer	Agilent	E5071C	MY46520378	2023-09-26	2024-09-25
Multi Meter	Keithley	Multi Meter 2000	4050073	2023-09-26	2024-09-25
Signal Generator	Agilent	ZHL-42W	9638	2023.10.07	2024.10.06
Power Amplifier	DESAY	NRP	100510	2023-09-26	2024-09-25
Power Meter	R&S	NRP-Z11	101919	2023-09-26	2024-09-25
Power Sensor	R&S	U2021XA	MY56280002	2023-09-26	2024-09-25
Temperature hygrometer	SuWei	SW-108	N/A	2023.09.28	2024.09.27
Thermograph	Elitech	RC-4	S/N EF7176501537	2023.10.12	2024.10.11



ISSUED BY
Shenzhen STS Test Services Co., Ltd.

Kind of Equipment	Manufacturer	Type No.	Serial No.	Last Calibration	Calibrated Until
PC	Acer	N/A	N/A	N/A	N/A
E-Field Probe	MVG	SSE2	SN 08/21 EPGO352	2024.09.18	2025.09.17
Dielectric Probe Kit	MVG	SCLMP	SN 32/14 OCPG67	2024.09.18	2025.09.17
Phantom1	MVG	SAM	SN 32/14 SAM115	N/A	N/A
Phantom2	MVG	SAM	SN 32/14 SAM116	N/A	N/A
Attenuator	Agilent	99899	DC-18GHz	N/A	N/A
Directional coupler	Narda	4226-20	3305	N/A	N/A
Network Analyzer	Agilent	E5071C	MY46520378	2024-09-25	2025-09-26
Multi Meter	Keithley	Multi Meter 2000	4050073	2024-09-25	2025-09-26
Signal Generator	Agilent	N5182A	MY50140530	2024-09-25	2025-09-26
Power Amplifier	DESAY	ZHL-42W	9638	2024-09-25	2025-09-26
Power Meter	R&S	NRP	100510	2024-09-25	2025-09-26
Power Sensor	R&S	NRP-Z11	101919	2024-09-25	2025-09-26
Power Sensor	Keysight	U2021XA	MY56280002	2024-09-25	2025-09-26
Temperature hygrometer	SuWei	SW-108	N/A	2024.10.15	2025.10.14
Thermograph	Elitech	RC-4	S/N EF7176501537	2024.10.15	2025.10.14



ISSUED BY
Shenzhen STS Test Services Co., Ltd.

Kind of Equipment	Manufacturer	Type No.	Serial No.	Last Calibration	Calibrated Until
SAR Test System	SATIMO	N/A	V5.3.15.11	N/A	N/A
Dielectric Probe Kit	MVG	SCLMP	SN 32/14 OCPG67	2025.09.15	2026.09.14
Antenna	MVG	ANTA3	SN 07/13 ZNTA52	N/A	N/A
Phantom1	MVG	SAM	SN 32/14 SAM115	N/A	N/A
Phantom3	MVG	SAM	SN 21/21 ELLI48	N/A	N/A
Phone holder	MVG	N/A	SN 32/14 MSH97	N/A	N/A
Laptop holder	MVG	N/A	SN 32/14 LSH29	N/A	N/A
Attenuator	Agilent	HXT-10-8-SMA	240327017	2025-02-22	2026-02-21
Directional coupler	Xi'an Xingbo	XBOH-OA08-20dB	211123-4-3	2025-02-22	2026-02-21
Network Analyzer	Agilent	E5071C	MY46520378	2025-09-26	2026-09-24
Multi Meter	Keithley	Multi Meter 2000	4050073	2025-09-22	2026-09-21
Signal Generator	Agilent	N5182A	MY50140530	2025-09-26	2026-09-25
Wireless Communication Test Set	Agilent	8960-E5515C	MY48360751	2025-02-22	2026-02-21
Wireless Communication Test Set	R&S	CMW500	156324	2025-09-25	2026-09-24
Power Amplifier	DESAY	WCS-DLNA50M8G50G1	CSKJLNA231227A	2025-09-29	2026-09-28
Power Meter	R&S	NRP	100510	2025-09-25	2026-09-24
Power Sensor	R&S	NRP-Z11	101919	2025-09-25	2026-09-24
Power Sensor	Keysight	U2021XA	MY56280002	2025-09-25	2026-09-24
Temperature hygrometer	TOPRIE	TP502V4-P	6700000124198	2025.10.09	2026.10.08
Thermograph	Elitech	RC-4	S/N EF7176501537	2025.10.17	2026.10.16



2. <Justification of the extended calibration>


Referring to KDB 865664 D01, if dipoles are verified in return loss < -20dB, (within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Head 750 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2023.07.04	-25.47	-	55.2	-
2024.07.01	-25.98	2.00	54.86	-0.34
2025.07.01	-25.49	0.08	55.49	0.029

The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Head 750 MHz

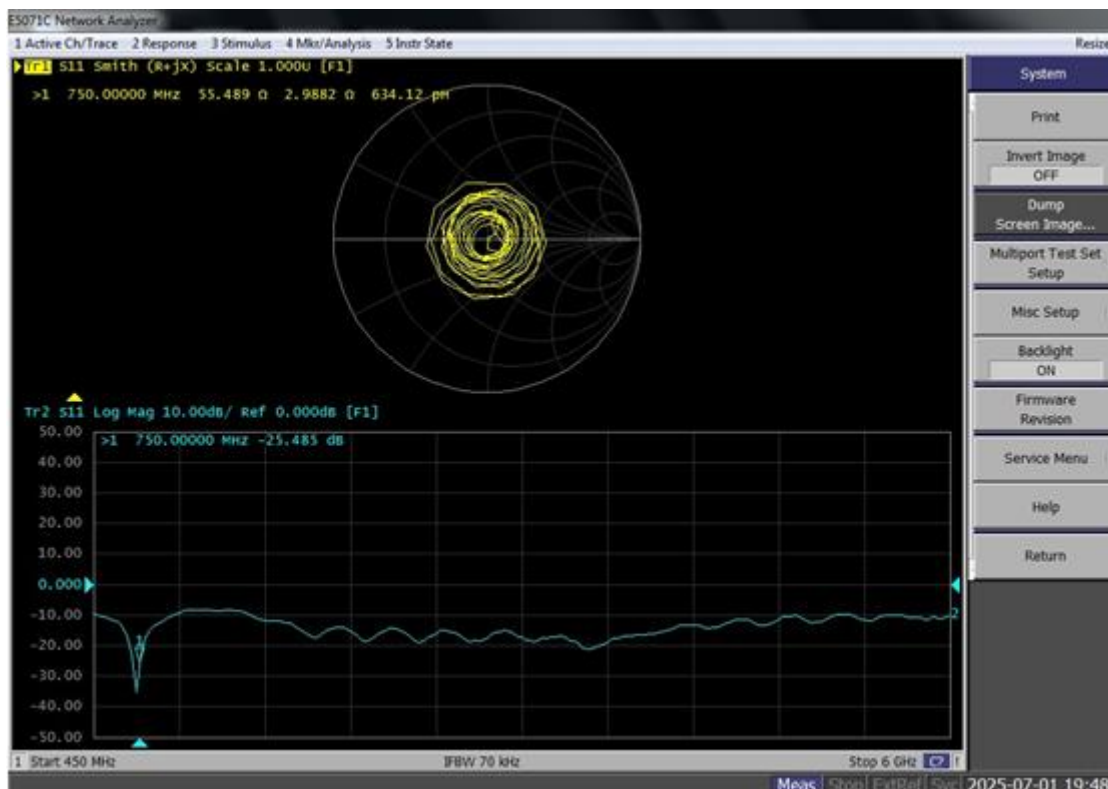




ISSUED BY
Shenzhen STS Test Services Co., Ltd.

Head 835 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2023.07.04	-28.13	-	51.4	-
2024.07.01	-28.43	1.07	52.62	1.22
2025.07.01	-27.70	-1.53	54.05	2.65

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Head 835MHz

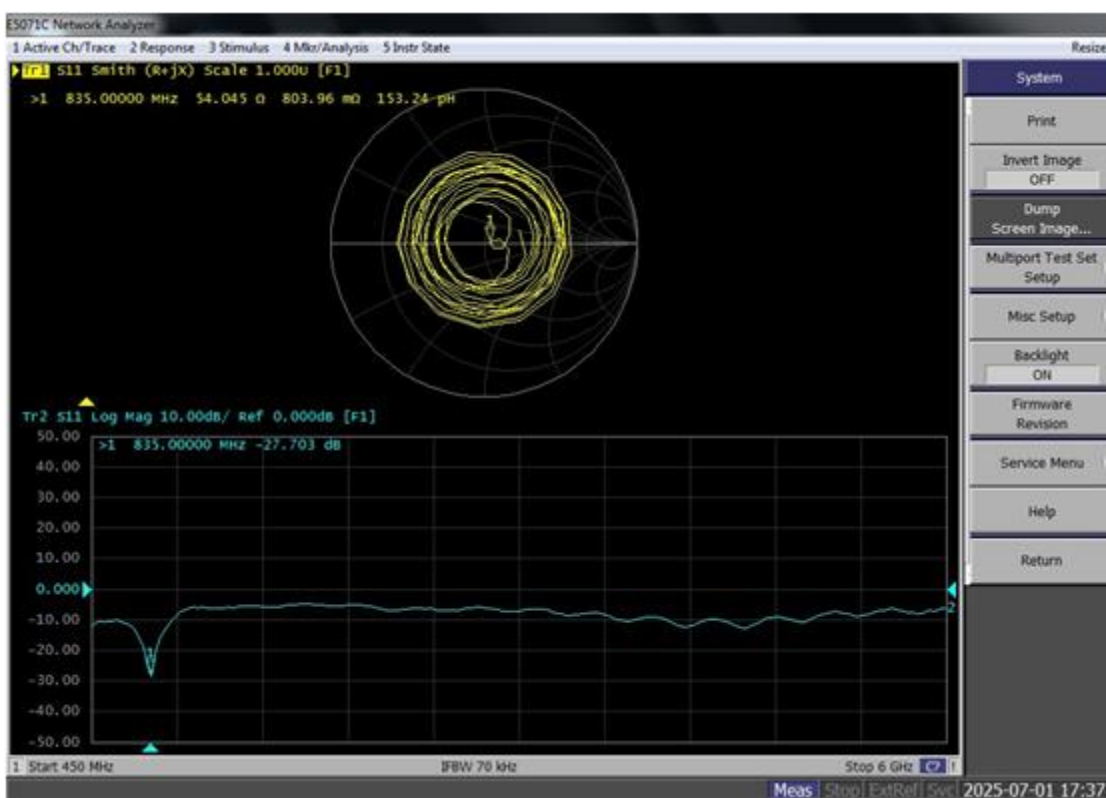




ISSUED BY
Shenzhen STS Test Services Co., Ltd.

Head 1800 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2023.12.20	-27.38	/	50.2	/
2024.07.01	-27.04	-1.23	48.48	-1.72
2025-07-01	-27.38	0	48.55	-1.65

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Head 1800 MHz

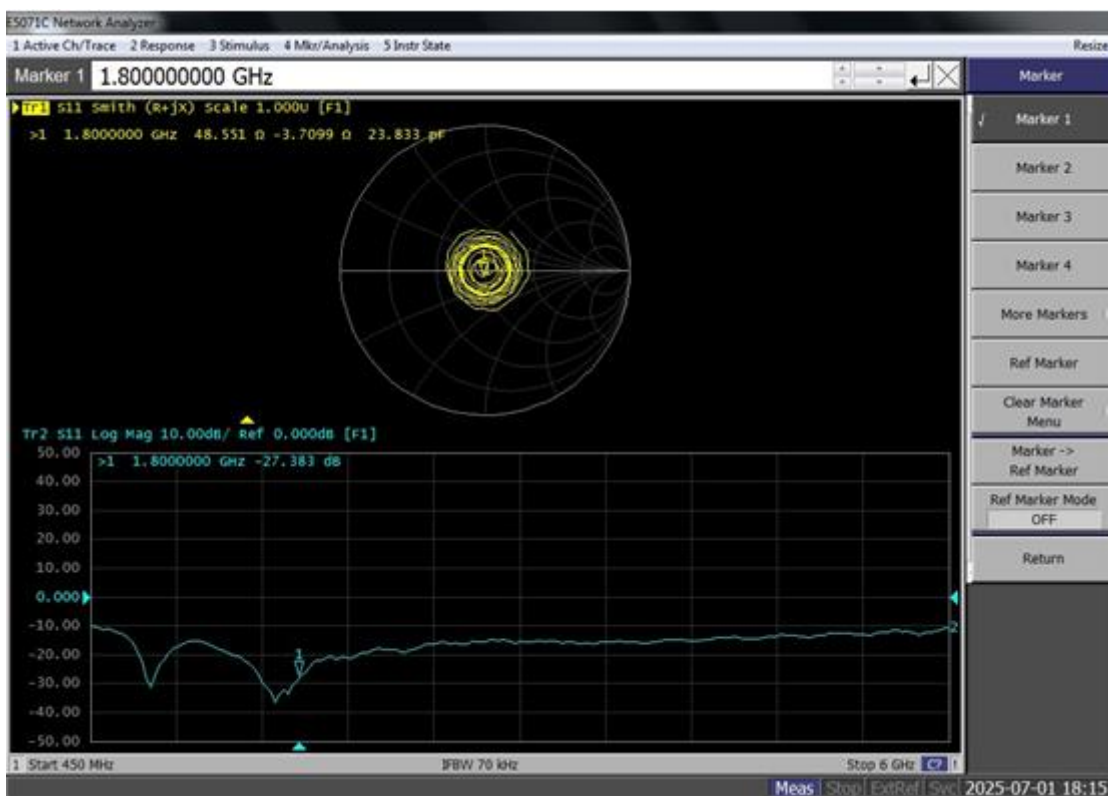




ISSUED BY
Shenzhen STS Test Services Co., Ltd.

Head 1900 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2023.09-14	-23.66	-	51.4	-
2024.07.01	-23.62	-0.17	50.73	-0.67
2025.07.02	-21.75	-8.07	47.01	-4.39

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Head 1900 MHz

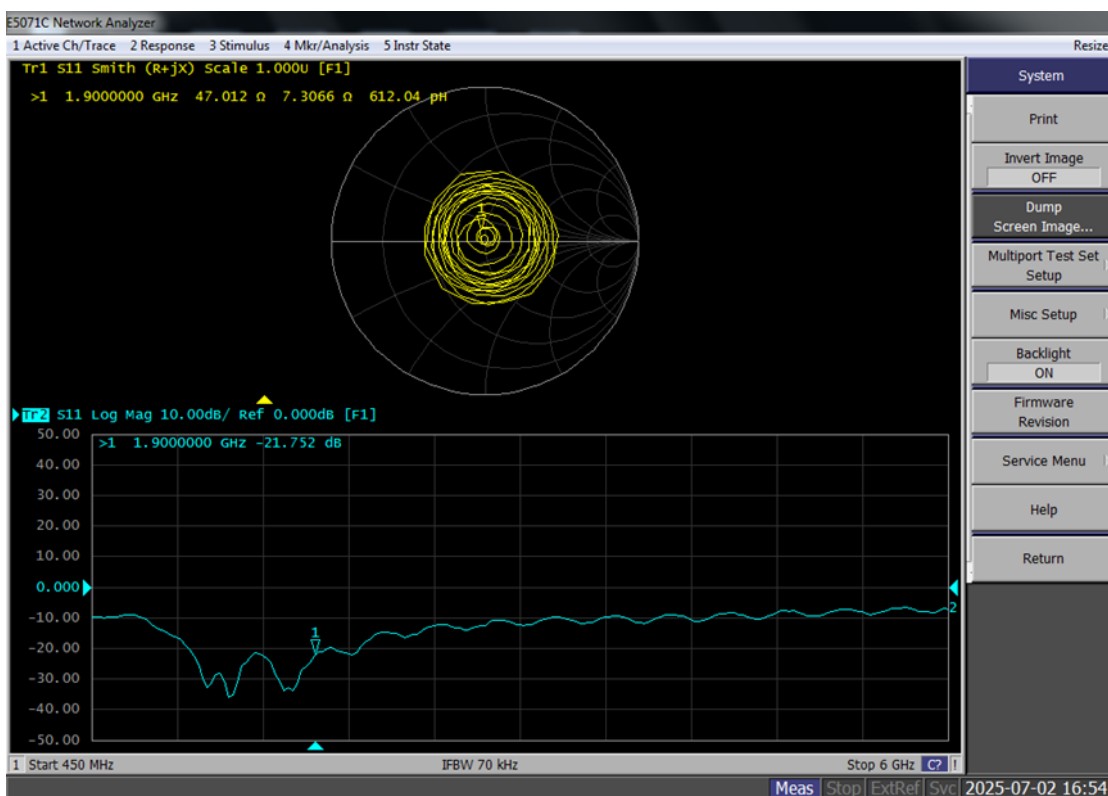




Head 2300 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2023.07.04	-25.73	-	53.2	-
2024.07.01	-25.12	-2.37	52.14	-1.06
2025.07.01	-25.47	-1.01	49.27	-3.93

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

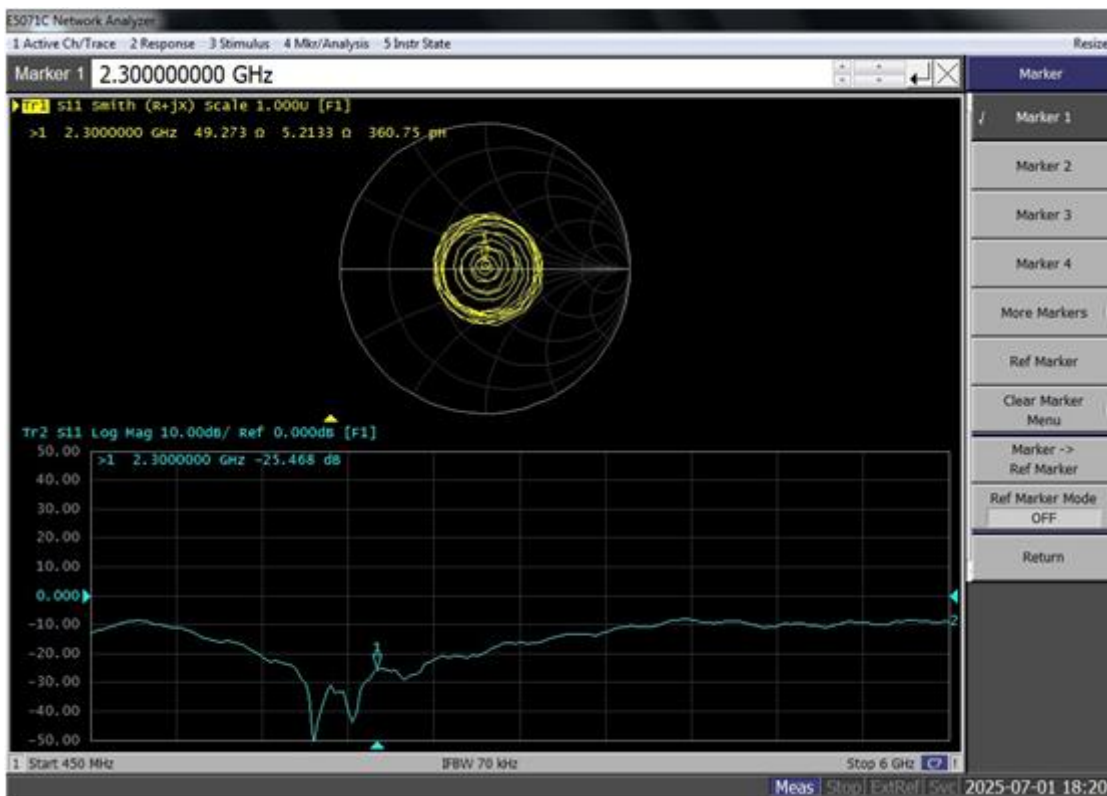



Head 2600 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2023.07.04	-34.32	-	50.3	-
2024.07.01	-33.58	-2.16	49.61	-0.69
2025.07.01	-32.91	-4.11	49.19	-1.11

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Head 2600 MHz

