

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200MHz

Impedance, transformed to feed point	56.0 Ω + 8.40j Ω
Return Loss	- 20.3dB

Antenna Parameters with Head TSL at 5400MHz

Impedance, transformed to feed point	49.8 Ω - 5.29j Ω
Return Loss	- 25.5dB

Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	57.0 Ω + 6.36j Ω
Return Loss	- 21.1dB

Antenna Parameters with Head TSL at 5800MHz

Impedance, transformed to feed point	52.3 Ω - 1.49j Ω
Return Loss	- 31.5dB

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	MVG
-----------------	-----

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

Date: 2025-10-23

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
SID5000 - SN: 02/21 DIP 5G000-543	5200	HSL	20

Exposure Conditions

Phantom	Position, Test	Band Group,	Frequency	Conversion	TSL Cond.	TSL
Section, TSL	Distance [mm]	UID	[MHz]	Factor	[S/m]	Permittivity
Flat	10	CW,	5200	5.37	4.63	35.8


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Right	HSL5G	EX3DV4 - SN7464, 2025-01-28	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	7.62
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.10
Sensor Surface [mm]	1.4	Power Drift [dB]	0.00
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.5	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	61.1
Scan Method	Measured	Dist 3dB Peak [mm]	6.8

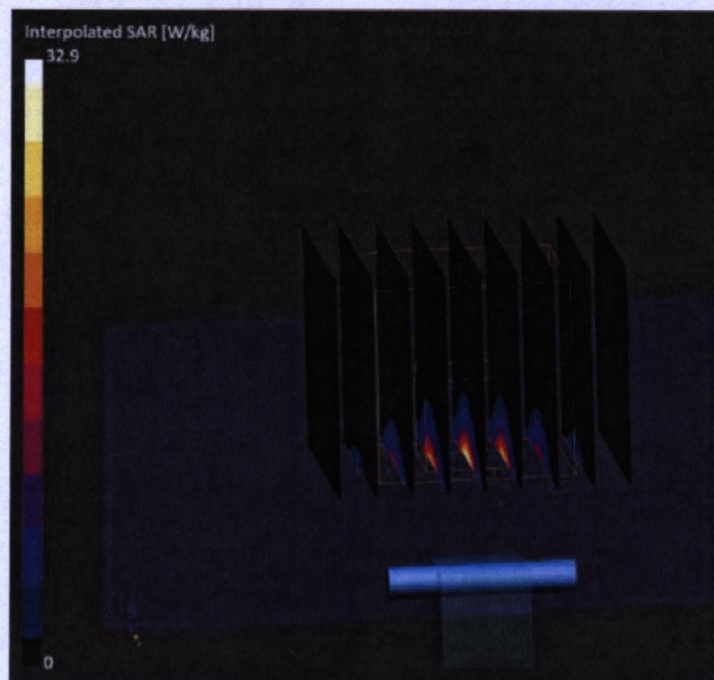

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2711
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

Date: 2025-10-23

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
SID5000 - SN: 02/21 DIP 5G000-543	5400	HSL	20

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat	10	CW,	5400	5.2	4.85	35.5


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Right	HSL5G	EX3DV4 - SN7464, 2025-01-28	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	7.98
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.21
Sensor Surface [mm]	1.4	Power Drift [dB]	0.00
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.5	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	59.3
Scan Method	Measured	Dist 3dB Peak [mm]	6.8

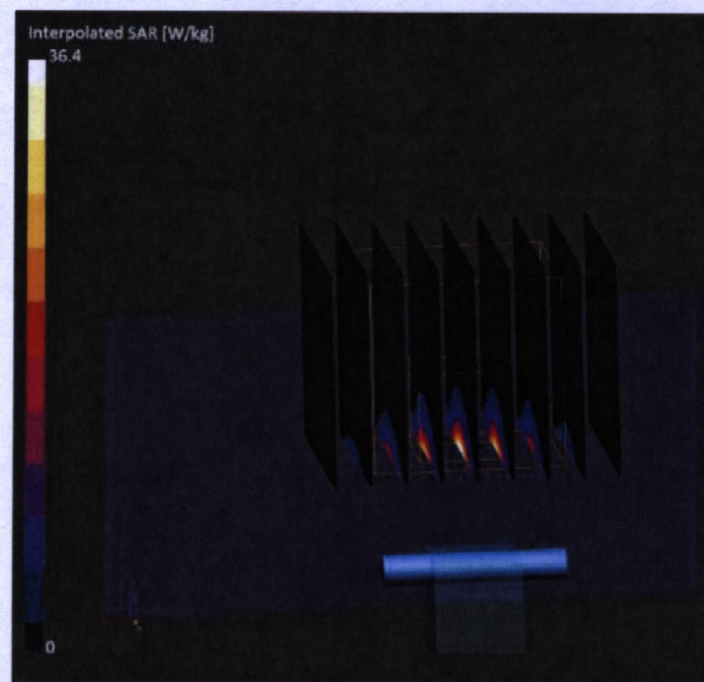

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2711
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL

Date: 2025-10-23

Test Laboratory: CTTL, Beijing, China

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
SID5000 - SN: 02/21 DIP 5G000-543	5600	HSL	20

Exposure Conditions

Phantom	Position, Test	Band Group,	Frequency	Conversion	TSL Cond.	TSL
Section, TSL	Distance [mm]	UID	[MHz]	Factor	[S/m]	Permittivity
Flat	10	CW,	5600	5.04	5.06	35.2


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Right	HSL5G	EX3DV4 - SN7464, 2025-01-28	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	7.90
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.19
Sensor Surface [mm]	1.4	Power Drift [dB]	0.01
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.5	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	57.5
Scan Method	Measured	Dist 3dB Peak [mm]	6.9

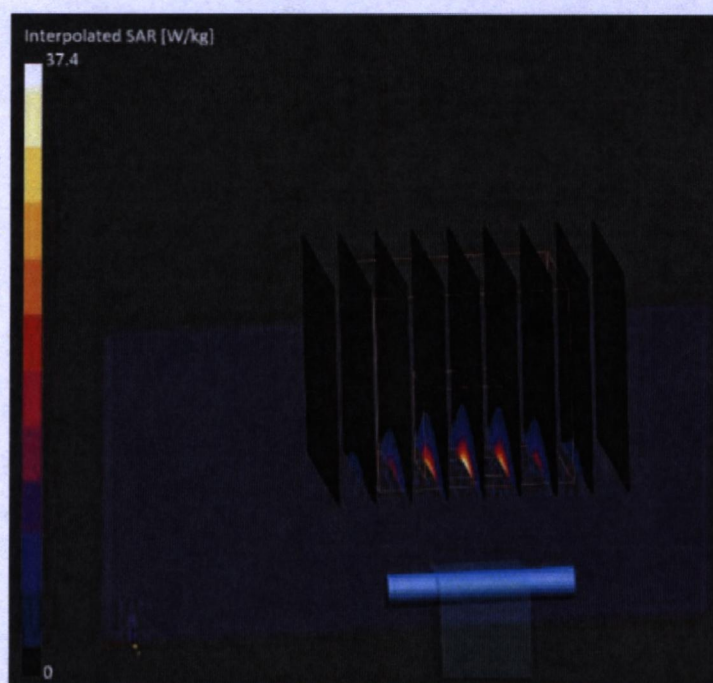

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL

Date: 2025-10-23

Test Laboratory: CTTL, Beijing, China

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
SID5000 - SN: 02/21 DIP 5G000-543	5800	HSL	20

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat	10	CW,	5800	4.91	5.28	34.8


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Right	HSL5G	EX3DV4 - SN7464, 2025-01-28	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	7.74
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.12
Sensor Surface [mm]	1.4	Power Drift [dB]	-0.02
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.5	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	55.4
Scan Method	Measured	Dist 3dB Peak [mm]	6.9

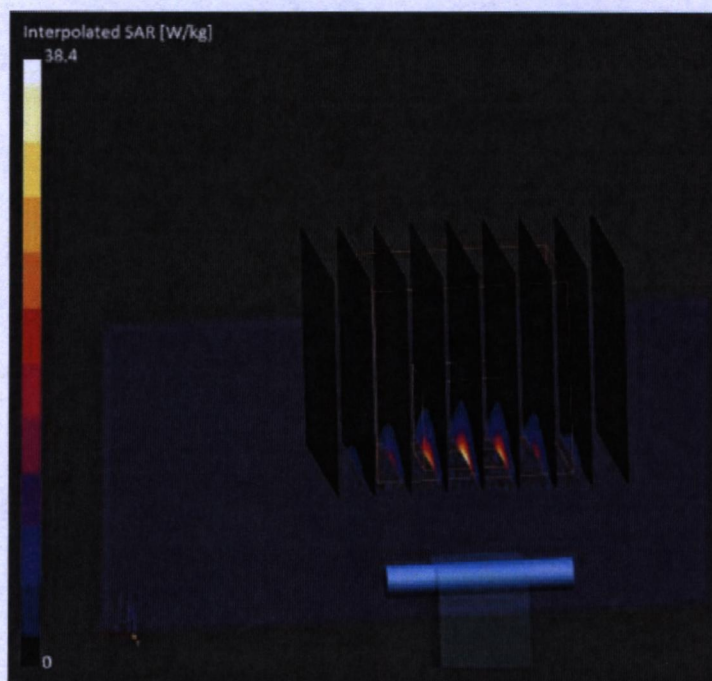

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2711
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Impedance Measurement Plot for Head TSL

